

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
 Data File : BP021560.D
 Acq On : 19 Aug 2024 19:37
 Operator : RC/JU
 Sample : P3518-25
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-13-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP021560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	25	rVB	2836089	3479352	30.67%	3.540%
2	3.546	91	95	104	rVB	169483	234230	2.06%	0.238%
3	4.940	326	332	339	rBV	299485	430824	3.80%	0.438%
4	5.399	403	410	420	rBV	4515530	6538846	57.64%	6.654%
5	6.969	668	677	687	rBV	4428510	7219782	63.64%	7.347%
6	7.404	745	751	757	rVB	105654	168091	1.48%	0.171%
7	7.804	810	819	826	rBV	1379605	2233134	19.68%	2.272%
8	8.951	1006	1014	1026	rBV	2511353	4564489	40.23%	4.645%
9	10.593	1286	1293	1301	rBV	1758707	3268555	28.81%	3.326%
10	11.340	1410	1420	1426	rBV	474991	807569	7.12%	0.822%
11	13.063	1707	1713	1720	rBV	6043850	8326310	73.39%	8.472%
12	14.169	1896	1901	1907	rBV	105709	178771	1.58%	0.182%
13	14.457	1944	1950	1957	rBV	3049291	4481634	39.50%	4.560%
14	14.669	1980	1986	1987	rBV	177470	240065	2.12%	0.244%
15	15.975	2201	2208	2216	rBV	5479963	7946261	70.04%	8.086%
16	16.463	2286	2291	2296	rBV5	64024	121923	1.07%	0.124%
17	17.257	2420	2426	2431	rBV	3466736	5361101	47.26%	5.455%
18	17.304	2431	2434	2439	rVB	429030	617674	5.44%	0.629%
19	17.386	2445	2448	2450	rBV2	92927	123903	1.09%	0.126%
20	17.410	2450	2452	2457	rVB	120364	152226	1.34%	0.155%
21	17.675	2493	2497	2502	rVB2	72621	116029	1.02%	0.118%
22	17.986	2545	2550	2560	rVB2	192414	327158	2.88%	0.333%
23	18.086	2561	2567	2570	rBV7	73076	162458	1.43%	0.165%
24	18.169	2574	2581	2584	rBV4	136297	286672	2.53%	0.292%
25	18.216	2584	2589	2597	rBV	2038373	3017290	26.60%	3.070%
26	18.374	2612	2616	2619	rBV2	133218	249051	2.20%	0.253%
27	18.410	2620	2622	2630	rVB	206051	355536	3.13%	0.362%
28	18.522	2638	2641	2645	rVB3	169233	208790	1.84%	0.212%
29	19.269	2763	2768	2771	rBV3	195676	319623	2.82%	0.325%
30	19.386	2783	2788	2797	rBV	1368101	2262399	19.94%	2.302%
31	19.539	2810	2814	2826	rBV2	1112132	1625901	14.33%	1.654%
32	19.769	2844	2853	2857	rBV	1331870	2190760	19.31%	2.229%
33	19.980	2884	2889	2898	rVB	9019389	11344631	100.00%	11.544%
34	20.663	3002	3005	3009	rVB3	399928	531111	4.68%	0.540%
35	21.398	3125	3130	3142	rVB3	956229	2090382	18.43%	2.127%
36	21.657	3171	3174	3178	rBV	413636	507233	4.47%	0.516%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021560.D
Acq On : 19 Aug 2024 19:37
Operator : RC/JU
Sample : P3518-25
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-13-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.727	3178	3186	3191	rVV2	3900099	6560468	57.83%	6.676%
38	21.768	3191	3193	3198	rVB	500426	692888	6.11%	0.705%
39	22.692	3346	3350	3363	rVB5	593981	1621023	14.29%	1.649%
40	24.351	3627	3632	3647	rVB2	801981	2044109	18.02%	2.080%
41	25.156	3763	3769	3781	rVB	1752081	5266692	46.42%	5.359%




Sum of corrected areas: 98274944

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021560.D
Acq On : 19 Aug 2024 19:37
Operator : RC/JU
Sample : P3518-25
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-13-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

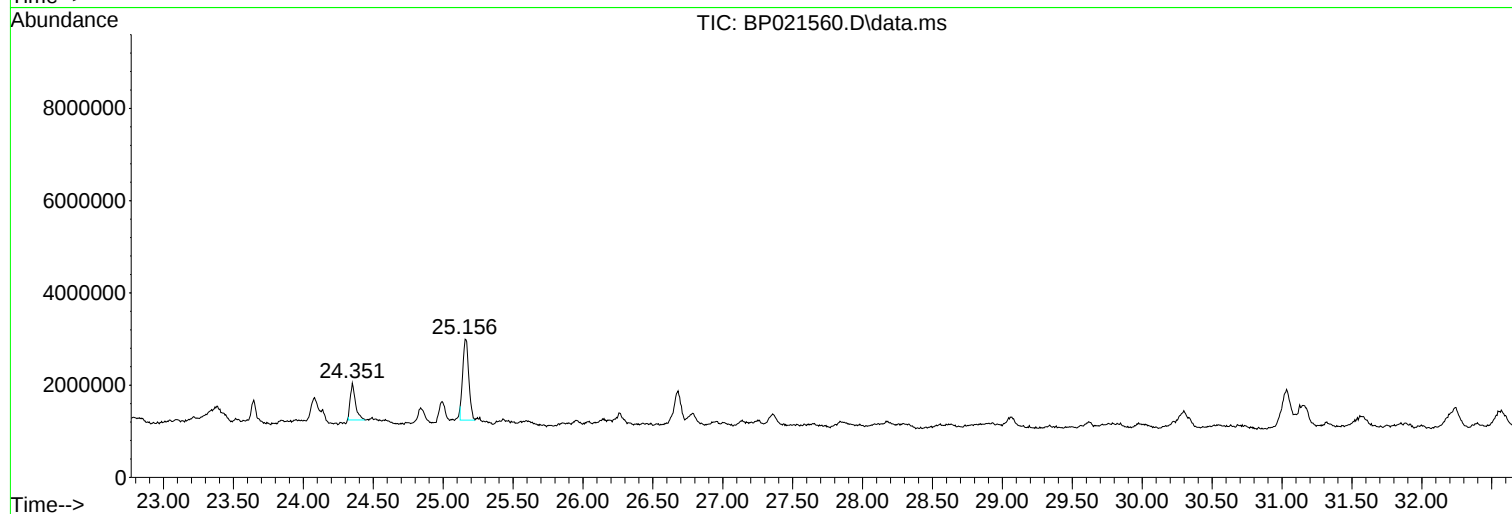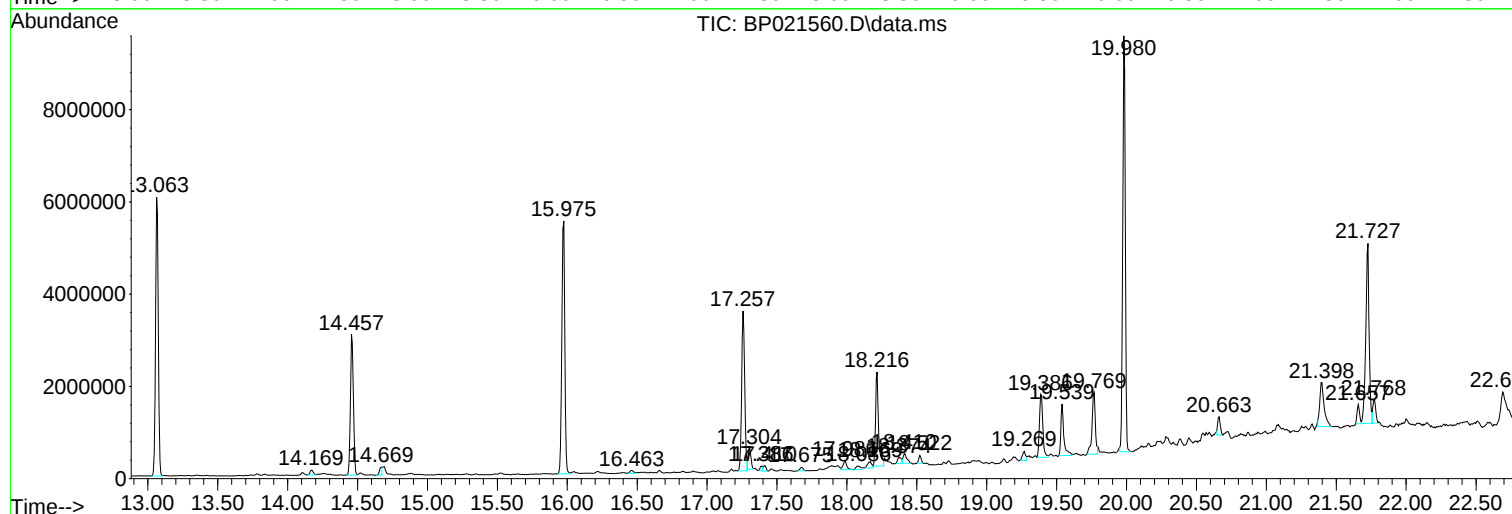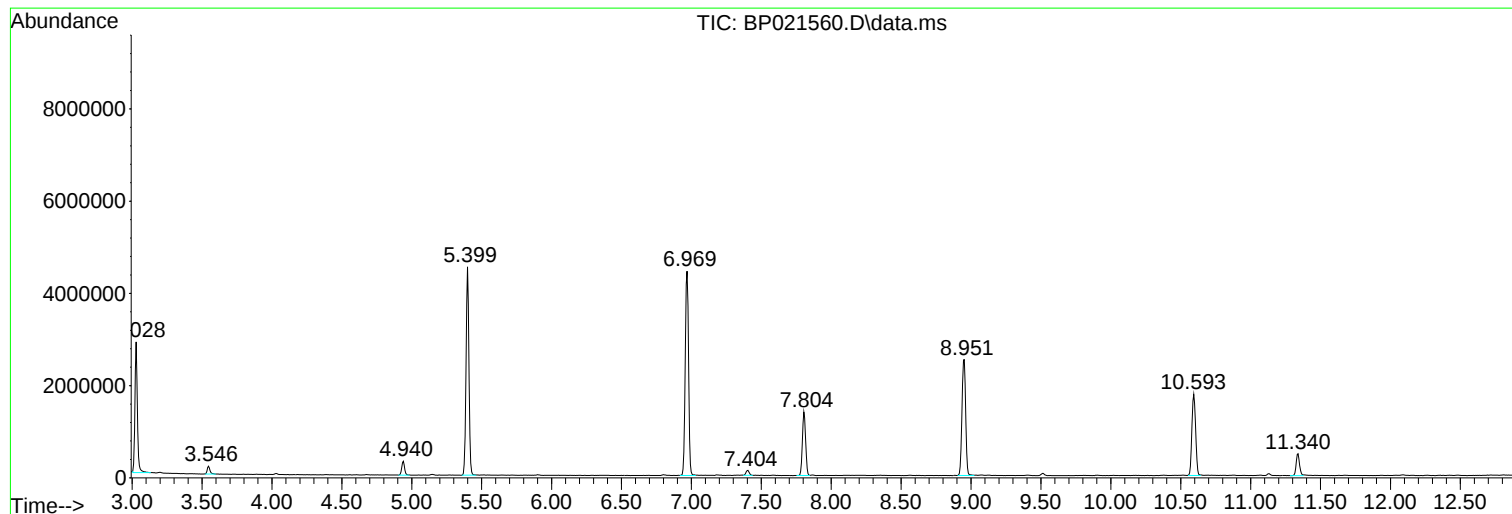

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021560.D
Acq On : 19 Aug 2024 19:37
Operator : RC/JU
Sample : P3518-25
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-13-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021560.D
Acq On : 19 Aug 2024 19:37
Operator : RC/JU
Sample : P3518-25
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-13-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------