

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
 Data File : BP021562.D
 Acq On : 19 Aug 2024 21:03
 Operator : RC/JU
 Sample : P3518-29
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-15-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP021562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	26	rVB	3176801	3878814	34.65%	3.357%
2	3.546	91	95	105	rBV	200634	280935	2.51%	0.243%
3	4.940	325	332	340	rVB	273970	389360	3.48%	0.337%
4	5.405	403	411	418	rBV	4654045	7104807	63.47%	6.149%
5	6.975	669	678	686	rBV	4725637	7669788	68.51%	6.638%
6	7.804	813	819	827	rBV	1423541	2371982	21.19%	2.053%
7	8.951	1005	1014	1022	rBV	2854677	4884307	43.63%	4.227%
8	10.593	1285	1293	1301	rBV	2021184	3465066	30.95%	2.999%
9	11.334	1410	1419	1426	rBV	247972	433965	3.88%	0.376%
10	13.069	1706	1714	1723	rVB	4799445	8054166	71.95%	6.970%
11	13.781	1830	1835	1840	rBV3	71384	120983	1.08%	0.105%
12	14.169	1896	1901	1908	rVV	133647	230330	2.06%	0.199%
13	14.451	1942	1949	1955	rBV	3107884	4727140	42.23%	4.091%
14	14.516	1956	1960	1970	rVB5	63796	155060	1.39%	0.134%
15	14.669	1980	1986	1987	rBV2	132129	174332	1.56%	0.151%
16	15.963	2199	2206	2215	rBV	5330408	8519105	76.10%	7.373%
17	16.210	2243	2248	2252	rBV3	105941	182285	1.63%	0.158%
18	16.451	2285	2289	2293	rVB	103486	136493	1.22%	0.118%
19	17.257	2419	2426	2430	rBV	3478630	5754545	51.41%	4.980%
20	17.298	2430	2433	2441	rVV	945511	1390103	12.42%	1.203%
21	17.380	2441	2447	2454	rVB2	272841	624130	5.58%	0.540%
22	17.663	2492	2495	2500	rVB	95370	134471	1.20%	0.116%
23	17.927	2537	2540	2543	rBV3	111330	144924	1.29%	0.125%
24	18.157	2573	2579	2582	rBV3	196137	379113	3.39%	0.328%
25	18.204	2582	2587	2595	rVV2	1316843	2103997	18.80%	1.821%
26	18.363	2611	2614	2618	rVB2	269489	319204	2.85%	0.276%
27	18.516	2636	2640	2645	rVB5	350518	513066	4.58%	0.444%
28	19.263	2763	2767	2770	rBV3	257548	376812	3.37%	0.326%
29	19.380	2782	2787	2793	rBV	2419515	3554110	31.75%	3.076%
30	19.533	2809	2813	2818	rBV2	609475	953685	8.52%	0.825%
31	19.727	2842	2846	2847	rBV	312614	385377	3.44%	0.334%
32	19.757	2847	2851	2859	rVB	2110209	2931091	26.18%	2.537%
33	19.980	2884	2889	2899	rVB	9238406	11194445	100.00%	9.688%
34	20.598	2989	2994	2998	rBV3	292923	662391	5.92%	0.573%
35	20.663	3002	3005	3010	rVB3	761223	974829	8.71%	0.844%
36	21.392	3125	3129	3142	rVB4	1222438	2289105	20.45%	1.981%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021562.D
Acq On : 19 Aug 2024 21:03
Operator : RC/JU
Sample : P3518-29
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-15-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.721	3178	3185	3190	rBV3	3787565	7388258	66.00%	6.394%
38	21.768	3191	3193	3199	rVB	759713	953963	8.52%	0.826%
39	22.680	3343	3348	3353	rBV2	770874	1703260	15.22%	1.474%
40	24.345	3624	3631	3647	rVB3	1992218	5228973	46.71%	4.525%
41	25.162	3762	3770	3779	rVB	2019634	5544356	49.53%	4.798%
42	26.674	4019	4027	4038	rVB	1593211	4827671	43.13%	4.178%
43	32.221	4962	4970	4971	rBV	1220130	2441098	21.81%	2.113%




Sum of corrected areas: 115551895

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021562.D
Acq On : 19 Aug 2024 21:03
Operator : RC/JU
Sample : P3518-29
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-15-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

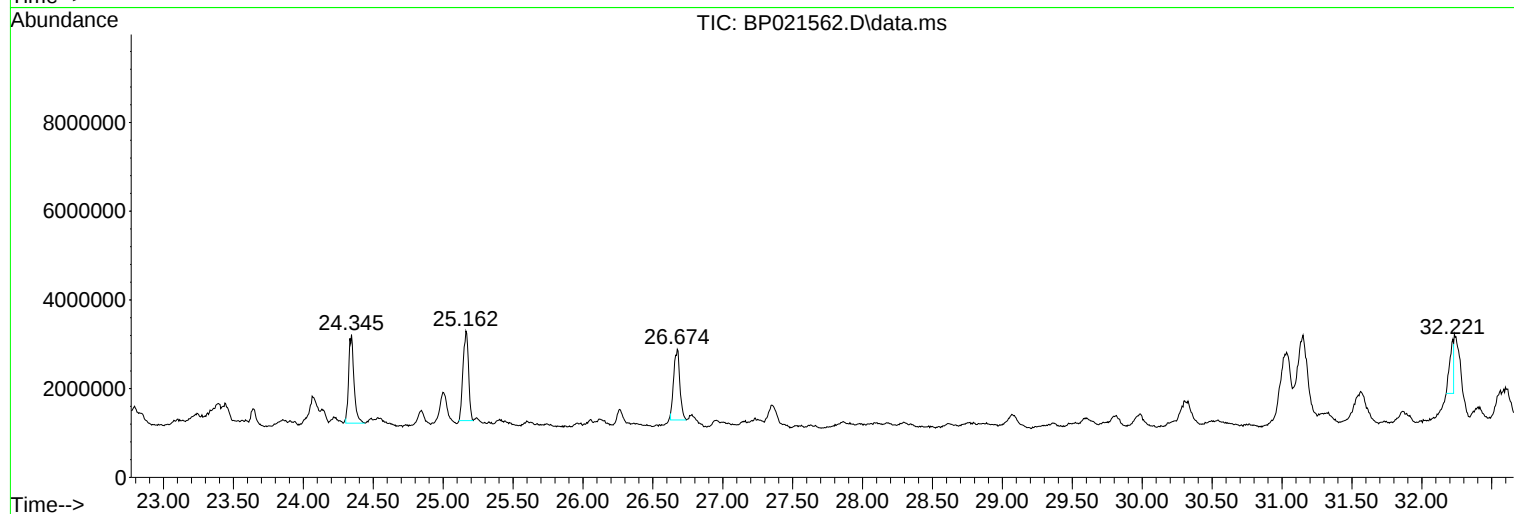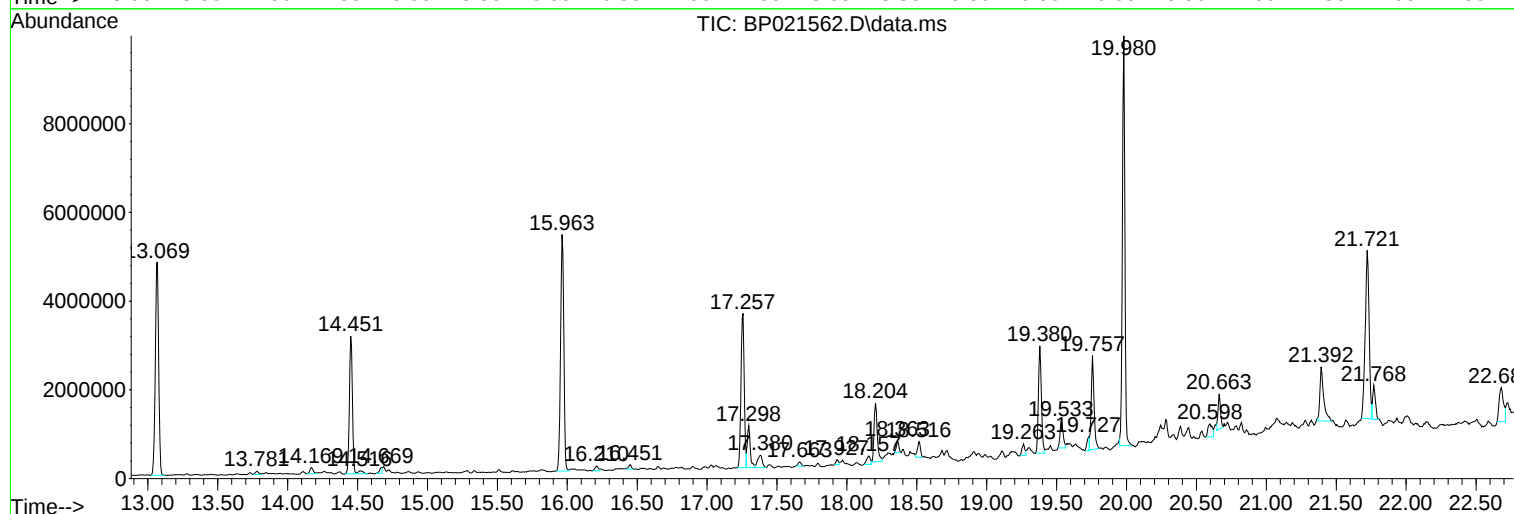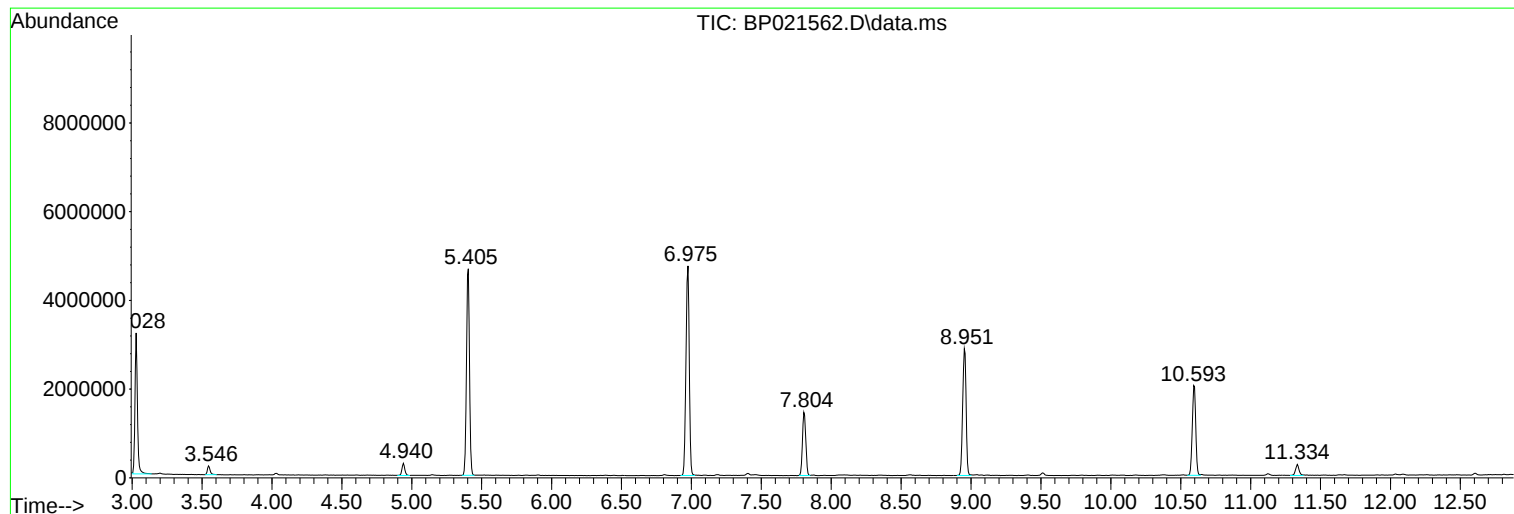

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021562.D
Acq On : 19 Aug 2024 21:03
Operator : RC/JU
Sample : P3518-29
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-15-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021562.D
Acq On : 19 Aug 2024 21:03
Operator : RC/JU
Sample : P3518-29
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-15-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------