

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
 Data File : BP021563.D
 Acq On : 19 Aug 2024 21:47
 Operator : RC/JU
 Sample : P3518-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-10-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP021563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	21	rVB	3276216	4067600	33.09%	3.366%
2	3.546	91	95	104	rBV	440881	601927	4.90%	0.498%
3	4.940	327	332	339	rVB	307457	439845	3.58%	0.364%
4	5.404	403	411	419	rBV	5381473	8142552	66.25%	6.738%
5	6.975	670	678	688	rBV	5367705	8787503	71.50%	7.272%
6	7.404	746	751	758	rVB	232967	341121	2.78%	0.282%
7	7.810	811	820	827	rBV	1572530	2486666	20.23%	2.058%
8	8.957	1003	1015	1027	rBV	3189191	5507760	44.81%	4.558%
9	10.598	1284	1294	1301	rBV	2055715	3594524	29.25%	2.975%
10	11.334	1411	1419	1426	rBV	584092	1106455	9.00%	0.916%
11	13.063	1705	1713	1724	rBV	5911837	9193116	74.80%	7.608%
12	14.110	1886	1891	1896	rBV3	75521	143265	1.17%	0.119%
13	14.175	1896	1902	1908	rVV	199022	296514	2.41%	0.245%
14	14.451	1942	1949	1956	rBV	3124453	4763756	38.76%	3.942%
15	14.522	1956	1961	1969	rVB	119135	224794	1.83%	0.186%
16	14.675	1979	1987	1988	rBV	662142	961488	7.82%	0.796%
17	15.975	2200	2208	2216	rBV	5512257	8971583	72.99%	7.424%
18	16.045	2216	2220	2228	rVB6	67584	144619	1.18%	0.120%
19	16.904	2363	2366	2376	rVB	70381	133802	1.09%	0.111%
20	17.263	2421	2427	2432	rBV	3538920	5599338	45.56%	4.634%
21	17.310	2432	2435	2440	rVB	1460983	2113568	17.20%	1.749%
22	17.398	2446	2450	2458	rVB	188547	362378	2.95%	0.300%
23	17.680	2490	2498	2504	rBV2	132196	297696	2.42%	0.246%
24	17.810	2516	2520	2523	rBV3	78877	134753	1.10%	0.112%
25	17.992	2547	2551	2558	rVB	209563	332323	2.70%	0.275%
26	18.092	2565	2568	2573	rBV6	88747	161147	1.31%	0.133%
27	18.174	2579	2582	2585	rVB	128363	148356	1.21%	0.123%
28	18.216	2585	2589	2594	rBV2	1119828	1692048	13.77%	1.400%
29	18.380	2612	2617	2620	rBV2	326280	710561	5.78%	0.588%
30	18.433	2620	2626	2634	rVV3	992254	2478704	20.17%	2.051%
31	18.627	2657	2659	2666	rVB6	120380	226805	1.85%	0.188%
32	18.692	2667	2670	2673	rBV	153594	199766	1.63%	0.165%
33	18.733	2673	2677	2681	rVV	1209328	1552985	12.64%	1.285%
34	19.257	2762	2766	2772	rBV2	209006	390155	3.17%	0.323%
35	19.398	2785	2790	2795	rBV	3955720	5679035	46.21%	4.700%
36	19.504	2804	2808	2809	rBV4	210399	237573	1.93%	0.197%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021563.D
Acq On : 19 Aug 2024 21:47
Operator : RC/JU
Sample : P3518-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-10-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.527	2809	2812	2817	rVB4	514928	874464	7.11%	0.724%
38	19.739	2844	2848	2850	rBV2	558032	869925	7.08%	0.720%
39	19.768	2850	2853	2859	rVB	3103216	3949927	32.14%	3.269%
40	19.986	2885	2890	2899	rVB	8743823	12290919	100.00%	10.171%
41	20.221	2925	2930	2936	rBV5	401556	951621	7.74%	0.788%
42	21.392	3125	3129	3150	rVB6	1281603	3409559	27.74%	2.822%
43	21.721	3178	3185	3190	rBV3	3526334	6399970	52.07%	5.296%
44	21.768	3190	3193	3198	rVB	763926	1138626	9.26%	0.942%
45	22.698	3345	3351	3353	rBV3	600689	1227129	9.98%	1.016%
46	24.345	3626	3631	3641	rVB2	702515	1777080	14.46%	1.471%
47	25.162	3762	3770	3781	rVB	2014732	5724512	46.58%	4.737%




Sum of corrected areas: 120839813

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021563.D
Acq On : 19 Aug 2024 21:47
Operator : RC/JU
Sample : P3518-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-10-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

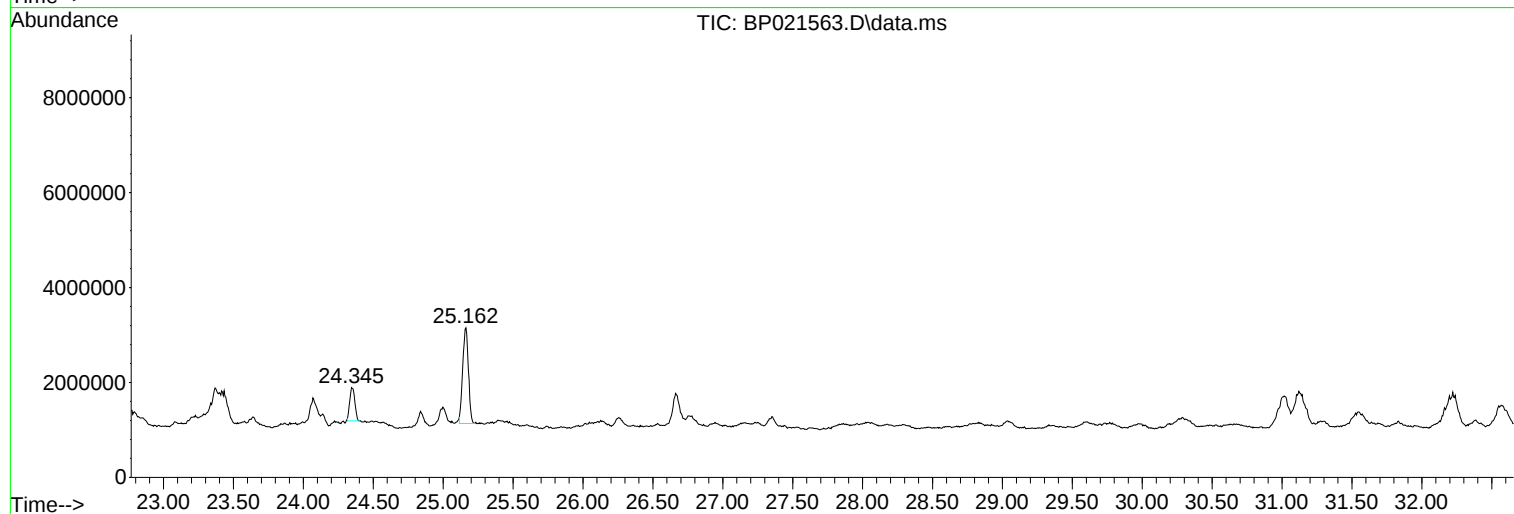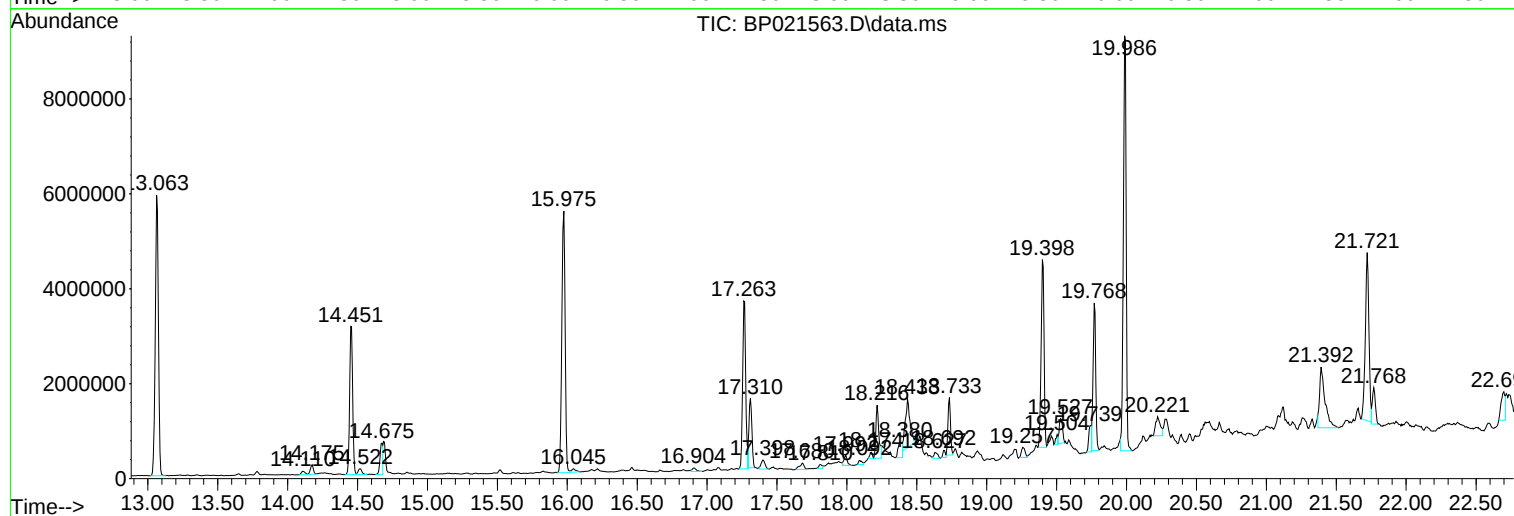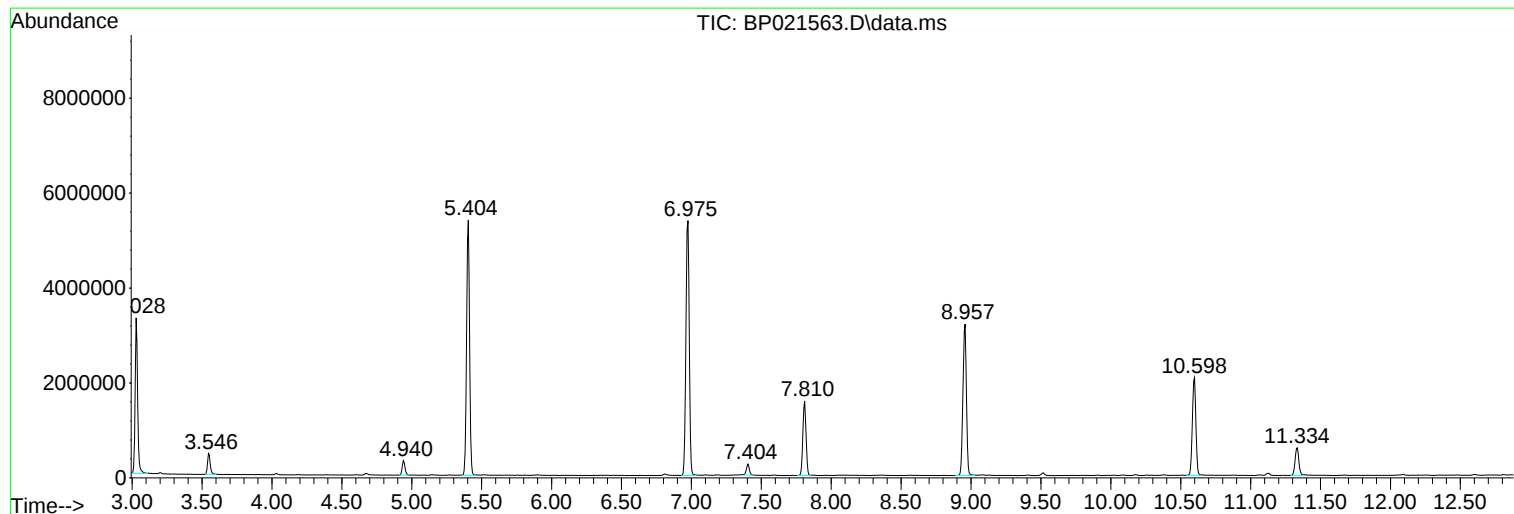

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021563.D
Acq On : 19 Aug 2024 21:47
Operator : RC/JU
Sample : P3518-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-10-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081924\
Data File : BP021563.D
Acq On : 19 Aug 2024 21:47
Operator : RC/JU
Sample : P3518-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-10-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------