


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081924\  
Data File : BP021548.D  
Acq On : 19 Aug 2024 10:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081324.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Aug 14 00:00:30 2024

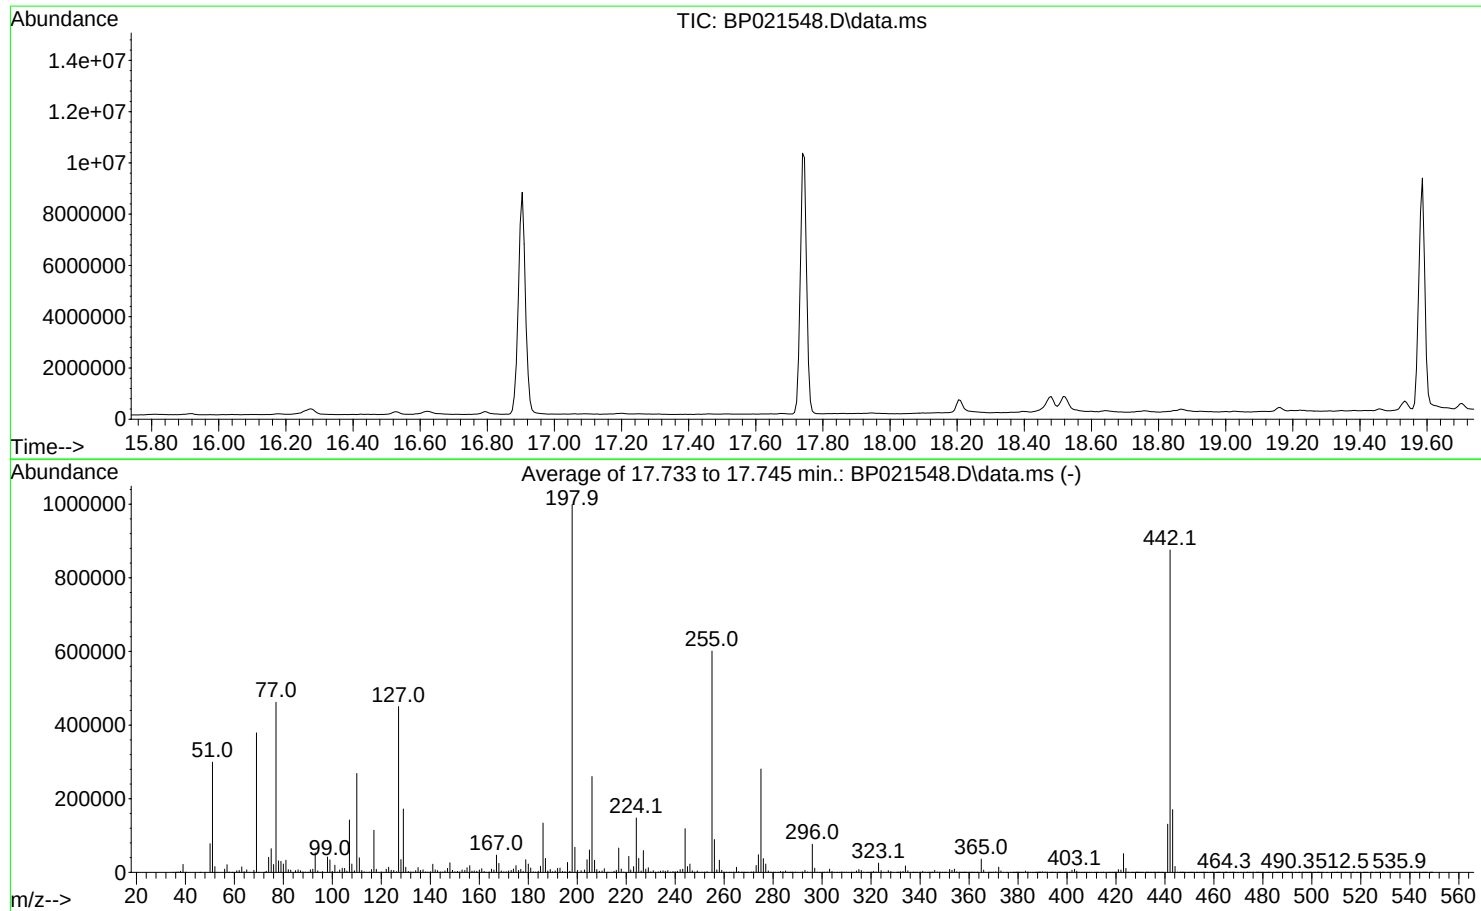

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2498

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 30.0         | 299560     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 5640       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.9         | 378962     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 671        | PASS                |
| 127            | 198             | 10              | 80              | 45.1         | 450384     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 2019       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 999193     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 68469      | PASS                |
| 275            | 198             | 10              | 60              | 28.1         | 280767     | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 36247      | PASS                |
| 441            | 198             | 0.01            | 100             | 13.1         | 130997     | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 875797     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 170263     | PASS                |

### DDT Breakdown


| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/19/2024     | BNA_P            | <u>BP021548.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 3598892          | 20.886             |
| DDD           | 196258           | 20.421             |
| DDE           | 3498             | 19.898             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 199756        | 3798648          | 5.26               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081924\  
Data File : BP021548.D  
Acq On : 19 Aug 2024 10:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Aug 19 13:07:07 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 14 00:00:30 2024  
Response via : Initial Calibration

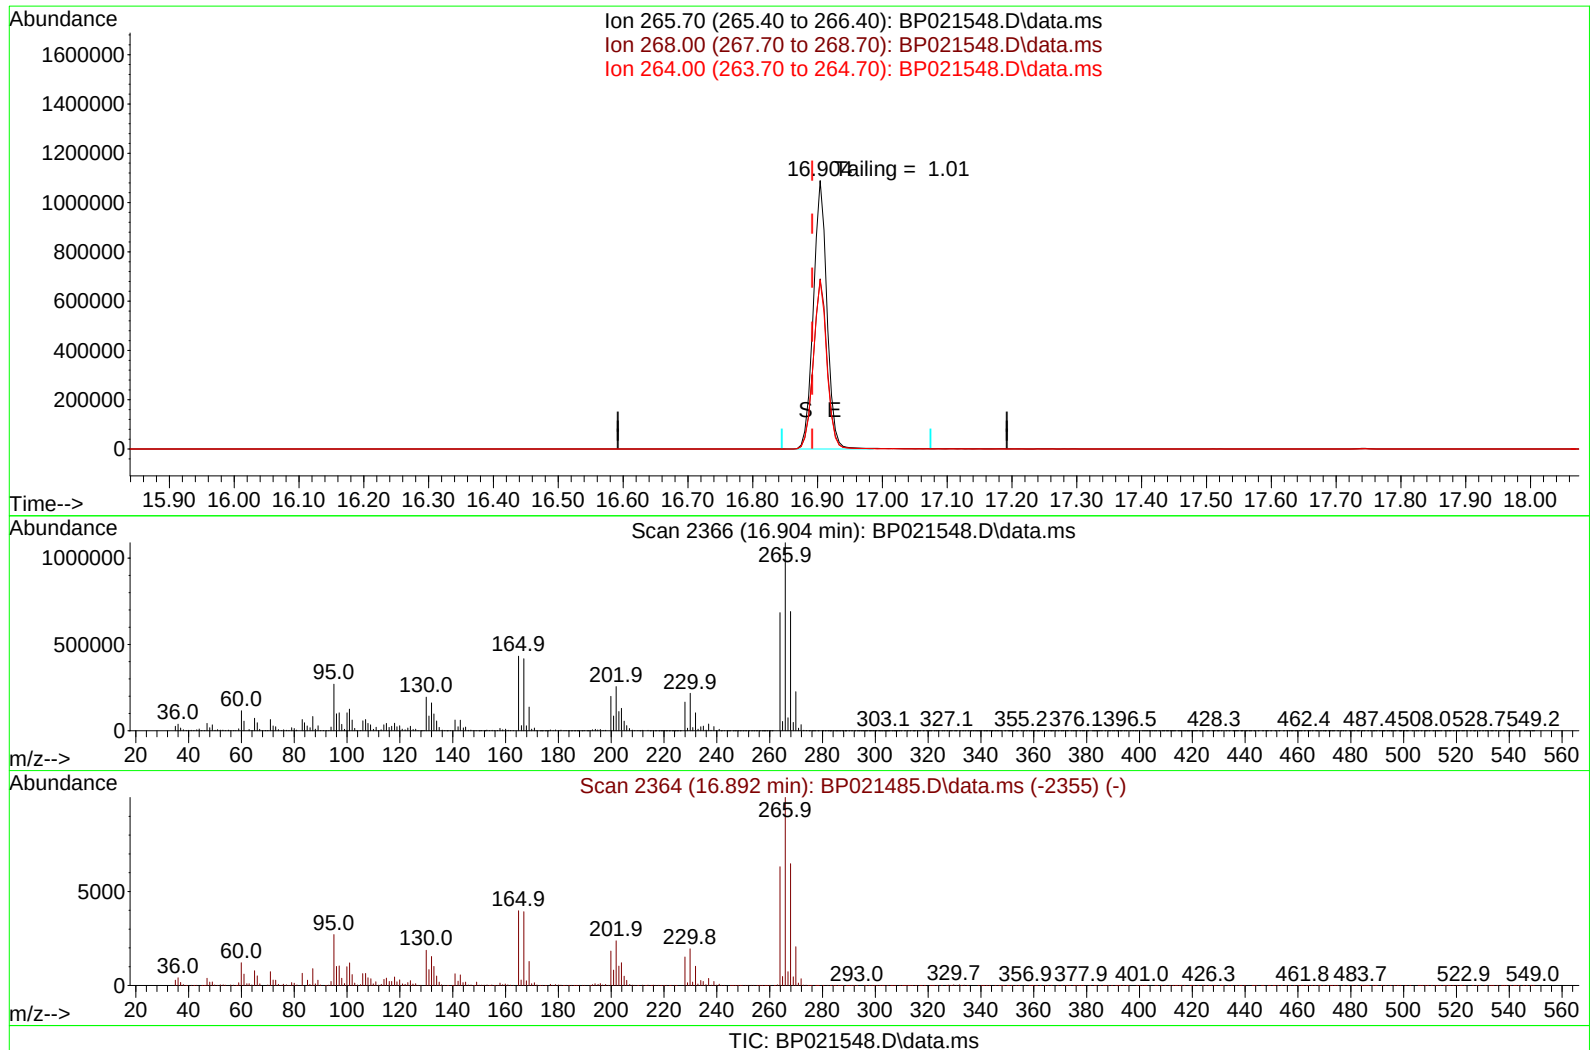

TIC: BP021548.D\data.ms

**(70) Pentachlorophenol (C)**

16.904min (+ 0.012) 2378228.58 ng




response 1591028

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.70  | 63.38  |
| 264.00 | 63.10  | 62.78  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081924\  
Data File : BP021548.D  
Acq On : 19 Aug 2024 10:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Aug 19 13:07:07 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 14 00:00:30 2024  
Response via : Initial Calibration

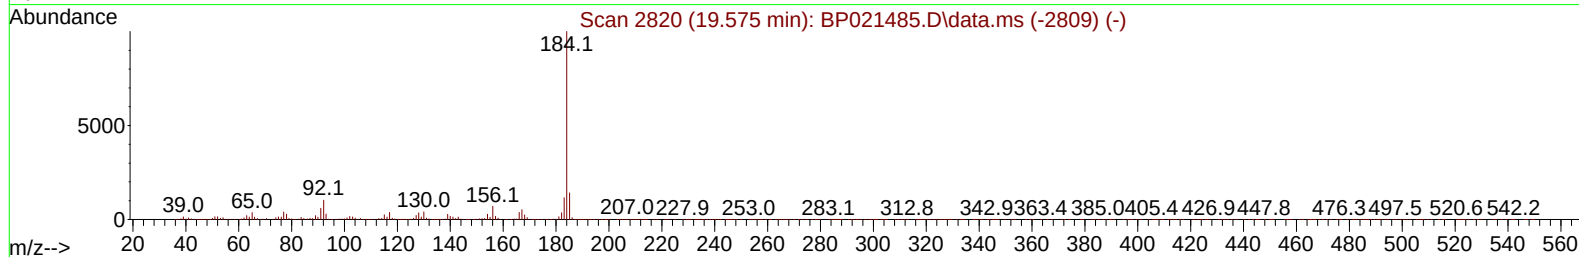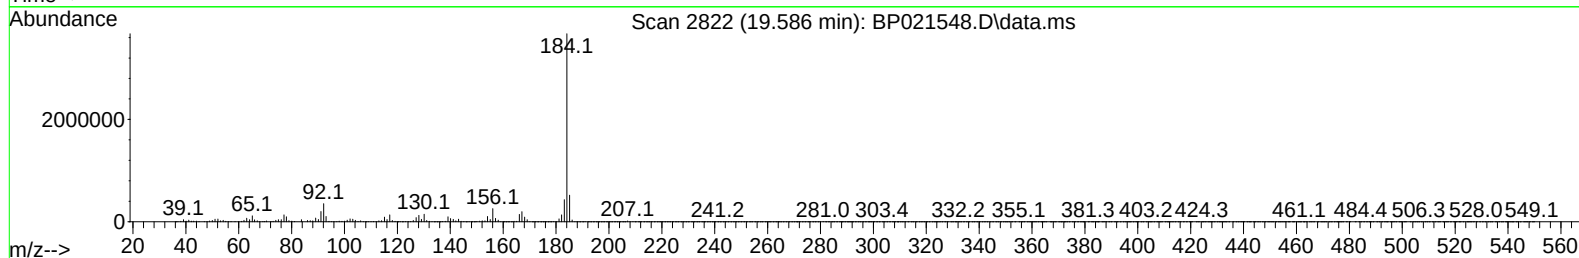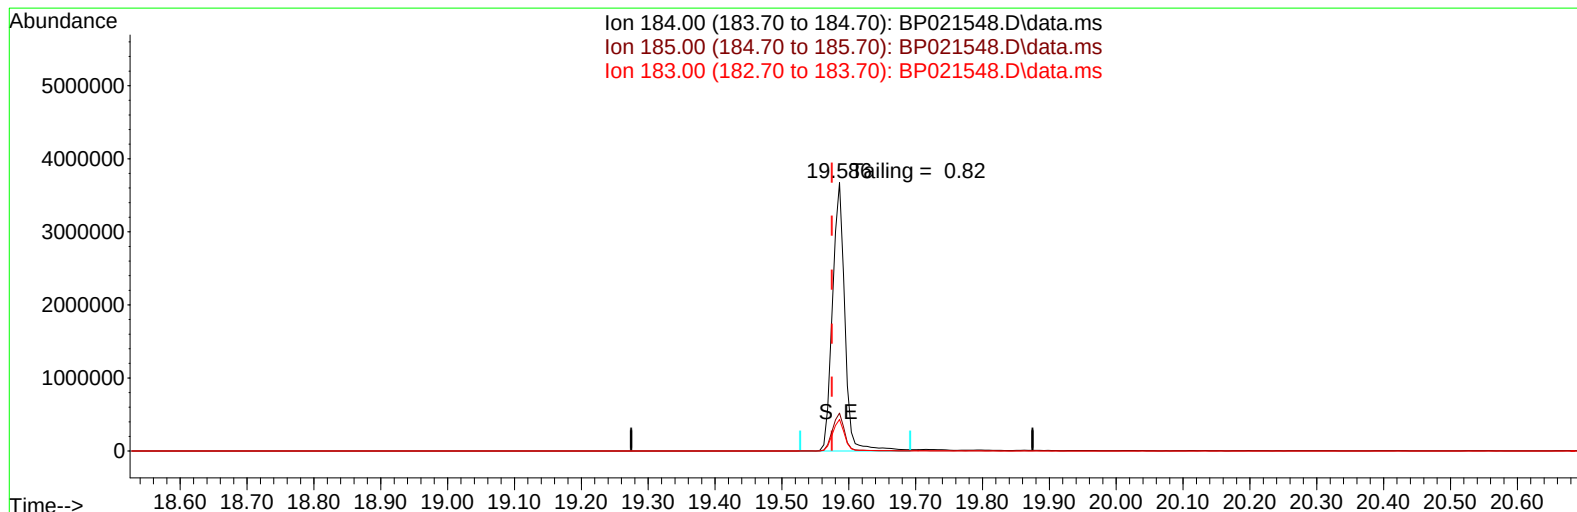

TIC: BP021548.D\data.ms

**(77) Benzidine**

**19.586min (+ 0.011) -20.00 ng**

**response 4716481**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.15  |
| 183.00 | 11.60  | 11.79  |
| 0.00   | 0.00   | 0.00   |