
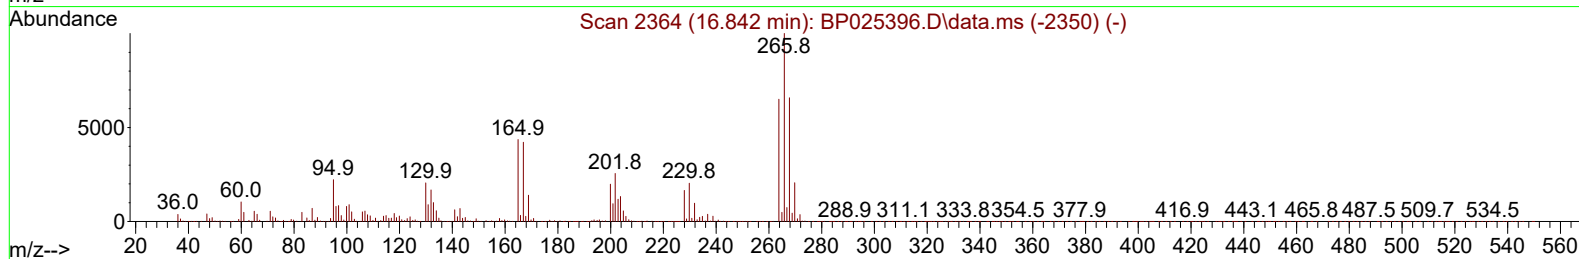
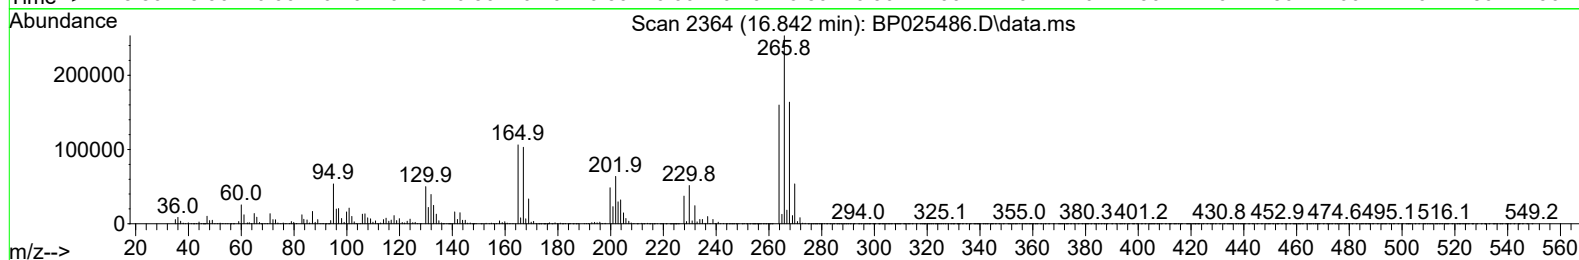


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081925\  
Data File : BP025486.D  
Acq On : 19 Aug 2025 23:05  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 02:50:06 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

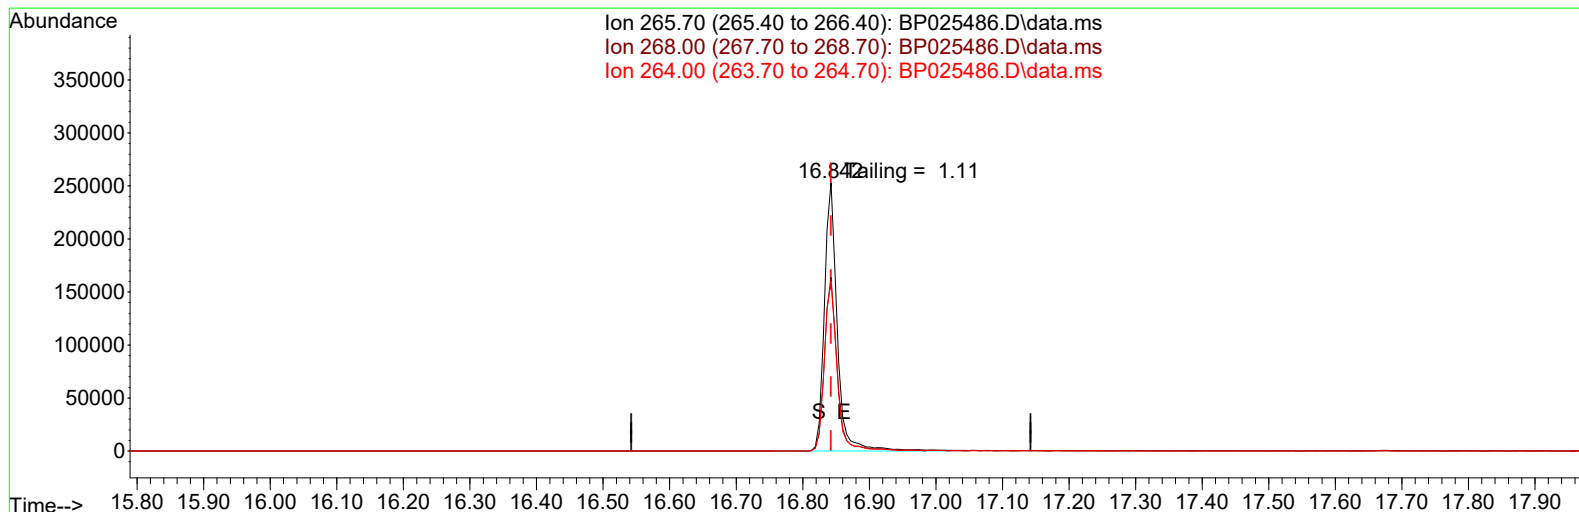

TIC: BP025486.D\data.ms

**(70) Pentachlorophenol (C)**




**16.842min (+ 0.000) 158046.45 ng**

**response 338337**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.80  | 64.68  |
| 264.00 | 65.00  | 63.19  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081925\  
Data File : BP025486.D  
Acq On : 19 Aug 2025 23:05  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 02:50:06 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

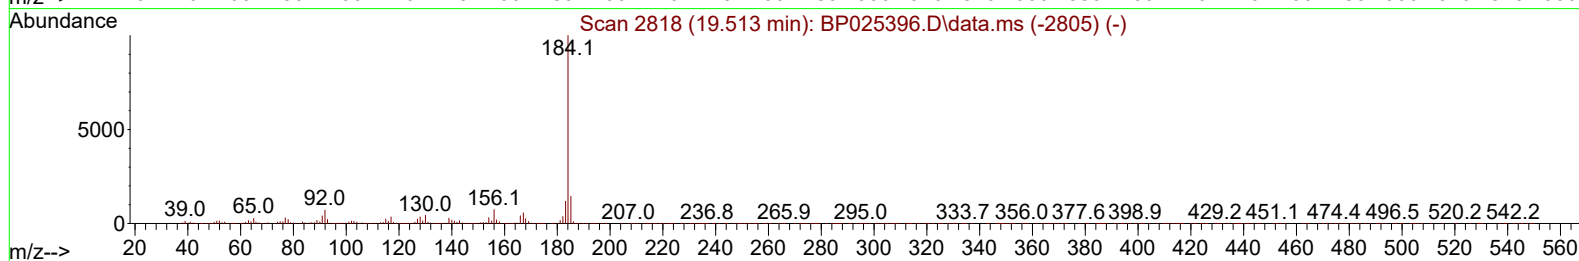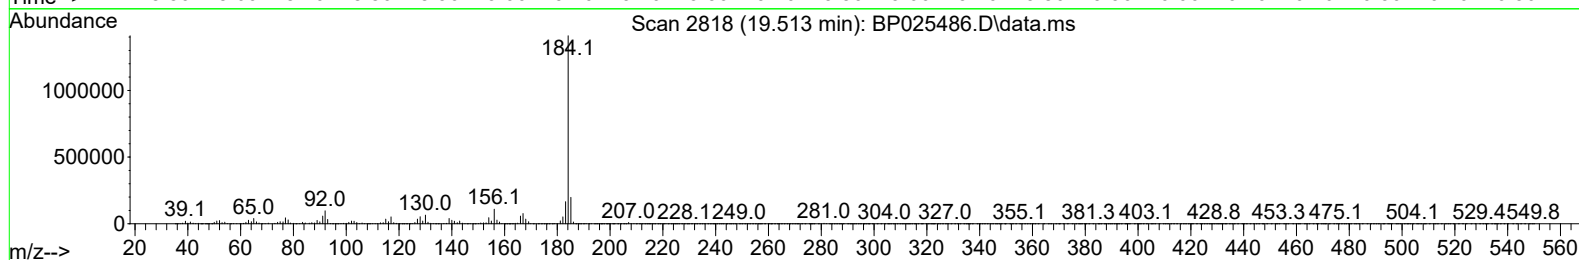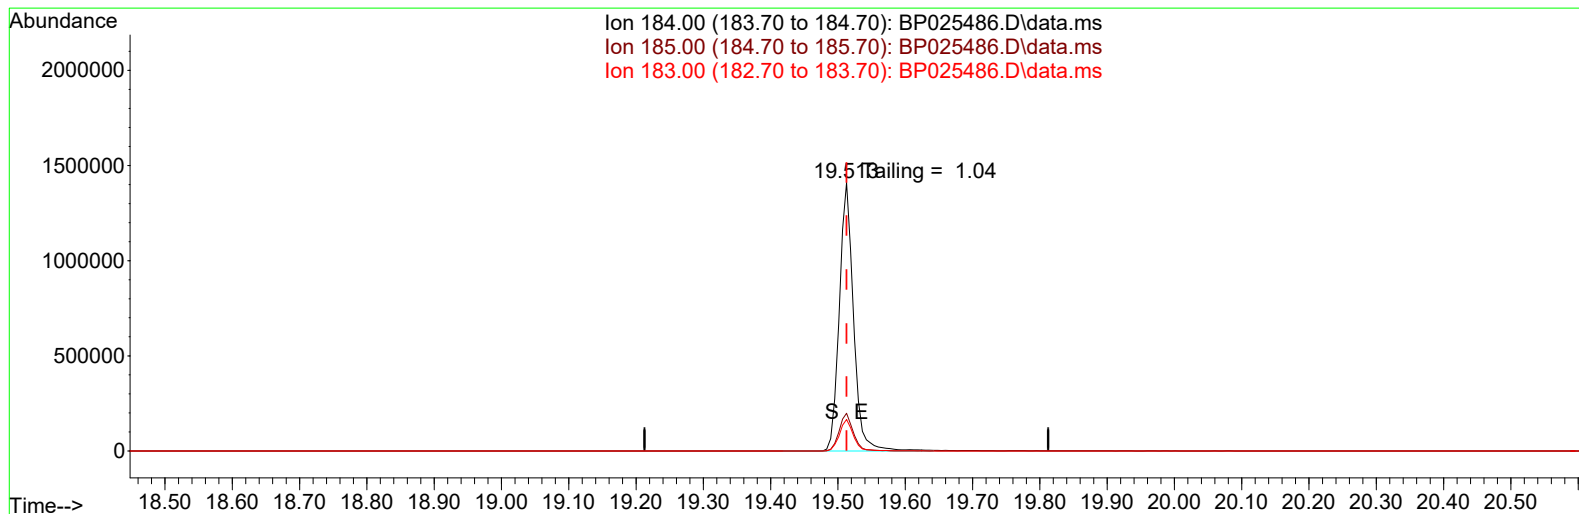

TIC: BP025486.D\data.ms

**(77) Benzidine**

19.513min (+ 0.000) 55037.12 ng

response 2058618

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.07  |
| 183.00 | 11.80  | 11.73  |
| 0.00   | 0.00   | 0.00   |