
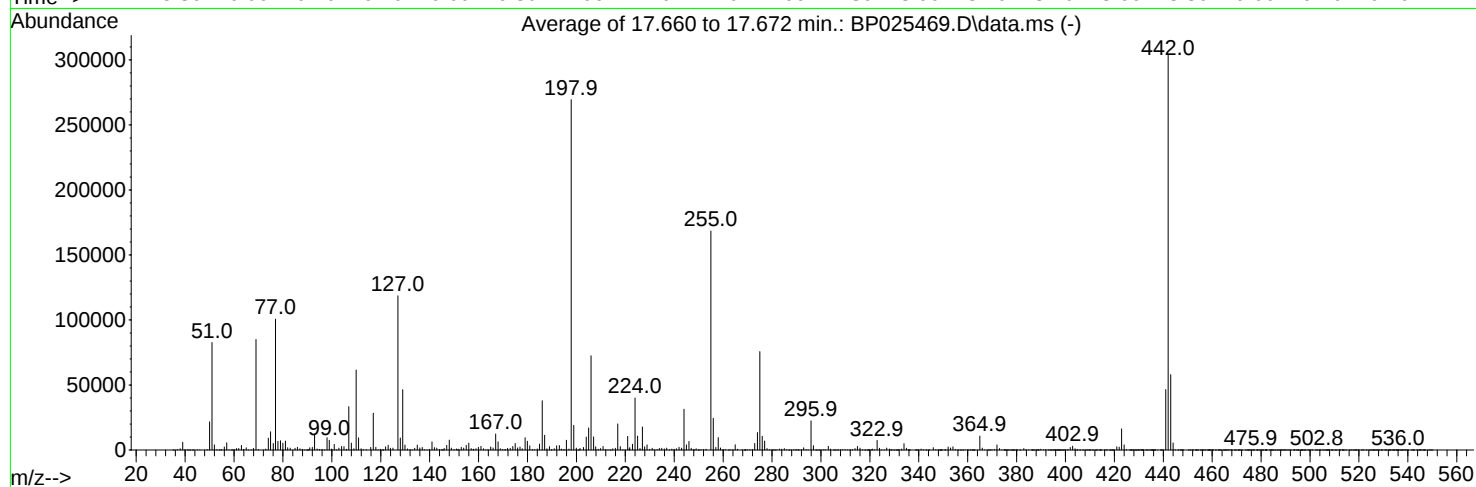


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081925\
Data File : BP025469.D
Acq On : 19 Aug 2025 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

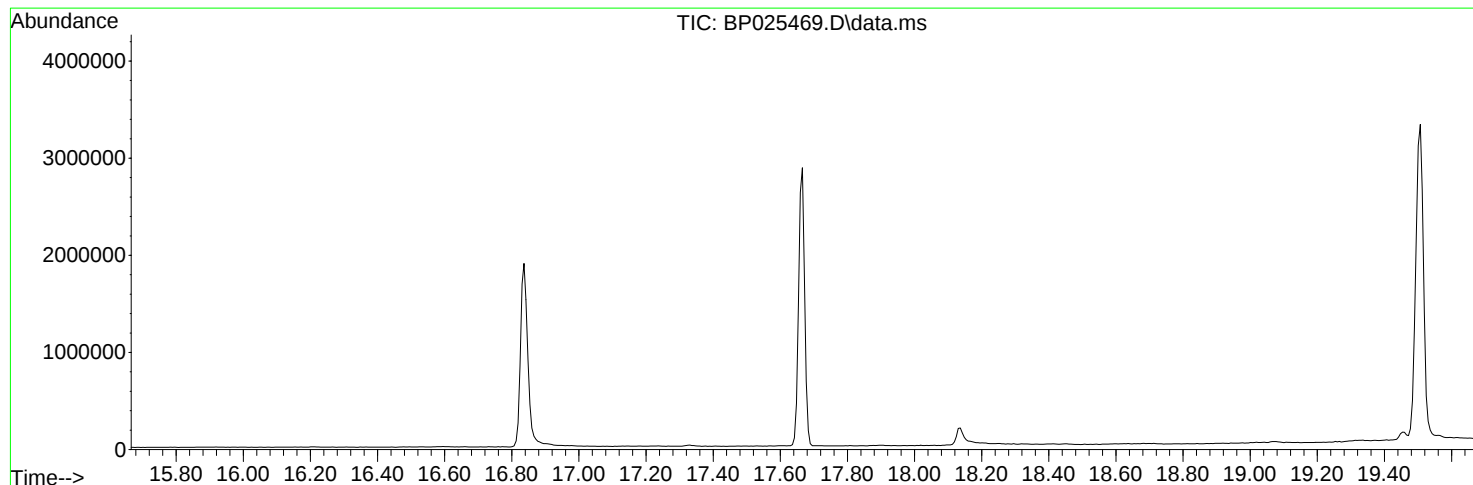




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2495

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	1264	PASS
69	69	100	100	100.0	85071	PASS
70	69	0.00	2	0.4	346	PASS
197	198	0.00	2	0.3	784	PASS
198	198	100	100	100.0	269485	PASS
199	198	5	9	7.0	18925	PASS
365	198	1	100	4.0	10734	PASS
441	443	0.01	150	80.2	46560	PASS
442	442	100	100	100.0	303675	PASS
443	442	15	24	19.1	58026	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081925\
Data File : BP025469.D
Acq On : 19 Aug 2025 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 19 12:14:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

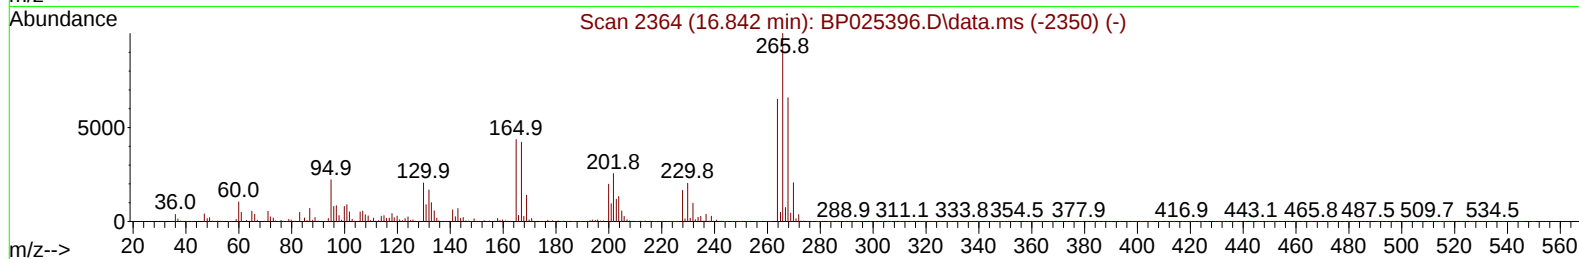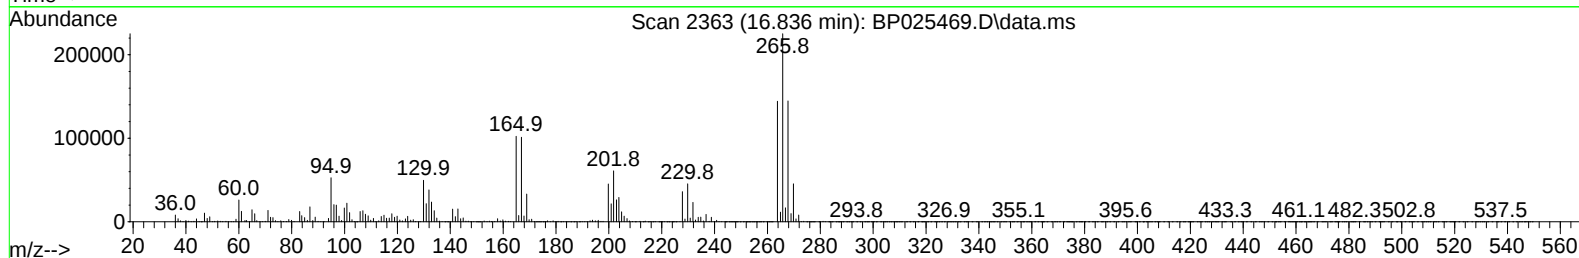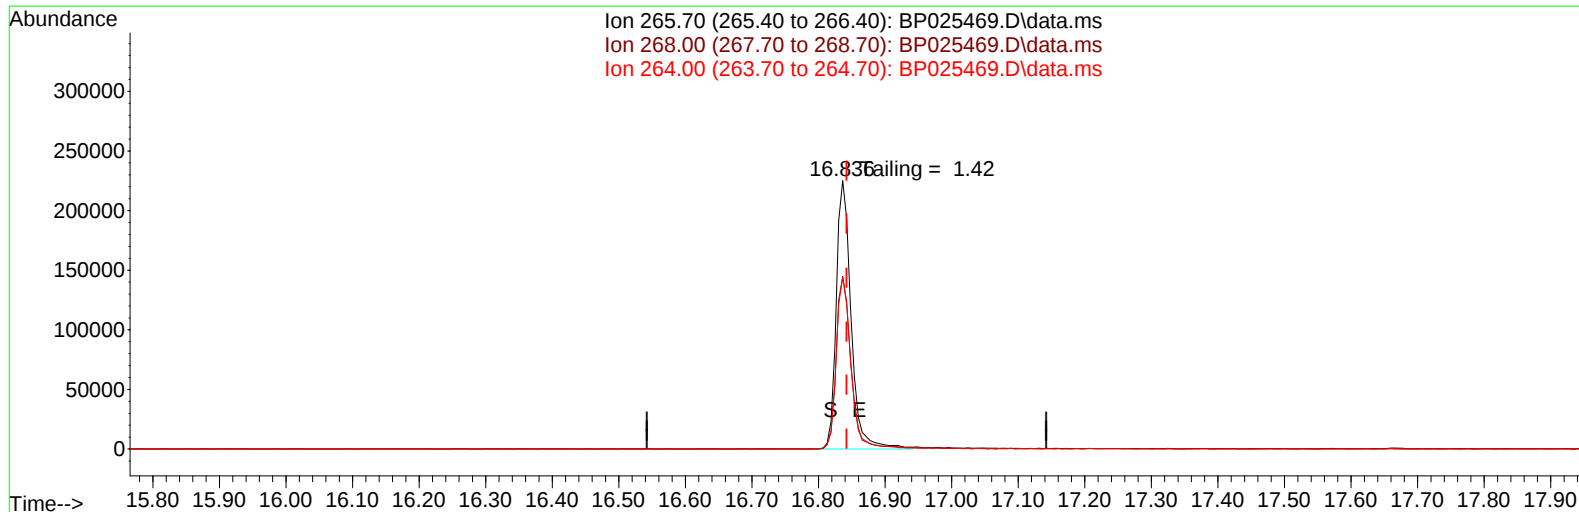

TIC: BP025469.D\data.ms

(70) Pentachlorophenol (C)

16.836min (-0.006) 311283.12 ng




response 350725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.27
264.00	65.00	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081925\
Data File : BP025469.D
Acq On : 19 Aug 2025 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 19 12:14:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

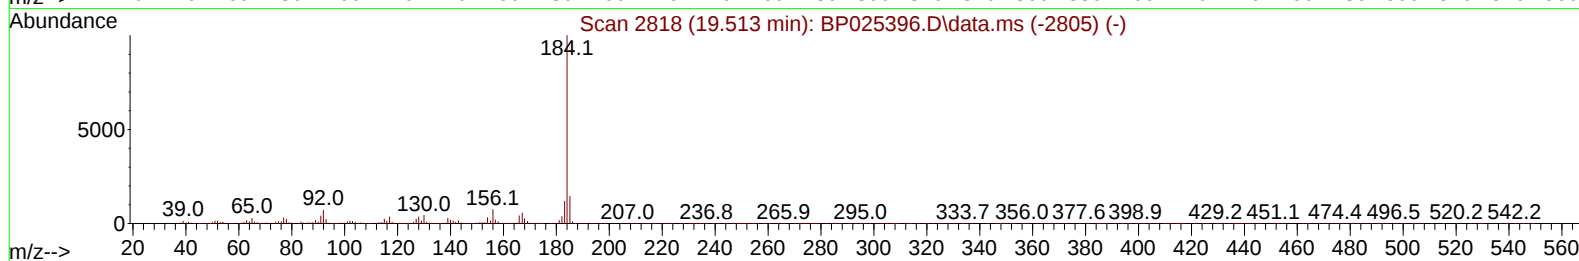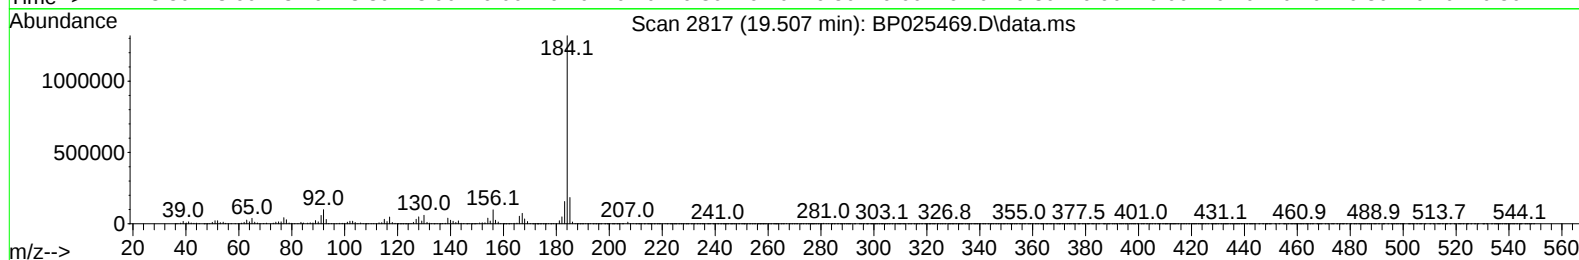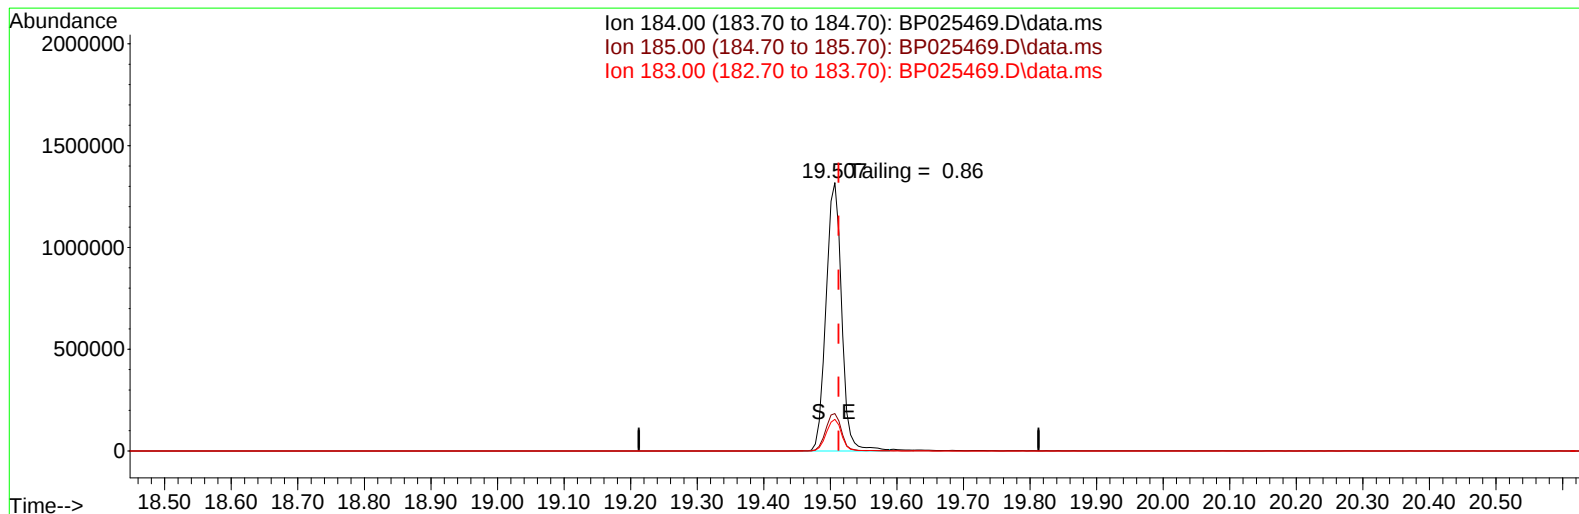

TIC: BP025469.D\data.ms

(77) Benzidine

19.507min (-0.006) 183825.79 ng

response 2158114

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	11.80	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/19/2025	BNA_P	<u>BP025469.D</u>
Compound Name	Response	Retention Time
DDT	1098473	20.807
DDD	16608	20.348
DDE	3876	19.819
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20484	1118957	1.83

Instrument :
BNA_P
ClientSampleId :
DFTPP