
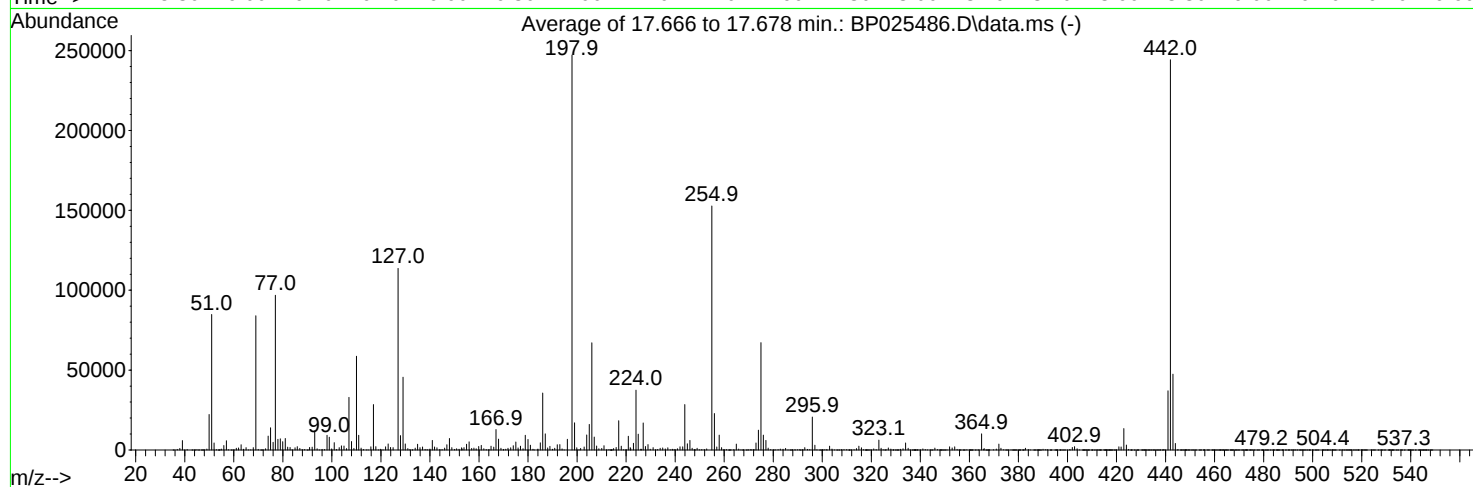


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081925\
Data File : BP025486.D
Acq On : 19 Aug 2025 23:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

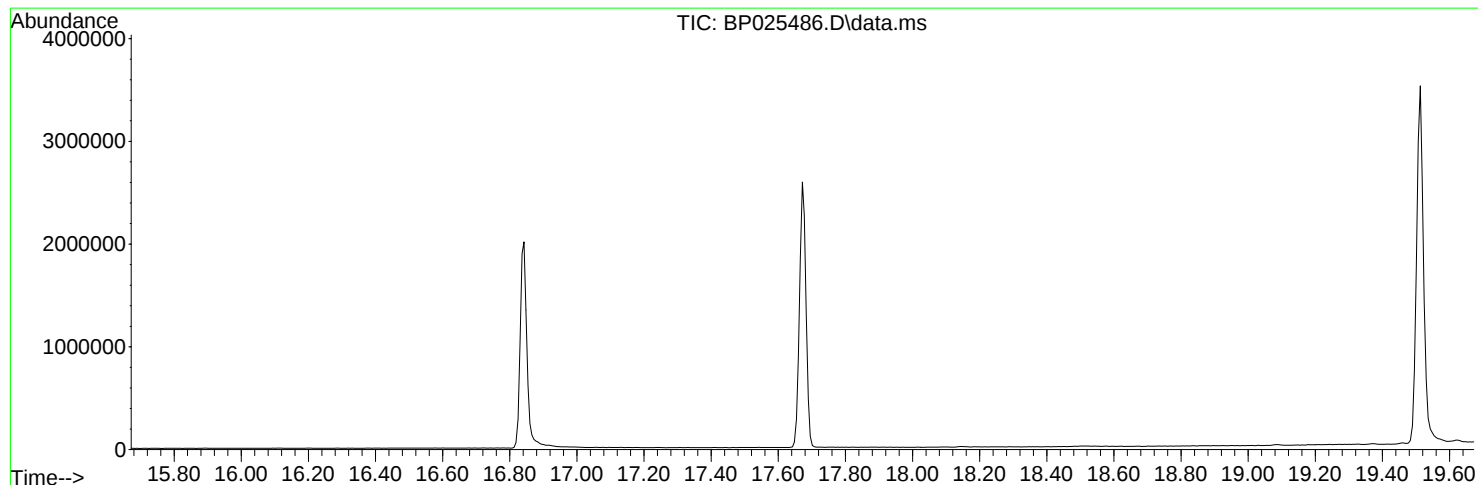




AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2490

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	1538	PASS
69	69	100	100	100.0	83998	PASS
70	69	0.00	2	0.5	443	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	247117	PASS
199	198	5	9	6.9	17035	PASS
365	198	1	100	4.1	10085	PASS
441	443	0.01	150	78.2	37107	PASS
442	442	100	100	100.0	244224	PASS
443	442	15	24	19.4	47432	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081925\
Data File : BP025486.D
Acq On : 19 Aug 2025 23:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 02:50:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

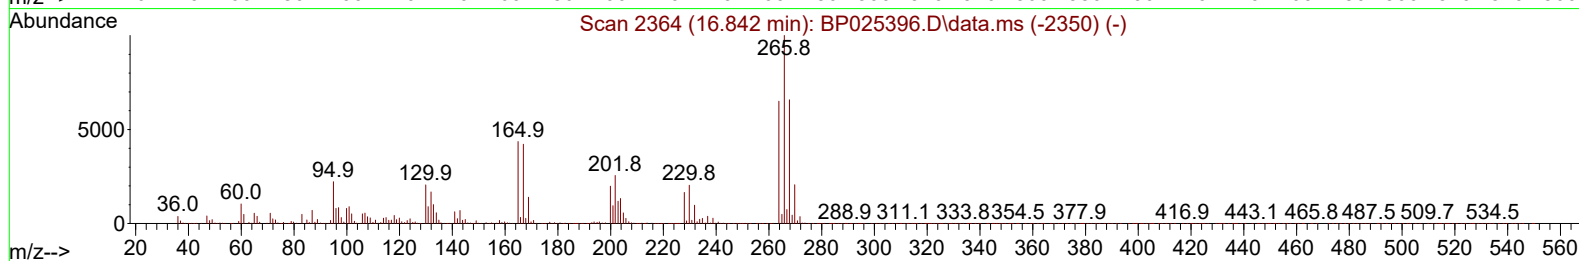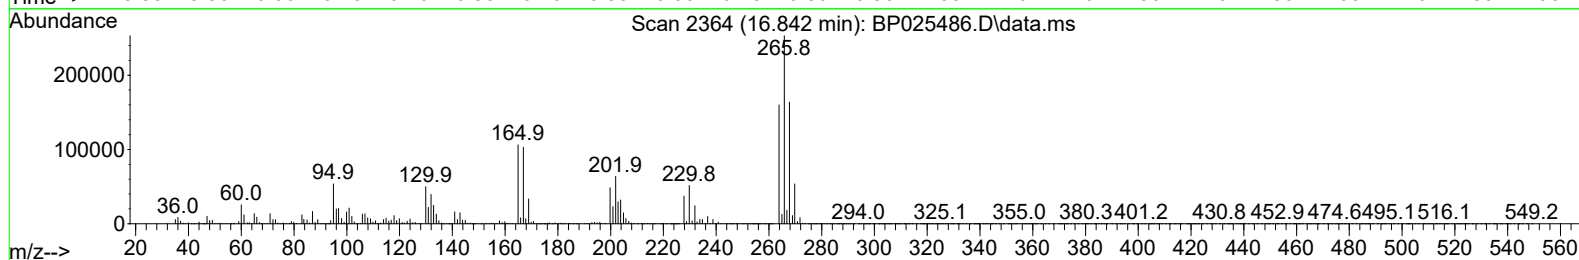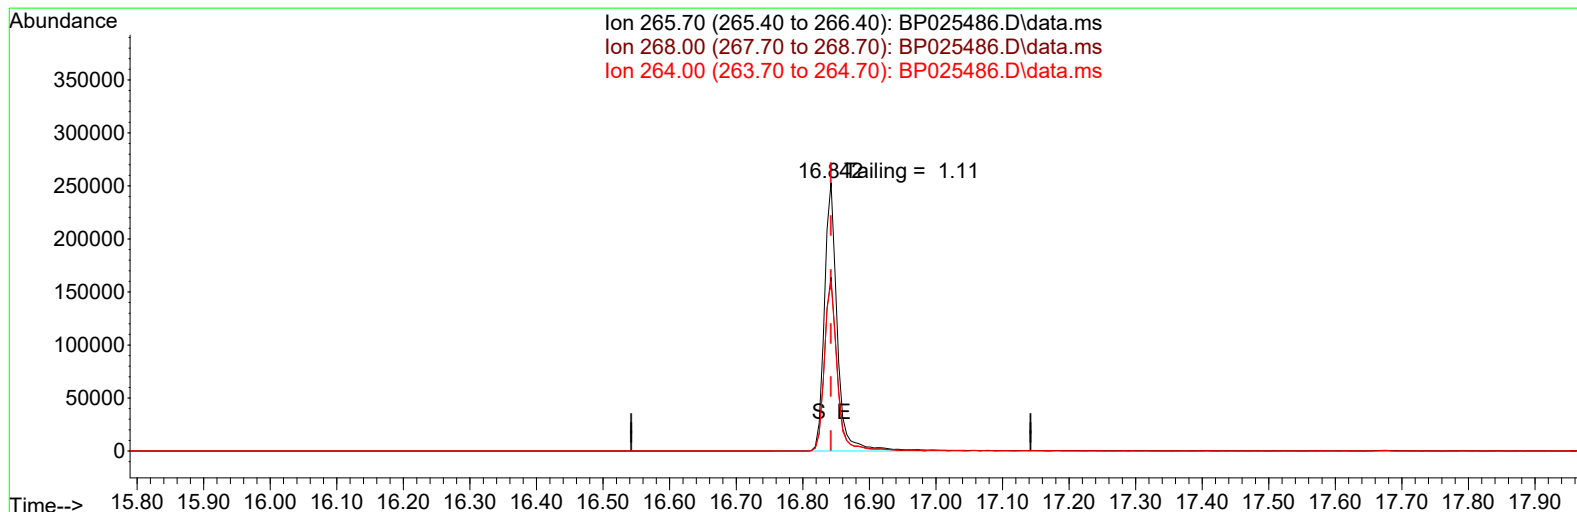

TIC: BP025486.D\data.ms

(70) Pentachlorophenol (C)

16.842min (+ 0.000) 158046.45 ng




response 338337

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.68
264.00	65.00	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081925\
Data File : BP025486.D
Acq On : 19 Aug 2025 23:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 02:50:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

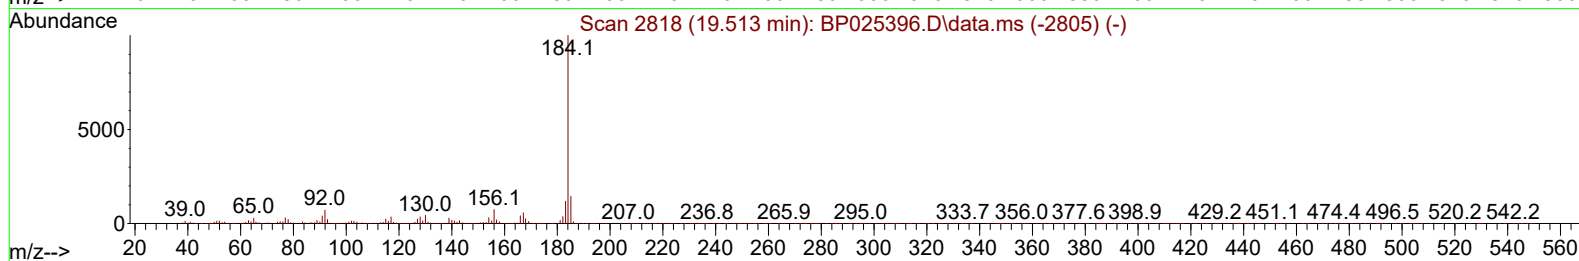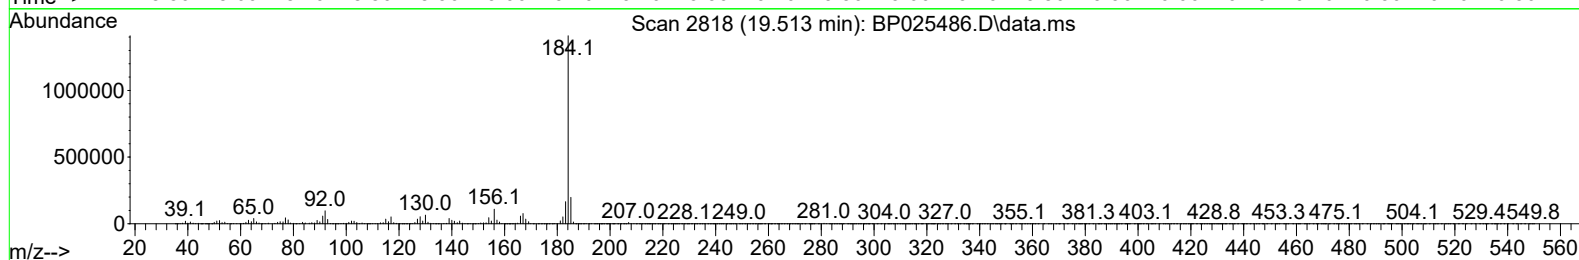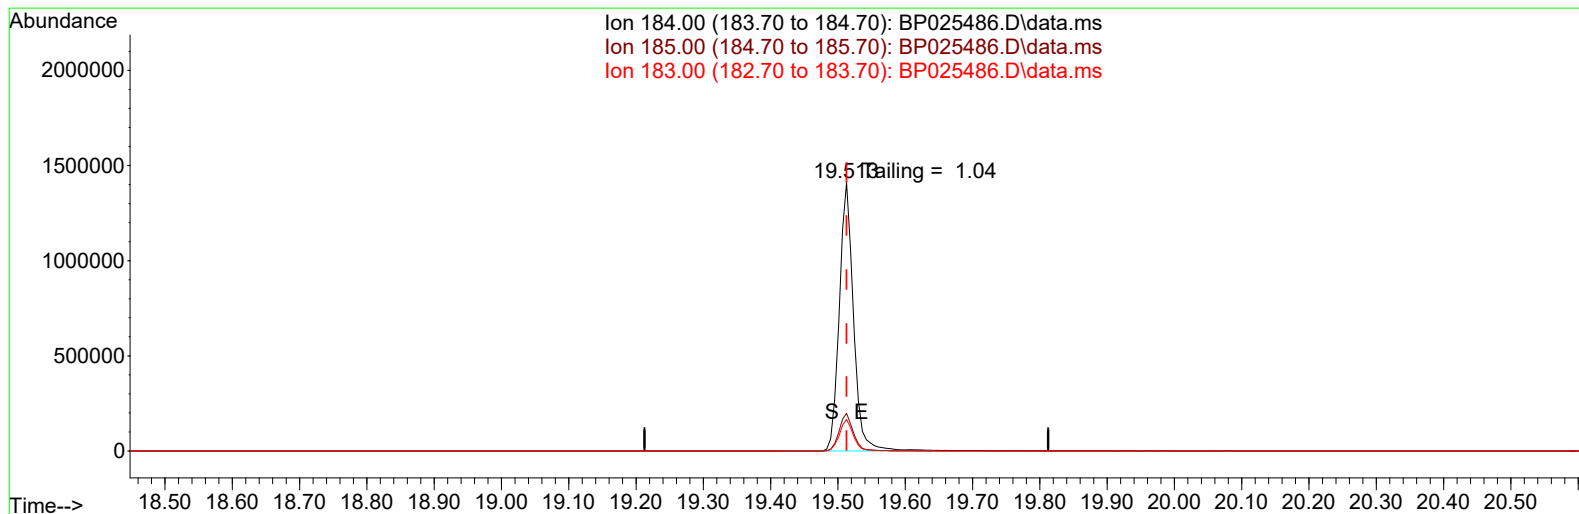

TIC: BP025486.D\data.ms

(77) Benzidine

19.513min (+ 0.000) 55037.12 ng

response 2058618

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.07
183.00	11.80	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/19/2025	BNA_P	<u>BP025486.D</u>
Compound Name	Response	Retention Time
DDT	1027414	20.807
DDD	15935	20.342
DDE	3495	19.83
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19430	1046844	1.86

Instrument :
BNA_P
ClientSampleId :
DFTPP