

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082020\
 Data File : BP003061.D
 Acq On : 20 Aug 2020 12:26
 Operator : CG/JU
 Sample : PB131060TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131060TB

Quant Time: Aug 20 14:49:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 14:07:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	392137	20.00	ng	0.00
21) Naphthalene-d8	10.46	136	1521054	20.00	ng	-0.01
39) Acenaphthene-d10	14.32	164	856960	20.00	ng	-0.01
64) Phenanthrene-d10	17.07	188	1695239	20.00	ng	-0.01
76) Chrysene-d12	21.16	240	1218893	20.00	ng	-0.01
86) Perylene-d12	23.40	264	1161310	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	2304936	89.96	ng	0.00
7) Phenol-d6	6.86	99	2663283	74.87	ng	0.00
23) Nitrobenzene-d5	8.83	82	1544711	55.00	ng	0.00
42) 2,4,6-Tribromophenol	15.82	330	1123760	105.51	ng	0.00
45) 2-Fluorobiphenyl	12.94	172	4181144	66.66	ng	-0.01
79) Terphenyl-d14	19.65	244	4967440	81.59	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082020\
Data File : BP003061.D
Acq On : 20 Aug 2020 12:26
Operator : CG/JU
Sample : PB131060TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131060TB

Quant Time: Aug 20 14:49:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 14:07:35 2020
Response via : Initial Calibration

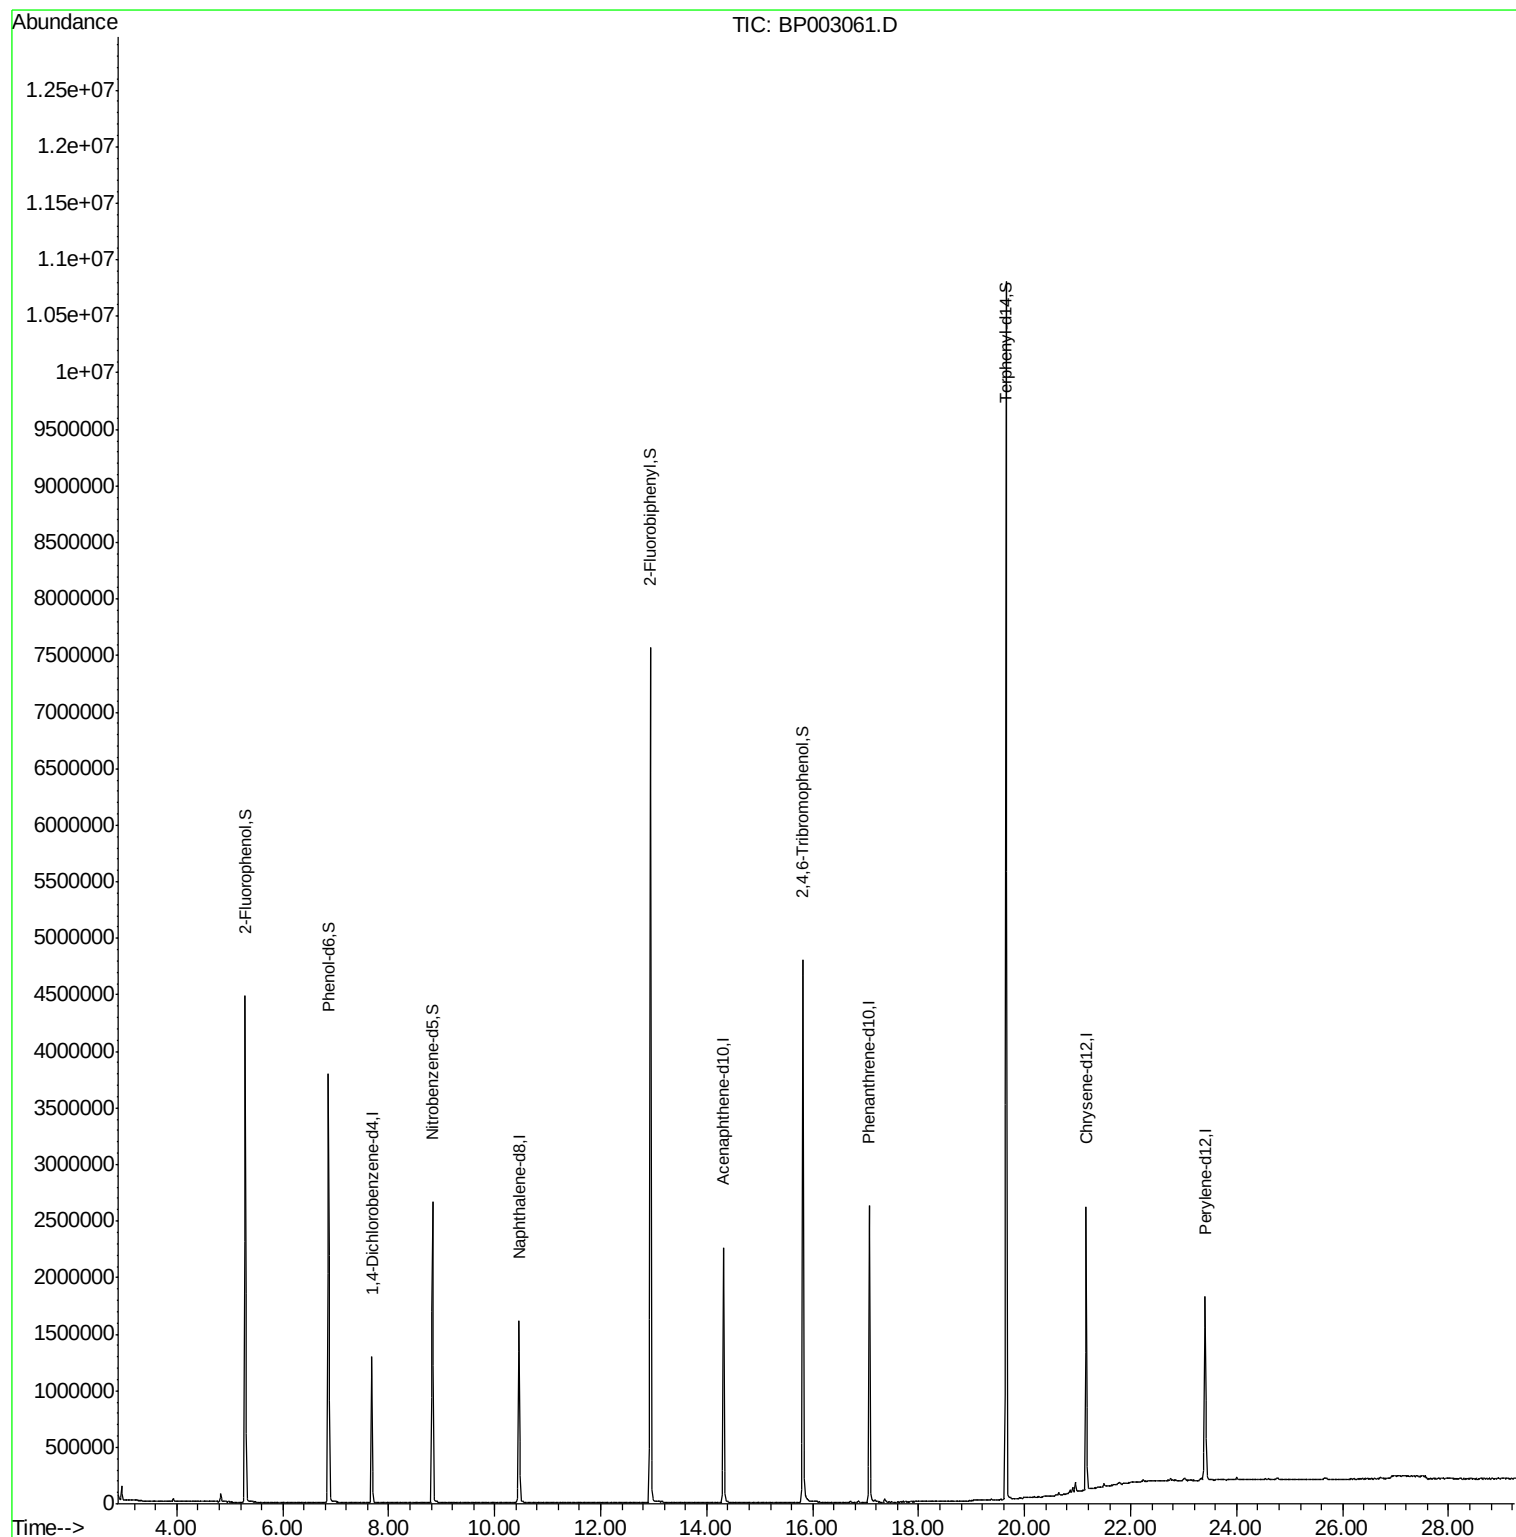




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.68 min Scan# 815
Delta R.T. -0.01 min
Lab File: BP003061.D
Acq: 20 Aug 2020 12:26

Instrument :
BNA_P
ClientSampleId :
PB131060TB

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.4	126.1	189.1
115	54.9	43.4	65.2



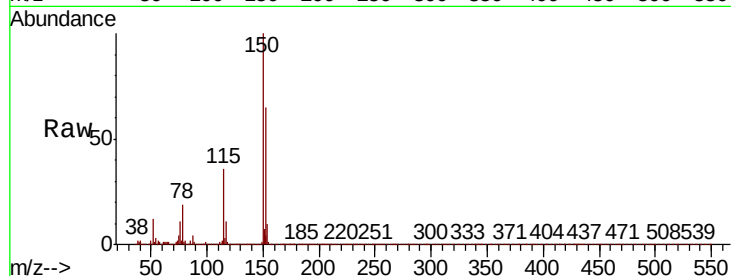


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

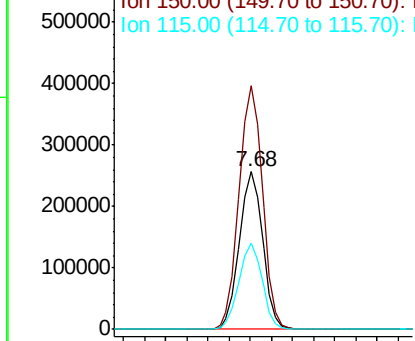

#5

2-Fluorophenol
Concen: 89.961 ng
RT: 5.29 min Scan# 409
Delta R.T. -0.00 min
Lab File: BP003061.D
Acq: 20 Aug 2020 12:26

Tgt Ion	Ratio	Lower	Upper
112	100		
64	39.9	33.4	50.2
63	20.7	17.4	26.0






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

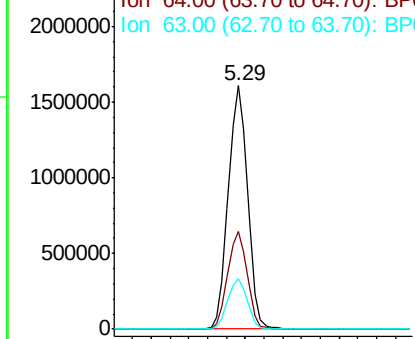

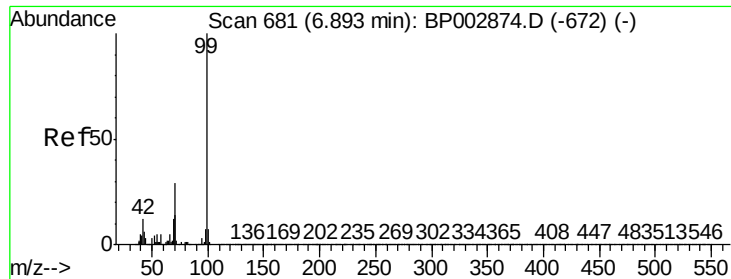

#7

Phenol-d6

Concen: 74.870 ng

RT: 6.86 min Scan# 676

Delta R.T. -0.01 min

Lab File: BP003061.D

Acq: 20 Aug 2020 12:26

Instrument :


BNA_P

ClientSampleId :

PB131060TB

Tot Ion: 99 Resp: 2663283

Ion	Ratio	Lower	Upper
99	100		
42	10.4	8.0	12.0
71	28.9	21.3	31.9






Abundance

Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

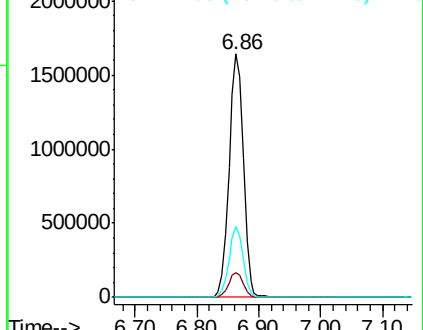

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.46 min Scan# 1287


Delta R.T. -0.01 min

Lab File: BP003061.D

Acq: 20 Aug 2020 12:26

Tgt Ion: 136 Resp: 1521054

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	4.6	3.8	5.8
68	4.3	3.8	5.8





Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0




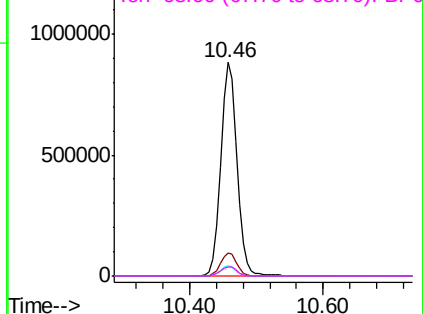


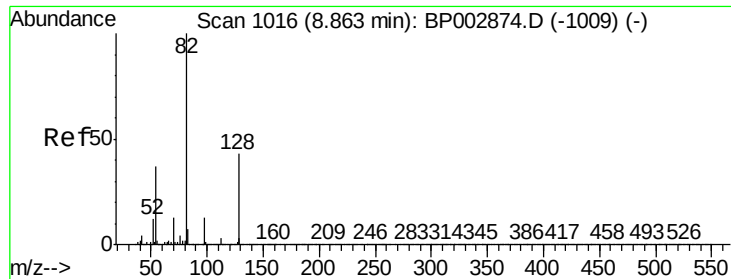

#23
Nitrobenzene-d5
Concen: 55.005 ng
RT: 8.83 min Scan# 1010
Delta R.T. -0.01 min
Lab File: BP003061.D
Acq: 20 Aug 2020 12:26




Instrument :
BNA_P
ClientSampleId :
PB131060TB


Tot Ion: 82 Resp: 1544711
Ion Ratio Lower Upper
82 100
128 58.2 45.1 67.7
54 36.0 28.8 43.2

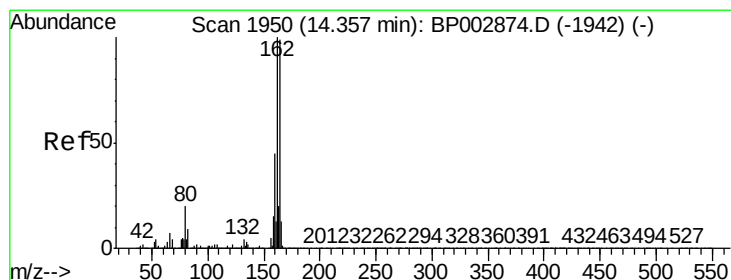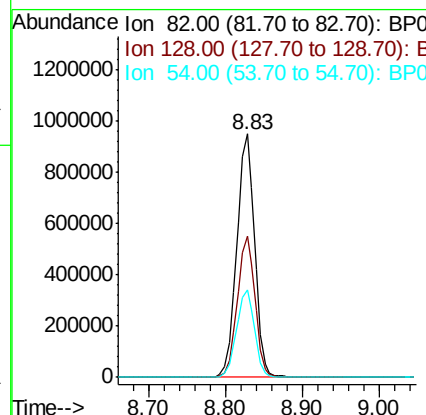

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.32 min Scan# 1943
Delta R.T. -0.01 min
Lab File: BP003061.D
Acq: 20 Aug 2020 12:26

Tgt Ion:164 Resp: 856960
Ion Ratio Lower Upper
164 100
162 102.0 81.4 122.0
160 45.1 35.5 53.3


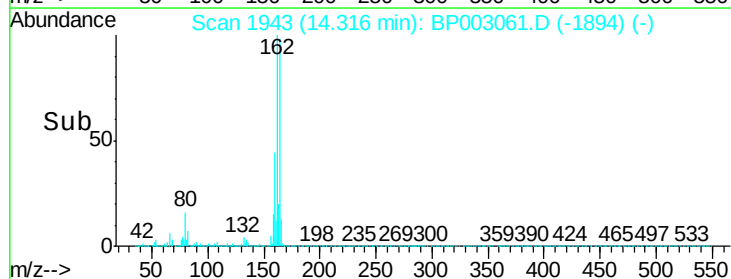
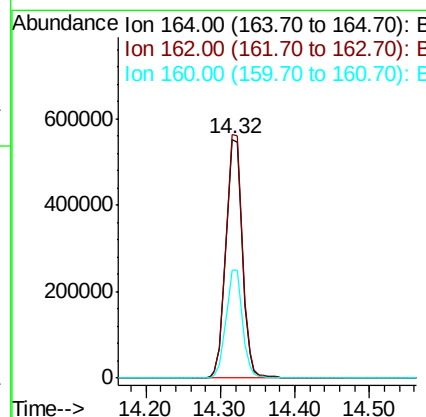
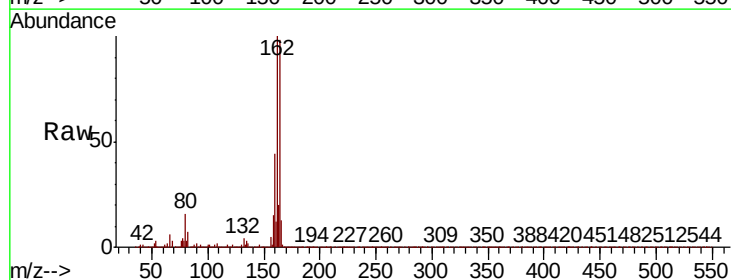


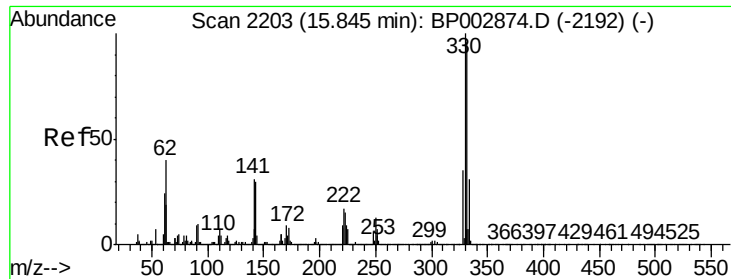

#42
2,4,6-Tribromophenol
Concen: 105.507 ng
RT: 15.82 min Scan# 2198
Delta R.T. -0.01 min
Lab File: BP003061.D
Acq: 20 Aug 2020 12:26




Instrument :
BNA_P
ClientSampleId :
PB131060TB


Tot Ion:330 Resp: 1123760
Ion Ratio Lower Upper
330 100
332 96.7 77.0 115.6
141 29.8 26.7 40.1

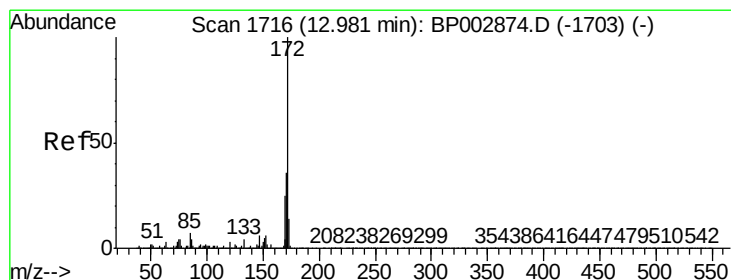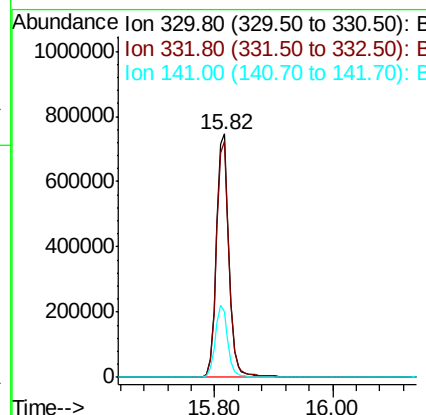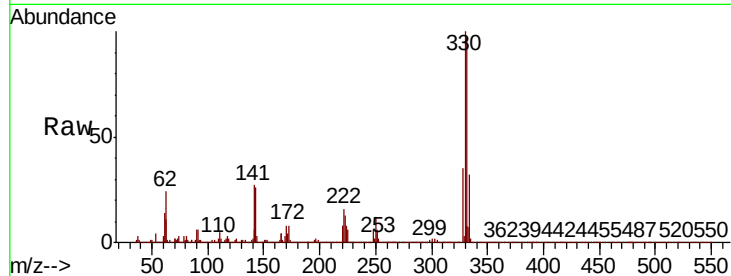

#45
2-Fluorobiphenyl
Concen: 66.662 ng
RT: 12.94 min Scan# 1709
Delta R.T. -0.01 min
Lab File: BP003061.D
Acq: 20 Aug 2020 12:26

Tgt Ion:172 Resp: 4181144
Ion Ratio Lower Upper
172 100
171 36.1 29.0 43.4
170 24.0 19.1 28.7

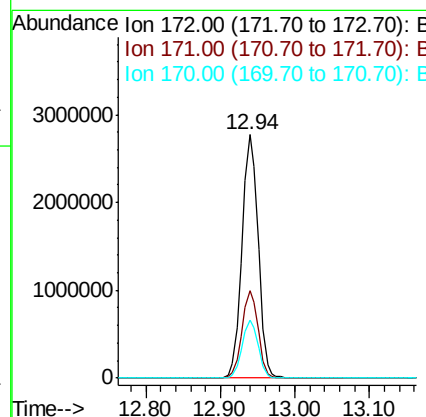

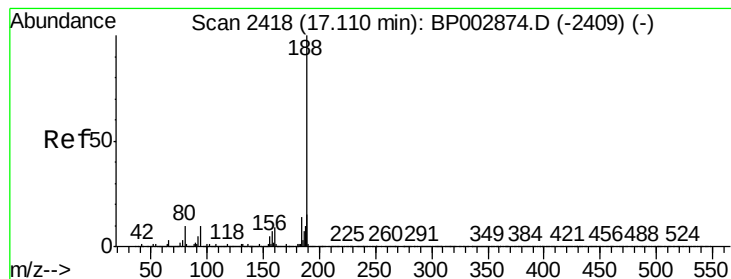

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.07 min Scan# 2411

Delta R.T. -0.01 min

Lab File: BP003061.D

Acq: 20 Aug 2020 12:26

Instrument :

BNA_P

ClientSampleId :

PB131060TB


Tot Ion:188 Resp: 1695239

Ion Ratio Lower Upper

188 100

94 8.2 7.1 10.7




80 8.1 6.7 10.1



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

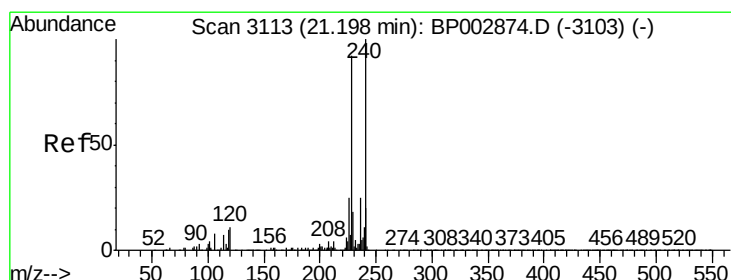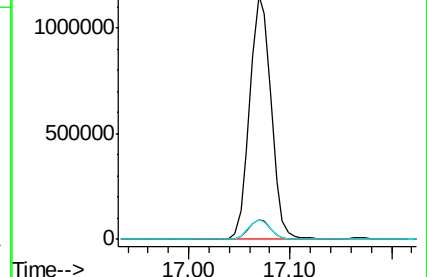

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.16 min Scan# 3107

Delta R.T. -0.01 min

Lab File: BP003061.D

Acq: 20 Aug 2020 12:26


Tgt Ion:240 Resp: 1218893

Ion Ratio Lower Upper

240 100

120 10.7 9.5 14.3



236 25.8 20.8 31.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

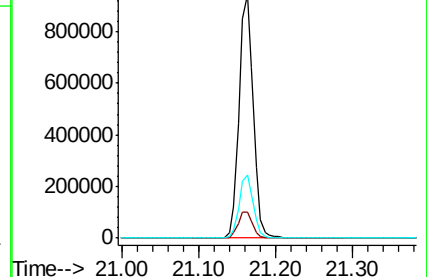

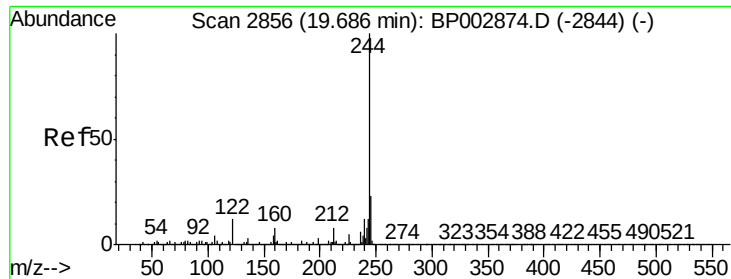

#79

Terphenyl-d14

Concen: 81.587 ng

RT: 19.65 min Scan# 2849

Delta R.T. -0.01 min

Lab File: BP003061.D

Acq: 20 Aug 2020 12:26

Instrument :


BNA_P

ClientSampleId :

PB131060TB

Tot Ion:244 Resp: 4967440



Ion	Ratio	Lower	Upper
244	100		
212	7.7	6.3	9.5
122	10.2	8.7	13.1

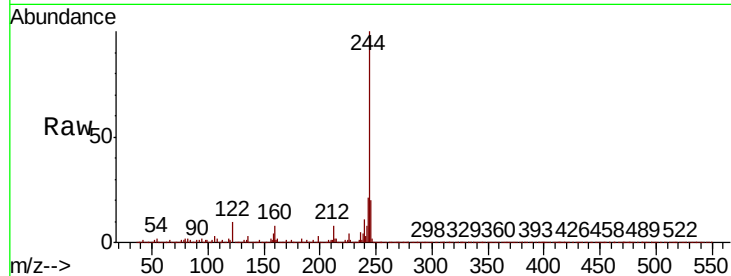

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

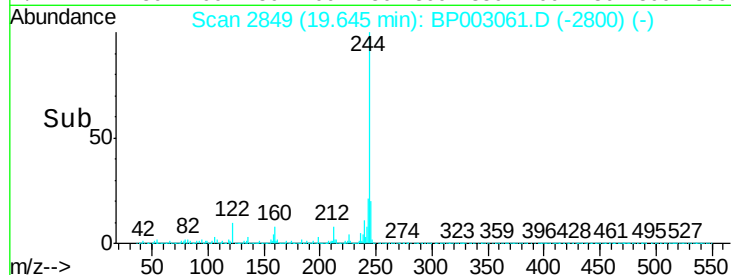

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.40 min Scan# 3488


Delta R.T. -0.02 min

Lab File: BP003061.D

Acq: 20 Aug 2020 12:26

Tgt Ion:264 Resp: 1161310

Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.2	28.8
265	21.8	17.3	25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

