


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082020\
 Data File : BP003055.D
 Acq On : 20 Aug 2020 08:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 14:07:35 2020

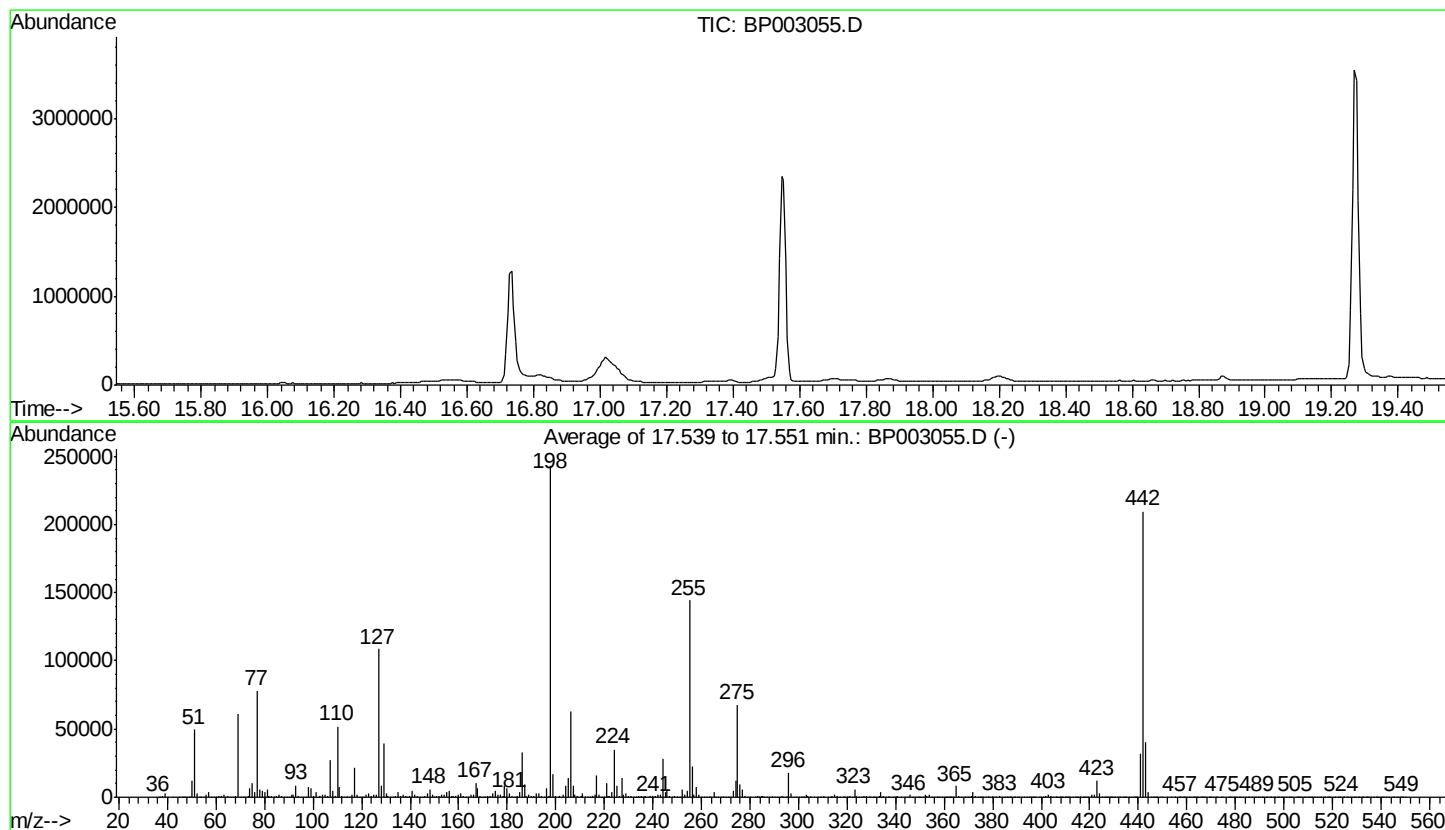

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.4	49698	PASS
68	69	0.00	2	1.8	1121	PASS
69	198	0.00	100	25.1	60911	PASS
70	69	0.00	2	0.5	297	PASS
127	198	10	80	44.7	108656	PASS
197	198	0.00	2	0.4	1089	PASS
198	198	100	100	100.0	243097	PASS
199	198	5	9	6.8	16556	PASS
275	198	10	60	27.8	67637	PASS
365	198	1	100	3.5	8392	PASS
441	198	0.01	100	13.2	32045	PASS
442	198	50	100	86.2	209472	PASS
443	442	15	24	19.3	40509	PASS