
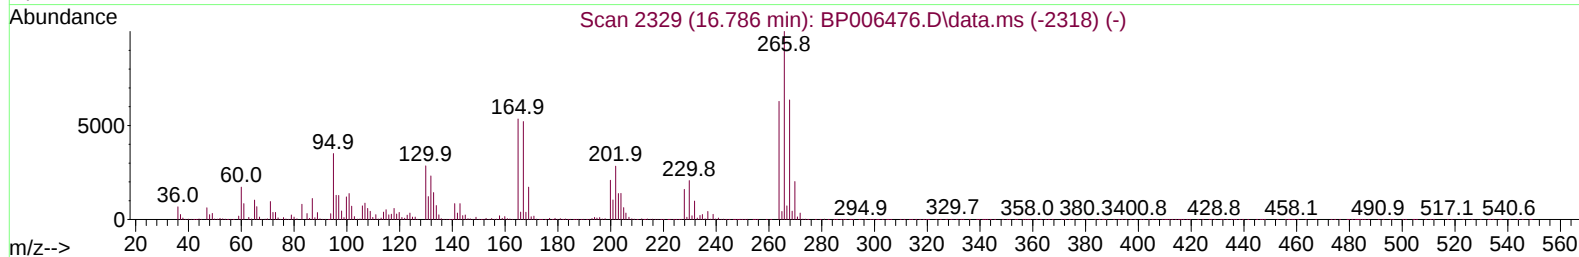
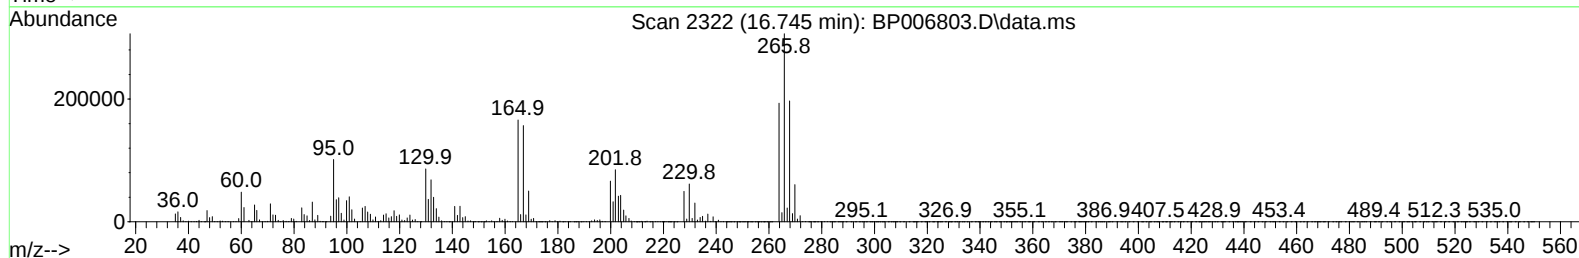


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006803.D
 Acq On : 20 Aug 2021 16:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 04:39:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 11:25:25 2021
 Response via : Initial Calibration

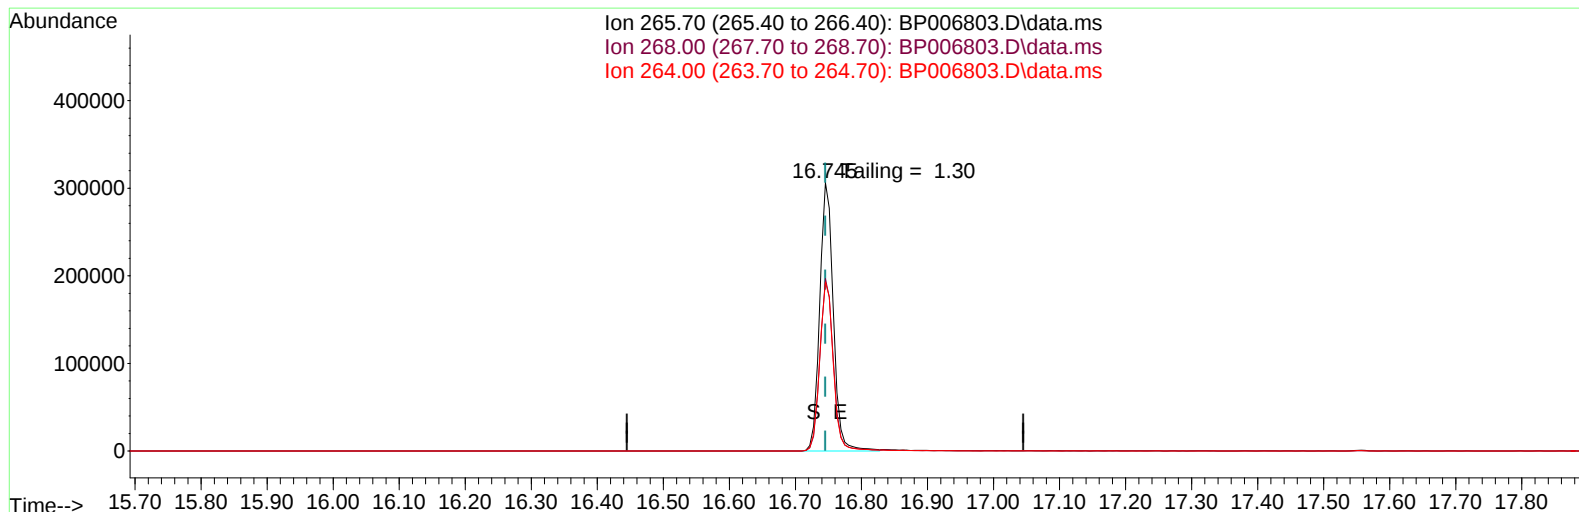

TIC: BP006803.D\data.ms

(70) Pentachlorophenol (C)




16.745min (+ 0.000) 1449037.93 ng

response 441698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.22
264.00	62.90	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006803.D
 Acq On : 20 Aug 2021 16:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 04:39:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 11:25:25 2021
 Response via : Initial Calibration

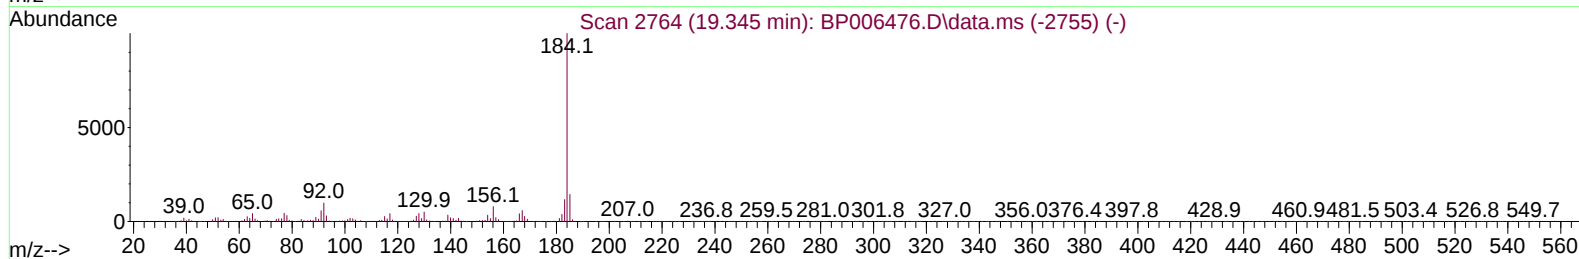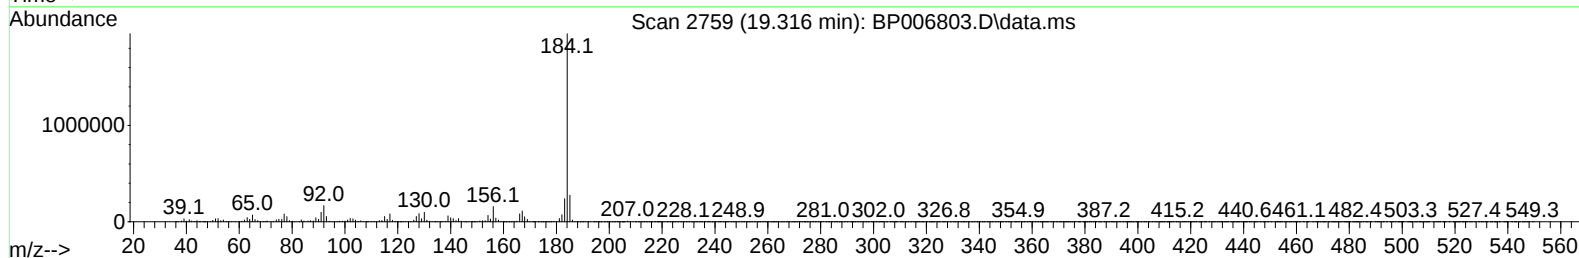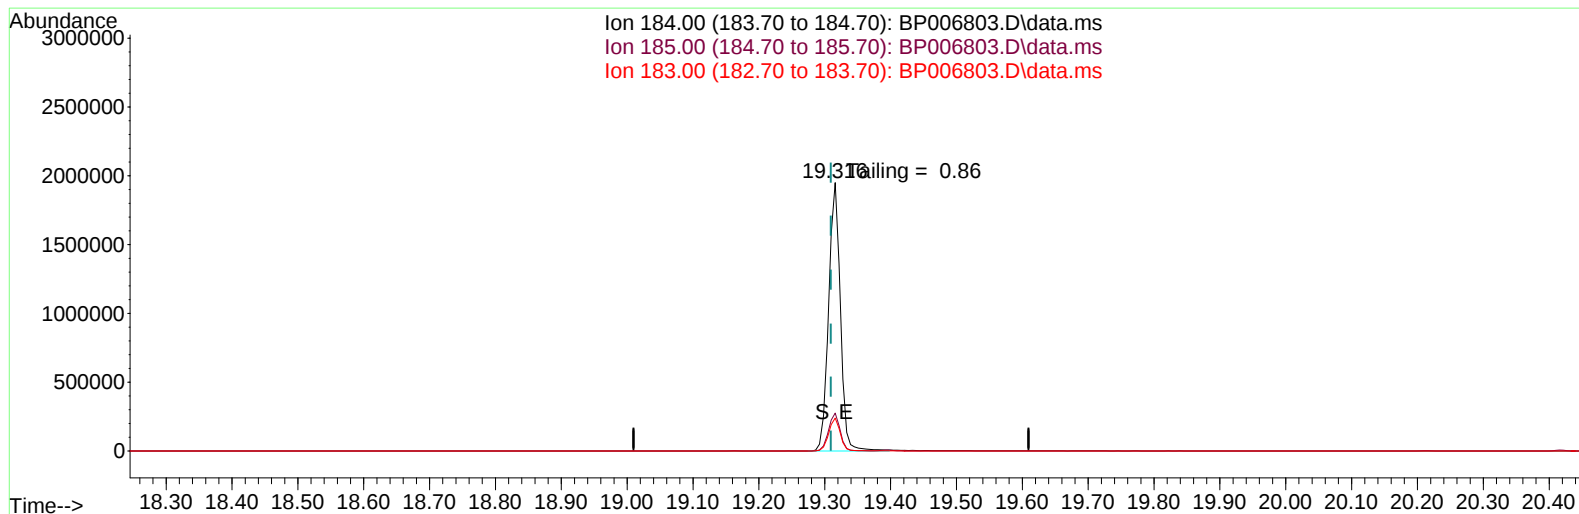

TIC: BP006803.D\data.ms

(77) Benzidine

19.316min (+ 0.006) 646139.55 ng

response 2425284

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.12
183.00	11.90	12.30
0.00	0.00	0.00