

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006806.D
 Acq On : 20 Aug 2021 18:37
 Operator : CG/JU
 Sample : M3426-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-10-0510

Quant Time: Aug 21 00:58:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 11:25:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	128317	20.000	ng	0.00
21) Naphthalene-d8	10.475	136	524588	20.000	ng	# 0.00
39) Acenaphthene-d10	14.334	164	293837	20.000	ng	0.00
64) Phenanthrene-d10	17.098	188	587762	20.000	ng	# 0.00
76) Chrysene-d12	21.204	240	601294	20.000	ng	# 0.00
86) Perylene-d12	23.515	264	736950	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.299	112	1204432	144.169	ng	0.00
7) Phenol-d6	6.881	99	1478970	124.624	ng	0.00
23) Nitrobenzene-d5	8.851	82	996079	87.643	ng	0.00
42) 2,4,6-Tribromophenol	15.833	330	518438	168.822	ng	0.00
45) 2-Fluorobiphenyl	12.957	172	1753799	89.298	ng	0.00
79) Terphenyl-d14	19.680	244	2352650	78.401	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006806.D
Acq On : 20 Aug 2021 18:37
Operator : CG/JU
Sample : M3426-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510

Quant Time: Aug 21 00:58:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 11:25:25 2021
Response via : Initial Calibration




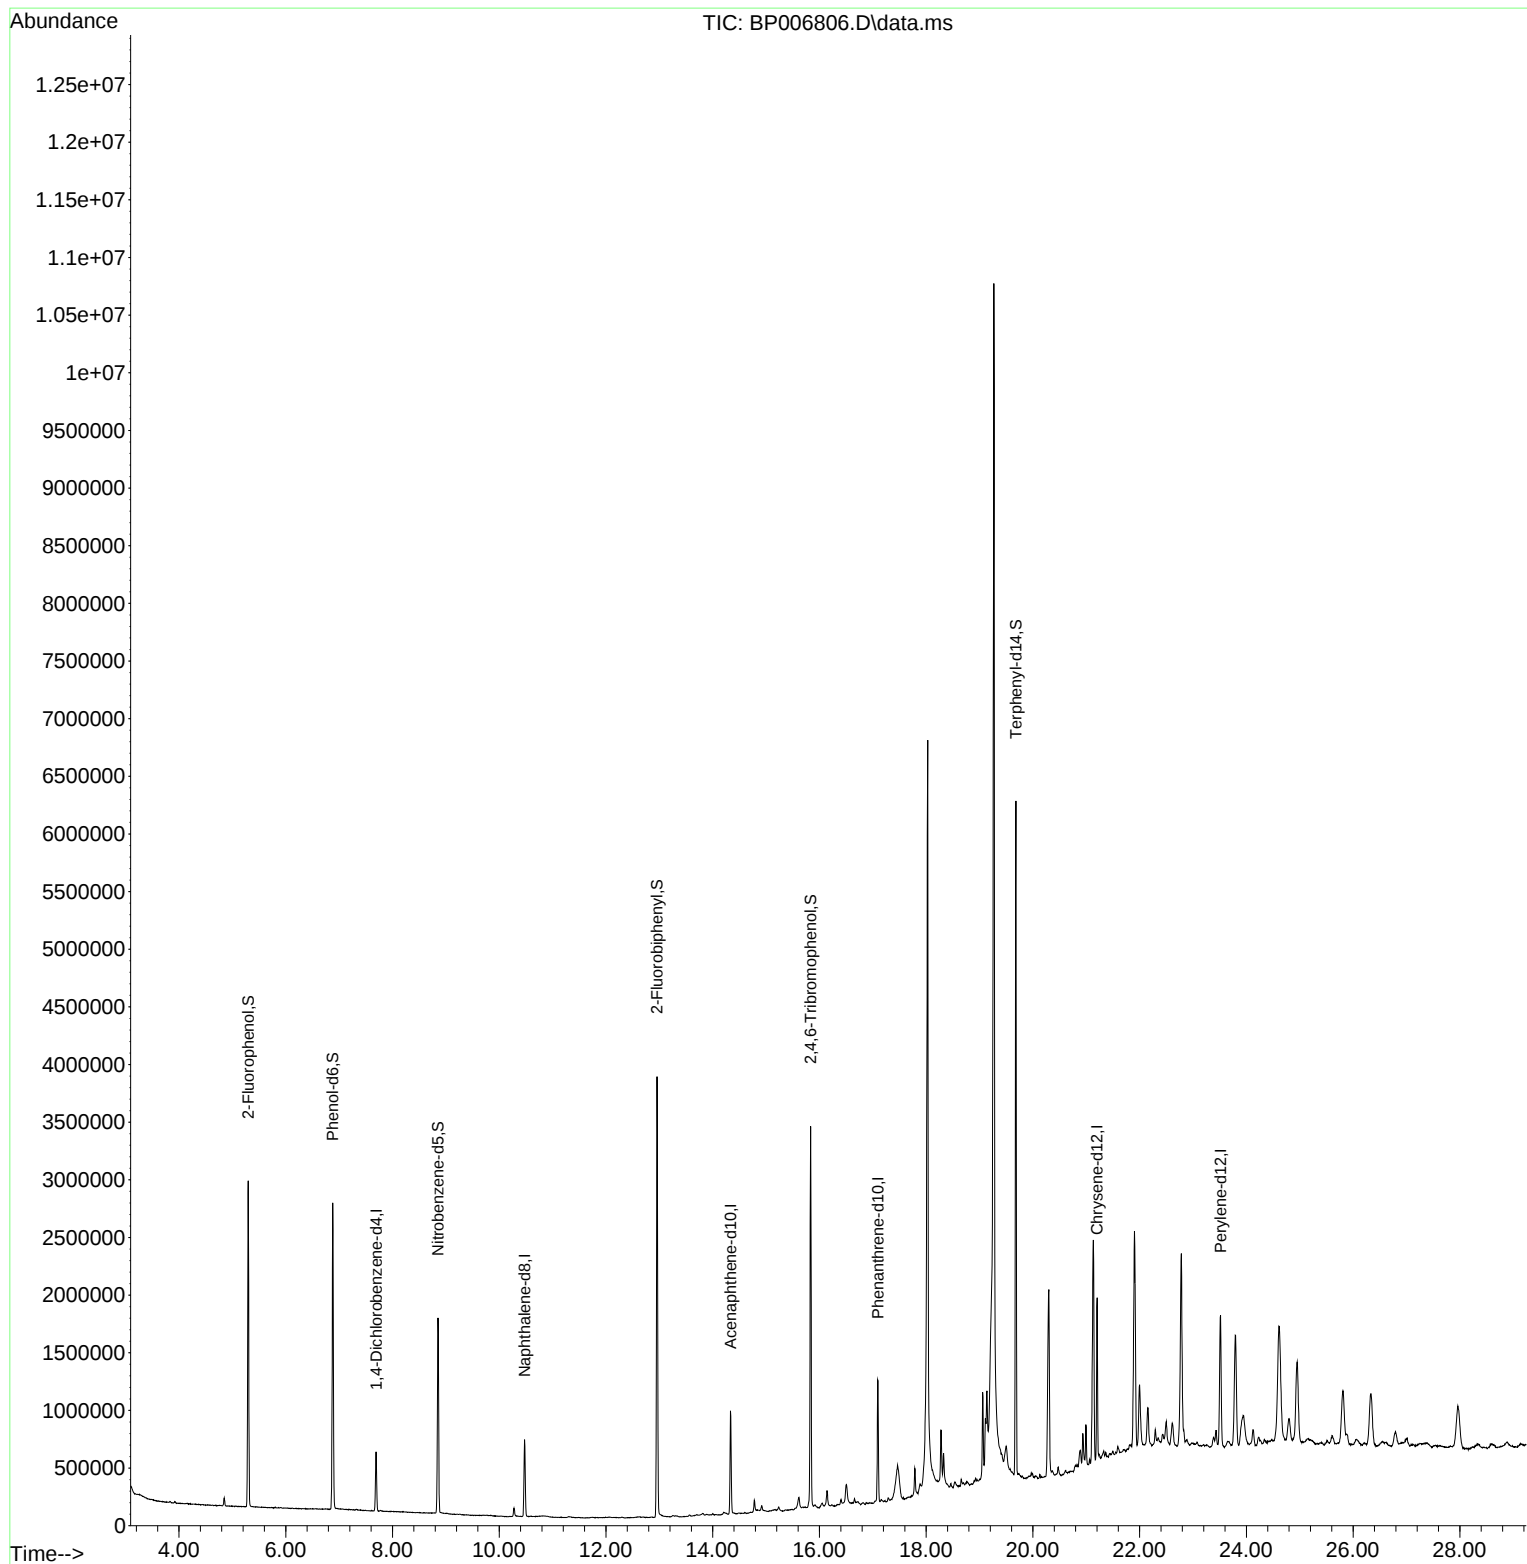


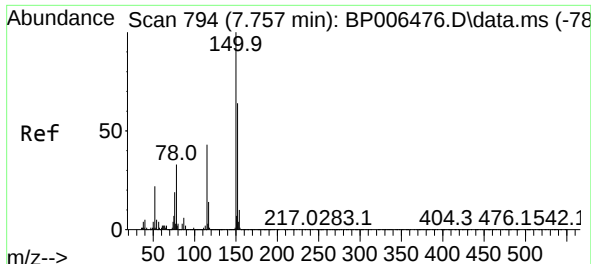

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.693 min Scan# 783
Delta R.T. -0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37




Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510


Tgt Ion:152 Resp: 128317
Ion Ratio Lower Upper
152 100
150 157.5 125.6 188.4
115 66.6 48.5 72.7

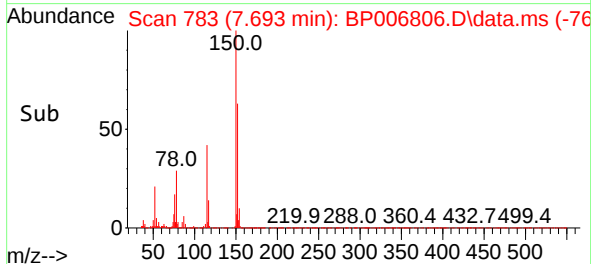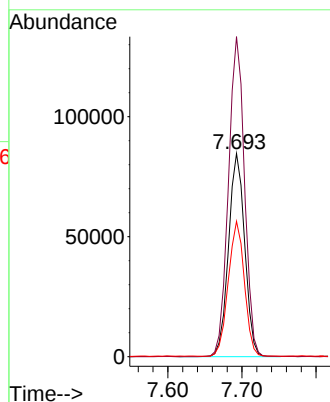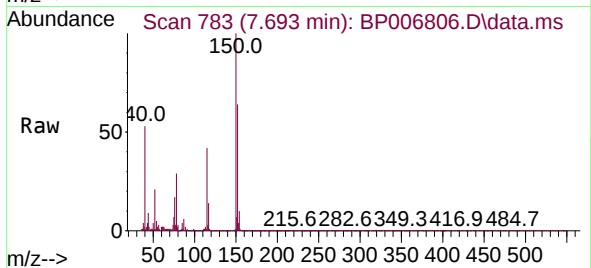

#5
2-Fluorophenol
Concen: 144.169 ng
RT: 5.299 min Scan# 376
Delta R.T. 0.006 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37

Tgt Ion:112 Resp: 1204432
Ion Ratio Lower Upper
112 100
64 55.4 41.4 62.2
63 29.4 23.8 35.8


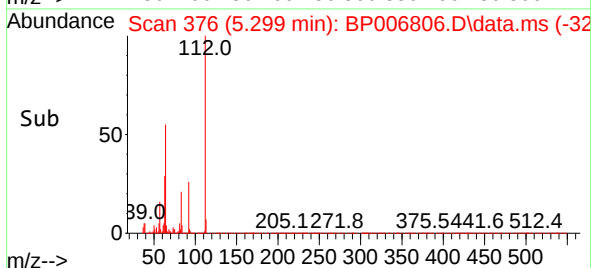
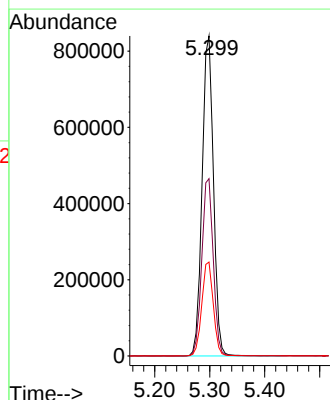
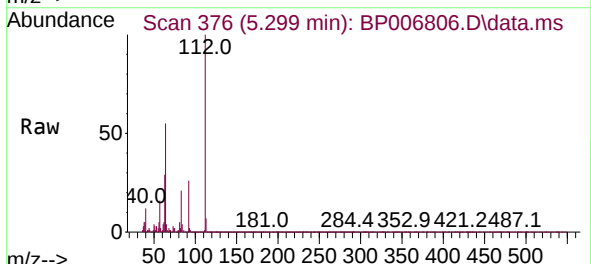




#7
Phenol-d6
Concen: 124.624 ng
RT: 6.881 min Scan# 645
Delta R.T. 0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37




Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510


Tgt Ion: 99 Resp: 1478970
Ion Ratio Lower Upper
99 100
42 15.7 13.4 20.0
71 37.3 30.6 46.0

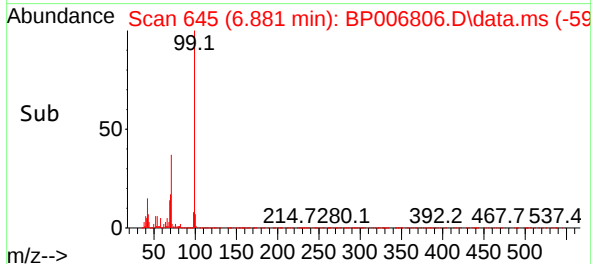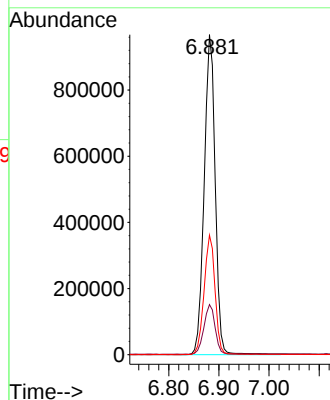

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.475 min Scan# 1256
Delta R.T. 0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37

Tgt Ion: 136 Resp: 524588
Ion Ratio Lower Upper
136 100
137 11.0 8.6 12.8
54 7.5 4.6 6.8#
68 6.5 3.6 5.4#


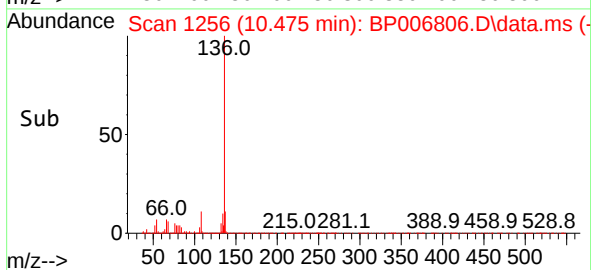
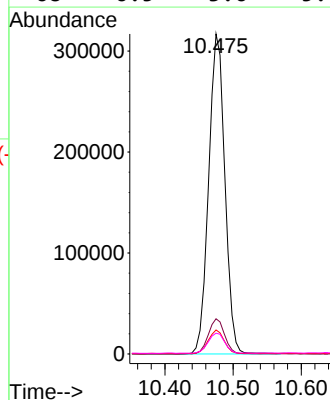
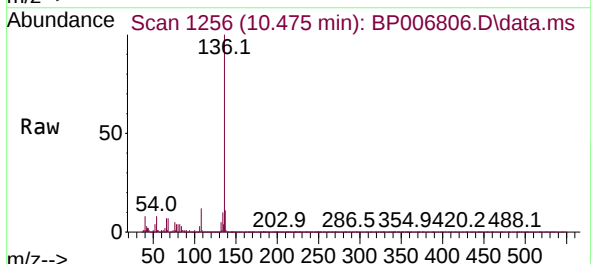


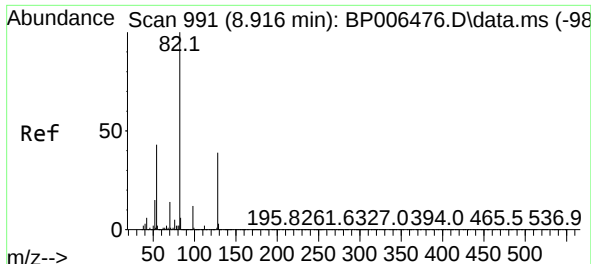

#23
Nitrobenzene-d5
Concen: 87.643 ng
RT: 8.851 min Scan# 980
Delta R.T. -0.006 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37




Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510

Tgt Ion:	82	Resp:	996079
Ion	Ratio	Lower	Upper
82	100		
128	40.2	35.7	53.5
54	42.2	35.0	52.4

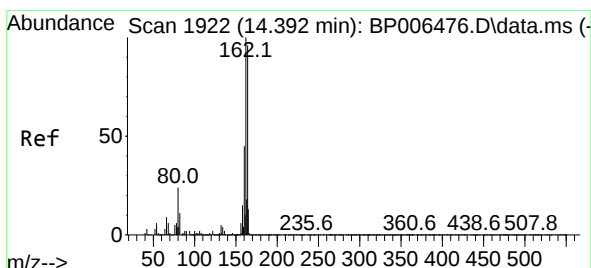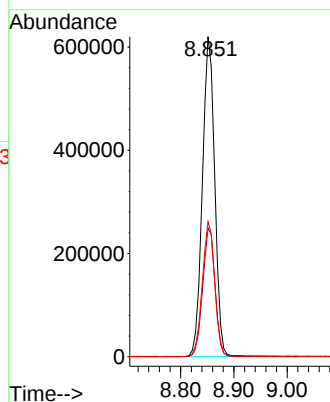

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.334 min Scan# 1912
Delta R.T. -0.006 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37

Tgt Ion:	164	Resp:	293837
Ion	Ratio	Lower	Upper
164	100		
162	100.2	80.2	120.2
160	45.8	34.5	51.7


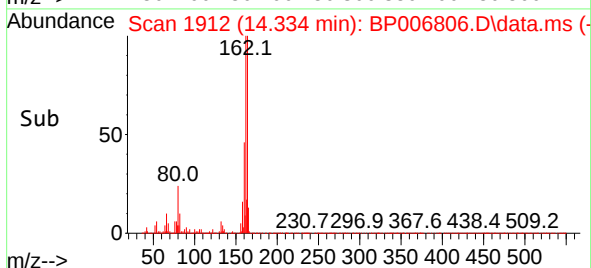
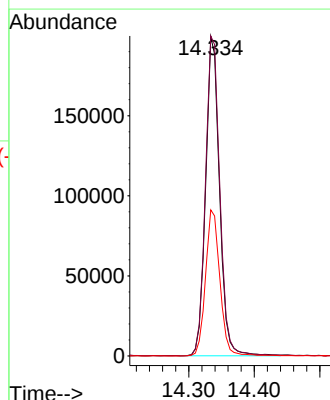
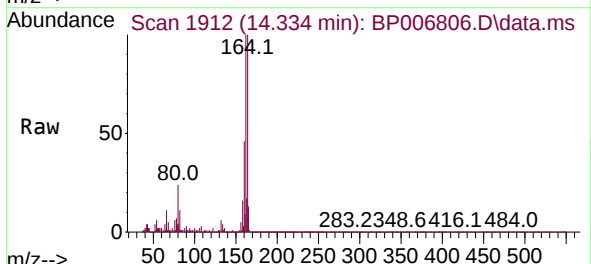




#42
2,4,6-Tribromophenol
Concen: 168.822 ng
RT: 15.833 min Scan# 2167
Delta R.T. -0.006 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37




Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510

Tgt Ion:330 Resp: 518438
Ion Ratio Lower Upper
330 100
332 96.4 77.8 116.8
141 46.9 25.4 38.2#

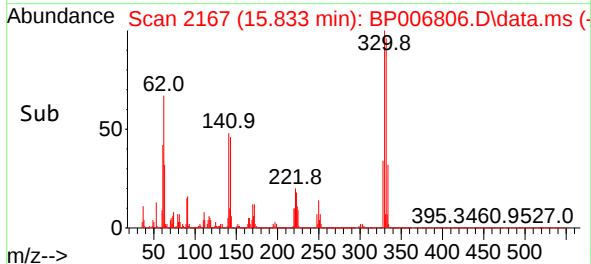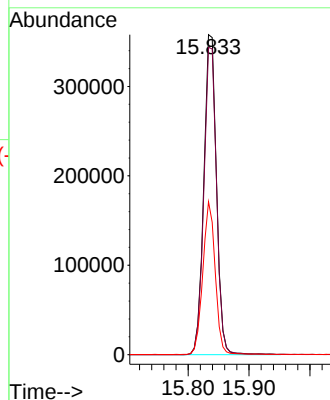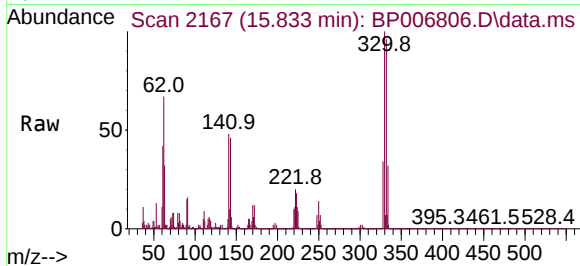

#45
2-Fluorobiphenyl
Concen: 89.298 ng
RT: 12.957 min Scan# 1678
Delta R.T. 0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37

Tgt Ion:172 Resp: 1753799
Ion Ratio Lower Upper
172 100
171 35.5 27.9 41.9
170 23.9 18.6 27.8


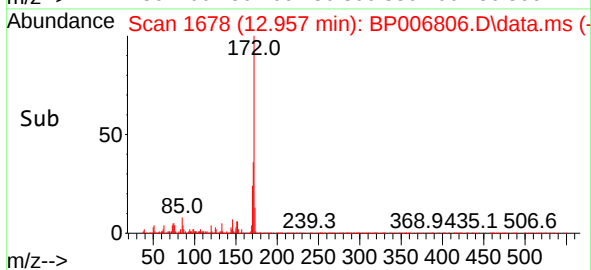
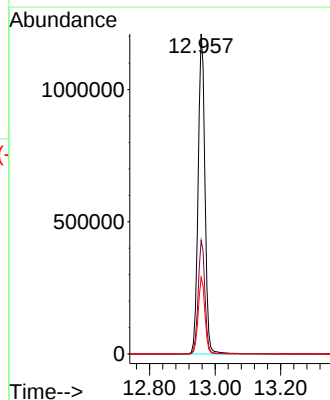
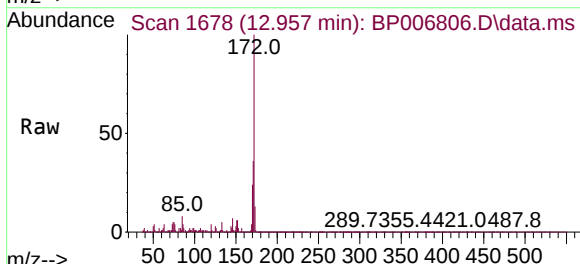




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.098 min Scan# 2382
Delta R.T. 0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37




Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510


Tgt Ion:188 Resp: 587762
Ion Ratio Lower Upper
188 100
94 10.7 5.6 8.4#
80 12.2 6.3 9.5#

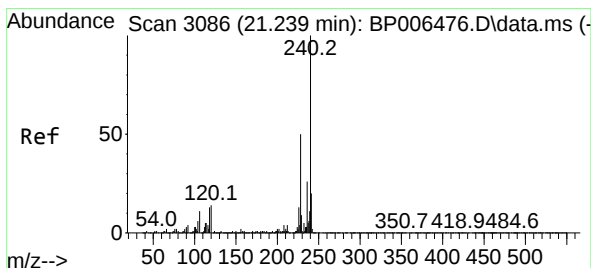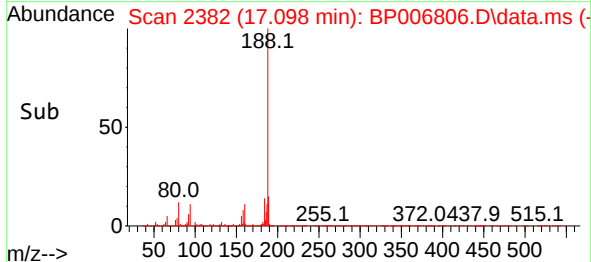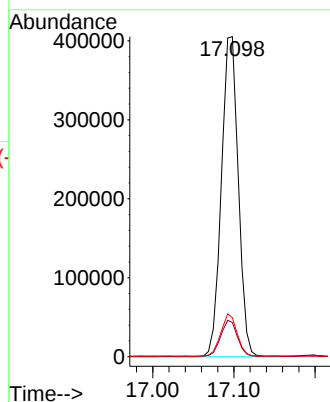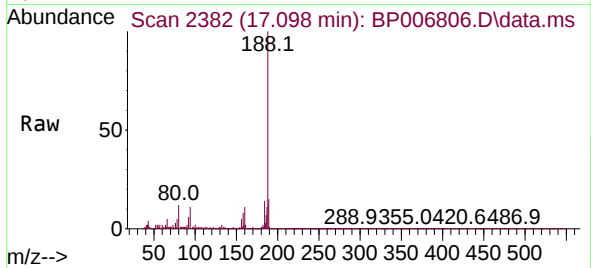

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.204 min Scan# 3080
Delta R.T. 0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37

Tgt Ion:240 Resp: 601294
Ion Ratio Lower Upper
240 100
120 12.5 6.5 9.7#
236 26.5 20.6 31.0


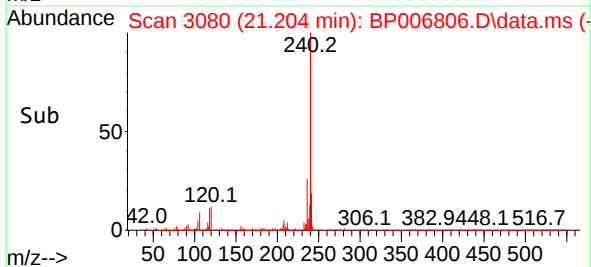
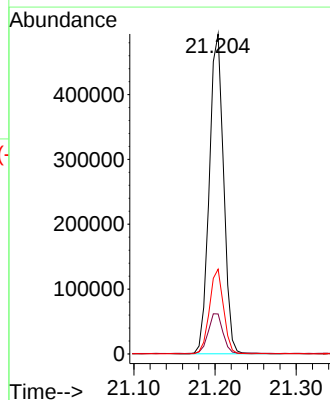
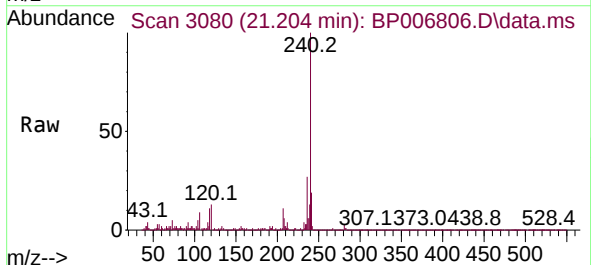




#79
Terphenyl-d14
Concen: 78.401 ng
RT: 19.680 min Scan# 2821
Delta R.T. 0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37

Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510

Tgt Ion:244 Resp: 2352650
Ion Ratio Lower Upper
244 100
212 7.7 6.0 9.0
122 12.0 7.1 10.7#

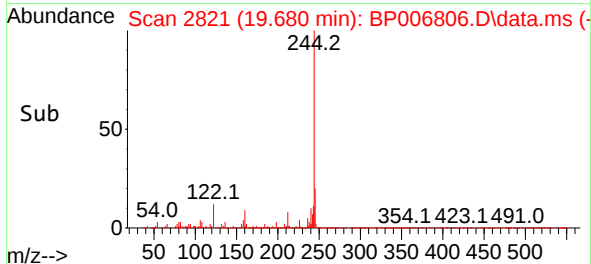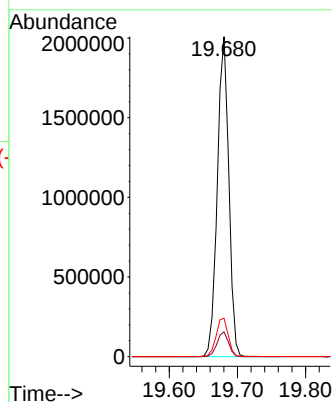

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.515 min Scan# 3473
Delta R.T. 0.000 min
Lab File: BP006806.D
Acq: 20 Aug 2021 18:37

Tgt Ion:264 Resp: 736950
Ion Ratio Lower Upper
264 100
260 24.7 18.6 28.0
265 22.1 17.6 26.4

