

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006795.D
 Acq On : 20 Aug 2021 11:59
 Operator : CG/JU
 Sample : PB138490BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB138490BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.846	296	299	310	rVB	75507	112276	1.11%	0.248%
2	5.299	370	376	388	rBV	3463288	4832634	47.74%	10.678%
3	6.881	638	645	663	rVB	3129043	4858786	48.00%	10.736%
4	7.693	777	783	790	rVB	599067	923543	9.12%	2.041%
5	8.852	973	980	989	rBV	2004311	3263839	32.24%	7.212%
6	10.475	1249	1256	1264	rBV	790817	1299799	12.84%	2.872%
7	12.957	1670	1678	1694	rBV	4652607	6818725	67.36%	15.067%
8	14.340	1906	1913	1929	rBV	1079363	1652727	16.33%	3.652%
9	15.834	2159	2167	2189	rBV	3589776	5304369	52.40%	11.721%
10	17.098	2375	2382	2394	rBV	1332849	1929003	19.06%	4.262%
11	19.681	2815	2821	2826	rBV	8834490	10122462	100.00%	22.367%
12	21.204	3075	3080	3086	rBV	1620452	2042203	20.17%	4.513%
13	23.516	3467	3473	3483	rVB2	1099121	2096046	20.71%	4.631%




Sum of corrected areas: 45256412

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006795.D
Acq On : 20 Aug 2021 11:59
Operator : CG/JU
Sample : PB138490BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138490BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

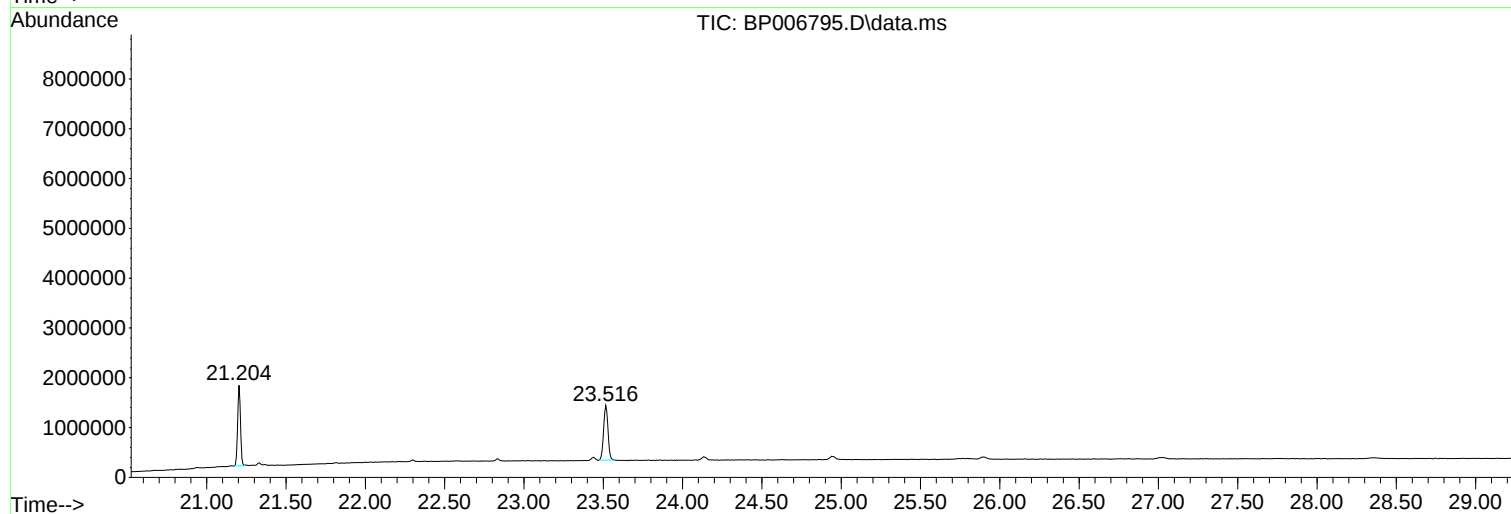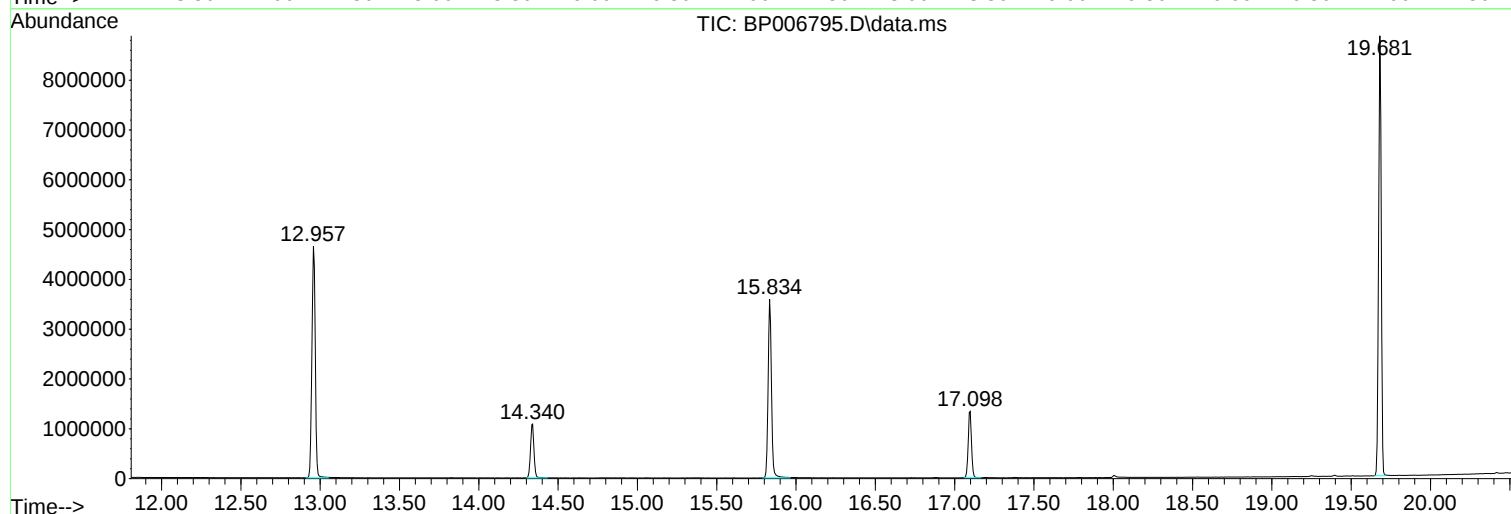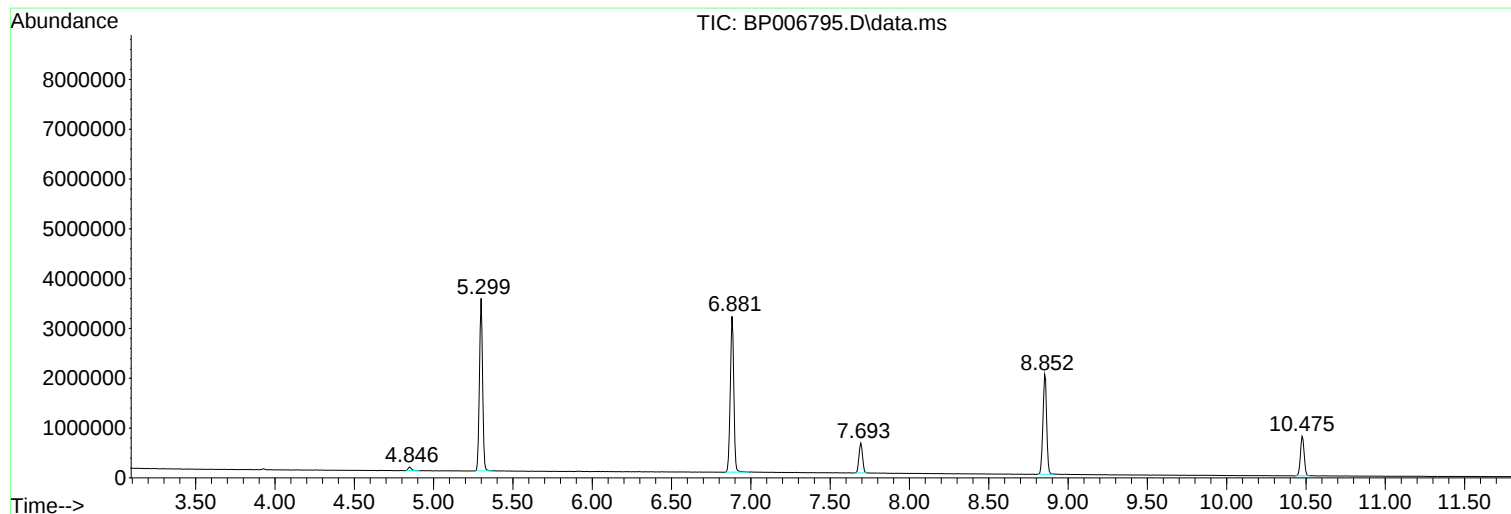

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006795.D
Acq On : 20 Aug 2021 11:59
Operator : CG/JU
Sample : PB138490BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138490BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006795.D
Acq On : 20 Aug 2021 11:59
Operator : CG/JU
Sample : PB138490BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138490BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------