

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006796.D
 Acq On : 20 Aug 2021 12:42
 Operator : CG/JU
 Sample : M3434-31
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-12-FD-03

Integration Parameters: rteint.p

Integrator: RTE

Smothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	370	376	385	rBV	4898931	7036157	27.36%	5.351%
2	6.887	638	646	655	rBV	4647858	7470497	29.05%	5.682%
3	7.693	777	783	794	rVB	814833	1284681	5.00%	0.977%
4	8.858	973	981	989	rBV	3054967	4941674	19.21%	3.758%
5	10.281	1216	1223	1231	rBV	165408	287119	1.12%	0.218%
6	10.481	1249	1257	1264	rBV	1138783	1903908	7.40%	1.448%
7	12.963	1671	1679	1688	rBV	6049976	8689204	33.79%	6.609%
8	14.340	1906	1913	1921	rBV	1652421	2456648	9.55%	1.868%
9	15.645	2123	2135	2141	rBV2	122732	469357	1.82%	0.357%
10	15.840	2158	2168	2177	rBV	5394629	7478490	29.08%	5.688%
11	16.510	2276	2282	2294	rVB5	193550	466459	1.81%	0.355%
12	17.098	2377	2382	2386	rBV	1858300	2360895	9.18%	1.796%
13	17.210	2386	2401	2420	rVB	3165446	16943223	65.88%	12.887%
14	17.440	2421	2440	2441	rBV	8201606	25719073	100.00%	19.561%
15	17.675	2468	2480	2495	rBV	928459	2850818	11.08%	2.168%
16	18.022	2533	2539	2558	rVB	3546189	5593572	21.75%	4.254%
17	18.281	2579	2583	2587	rBV	406293	580344	2.26%	0.441%
18	18.328	2587	2591	2600	rVB	434179	754569	2.93%	0.574%
19	18.686	2645	2652	2658	rBV2	150441	391677	1.52%	0.298%
20	19.122	2721	2726	2735	rBV2	687251	1707901	6.64%	1.299%
21	19.263	2742	2750	2771	rVB	5343966	8511956	33.10%	6.474%
22	19.475	2782	2786	2790	rVB	422719	530803	2.06%	0.404%
23	19.681	2816	2821	2826	rBV	6927262	8851994	34.42%	6.733%
24	20.169	2899	2904	2909	rVB	272061	490951	1.91%	0.373%
25	20.539	2963	2967	2976	rVB2	406164	767129	2.98%	0.583%
26	20.704	2990	2995	3004	rVB3	278473	642467	2.50%	0.489%
27	20.939	3031	3035	3041	rBV3	631290	894750	3.48%	0.681%
28	20.998	3042	3045	3051	rVB	234041	318663	1.24%	0.242%
29	21.204	3075	3080	3083	rBV	1736445	2421061	9.41%	1.841%
30	21.233	3083	3085	3092	rVB2	839235	1146532	4.46%	0.872%
31	21.822	3181	3185	3186	rBV	213337	280924	1.09%	0.214%
32	21.845	3186	3189	3195	rVV	385099	570377	2.22%	0.434%
33	21.916	3196	3201	3207	rVV	633603	1068130	4.15%	0.812%
34	22.692	3328	3333	3340	rVB	687401	1249881	4.86%	0.951%
35	23.522	3467	3474	3489	rVB3	1180075	3466495	13.48%	2.637%
36	24.563	3646	3651	3660	rVB	383586	881820	3.43%	0.671%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006796.D
Acq On : 20 Aug 2021 12:42
Operator : CG/JU
Sample : M3434-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-FD-03

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 131480199

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006796.D
Acq On : 20 Aug 2021 12:42
Operator : CG/JU
Sample : M3434-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-FD-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

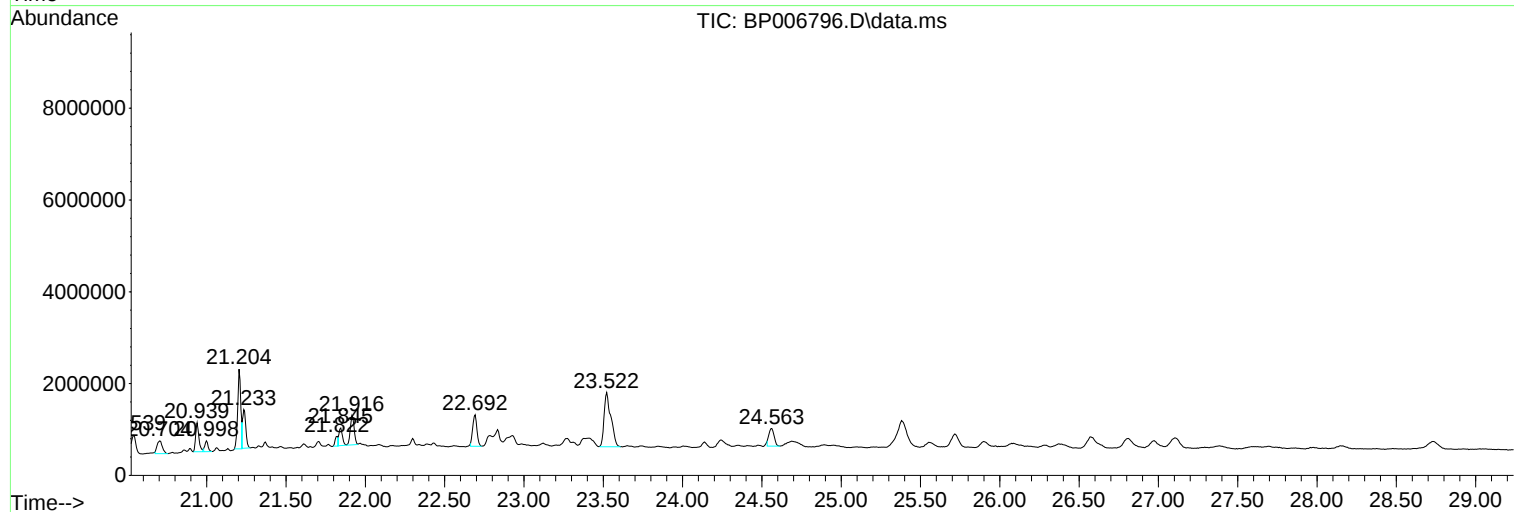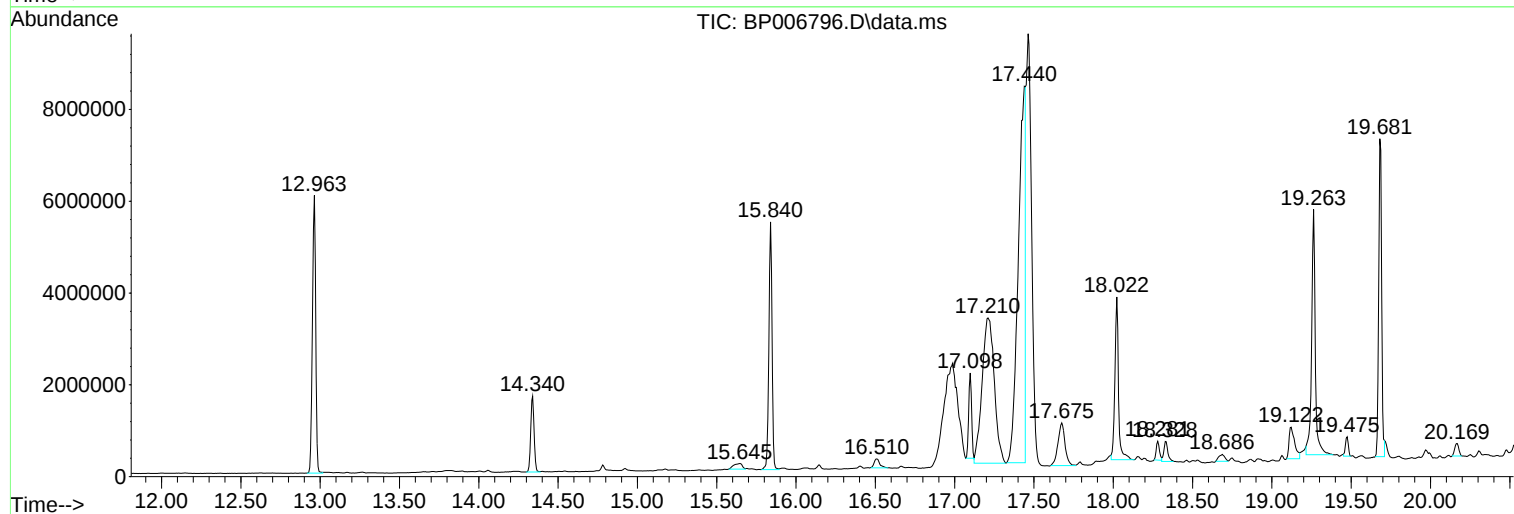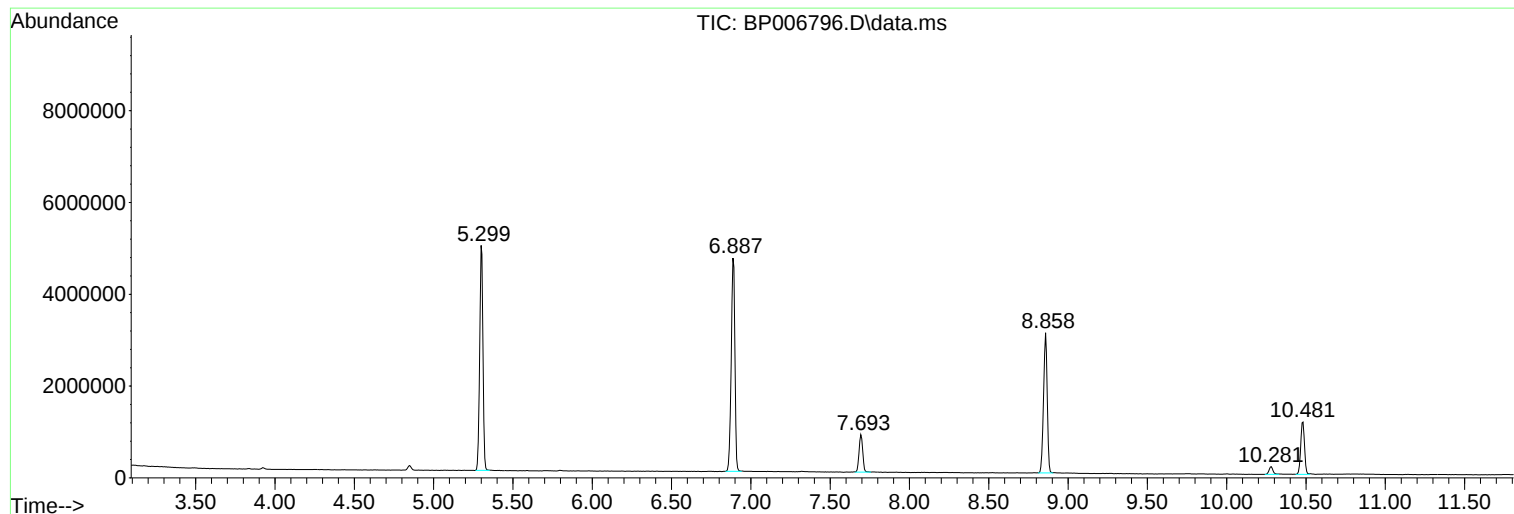

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006796.D
Acq On : 20 Aug 2021 12:42
Operator : CG/JU
Sample : M3434-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-FD-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006796.D
Acq On : 20 Aug 2021 12:42
Operator : CG/JU
Sample : M3434-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-FD-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------