

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006806.D
 Acq On : 20 Aug 2021 18:37
 Operator : CG/JU
 Sample : M3426-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-10-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	370	376	387	rVB	2827316	4066358	16.68%	3.873%
2	6.881	638	645	655	rBV	2656679	4094807	16.80%	3.900%
3	7.693	777	783	790	rVB	514936	780777	3.20%	0.744%
4	8.851	973	980	988	rBV	1692530	2715452	11.14%	2.586%
5	10.475	1249	1256	1264	rBV	666559	1093552	4.49%	1.042%
6	12.957	1671	1678	1688	rBV	3822195	5451533	22.37%	5.192%
7	14.334	1906	1912	1920	rBV	896117	1341447	5.50%	1.278%
8	15.833	2158	2167	2176	rBV	3300317	4756663	19.52%	4.530%
9	16.504	2276	2281	2292	rVB3	160314	387719	1.59%	0.369%
10	17.092	2376	2381	2388	rVB	1056843	1544648	6.34%	1.471%
11	17.786	2495	2499	2507	rBV	217612	298287	1.22%	0.284%
12	18.027	2524	2540	2554	rBV	6426511	12930222	53.05%	12.315%
13	18.275	2578	2582	2587	rBV	433693	664327	2.73%	0.633%
14	18.327	2588	2591	2600	rVB	265100	419203	1.72%	0.399%
15	19.057	2711	2715	2720	rBV	718729	964036	3.96%	0.918%
16	19.110	2720	2724	2726	rVV2	473345	693782	2.85%	0.661%
17	19.139	2726	2729	2733	rVV	702432	1266207	5.19%	1.206%
18	19.269	2735	2751	2781	rVB	10250585	24374352	100.00%	23.215%
19	19.680	2815	2821	2827	rBV	5844357	6995604	28.70%	6.663%
20	20.298	2918	2926	2934	rBV	1584228	3347155	13.73%	3.188%
21	20.933	3031	3034	3041	rBV2	253274	404888	1.66%	0.386%
22	20.992	3041	3044	3051	rVB	349031	432164	1.77%	0.412%
23	21.133	3060	3068	3074	rBV	1910388	3974240	16.31%	3.785%
24	21.204	3075	3080	3084	rBV	1402286	1754508	7.20%	1.671%
25	21.904	3191	3199	3207	rBV	1861964	4297877	17.63%	4.093%
26	21.998	3210	3215	3225	rVB	518981	1203280	4.94%	1.146%
27	22.780	3341	3348	3360	rVB	1635252	3851704	15.80%	3.668%
28	23.515	3466	3473	3483	rVB2	1142074	2330368	9.56%	2.220%
29	23.792	3514	3520	3531	rVB	956620	2476239	10.16%	2.358%
30	24.609	3652	3659	3678	rVB3	987546	3888479	15.95%	3.704%
31	24.951	3710	3717	3729	rVB2	693871	2194129	9.00%	2.090%




Sum of corrected areas: 104994007

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006806.D
Acq On : 20 Aug 2021 18:37
Operator : CG/JU
Sample : M3426-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

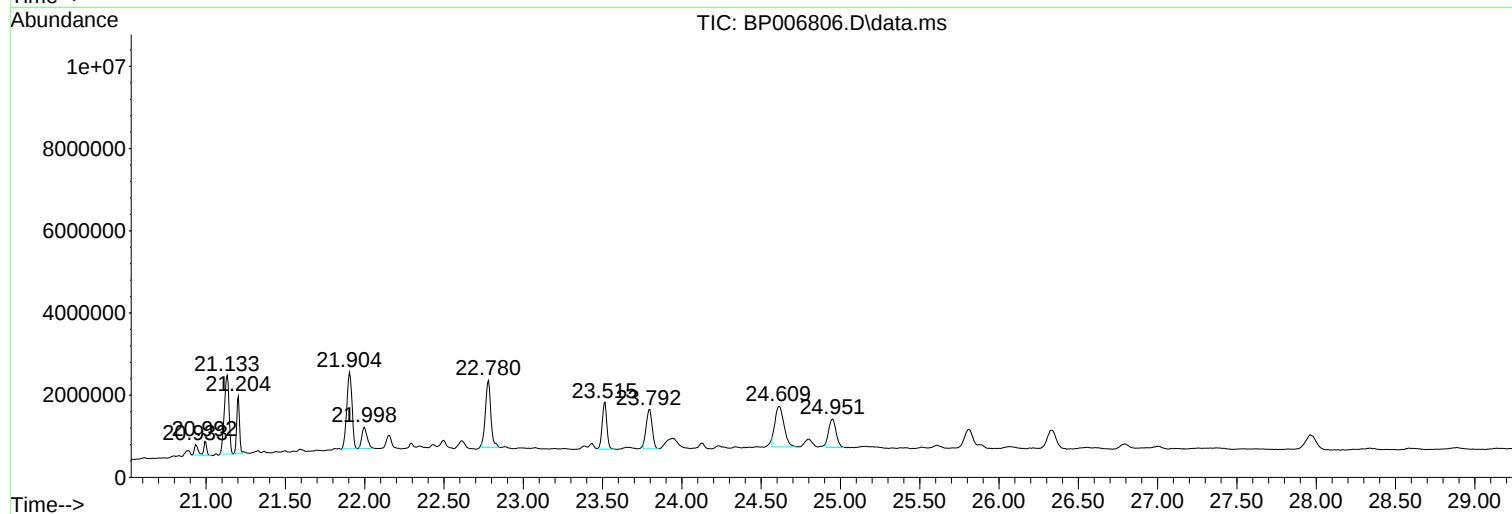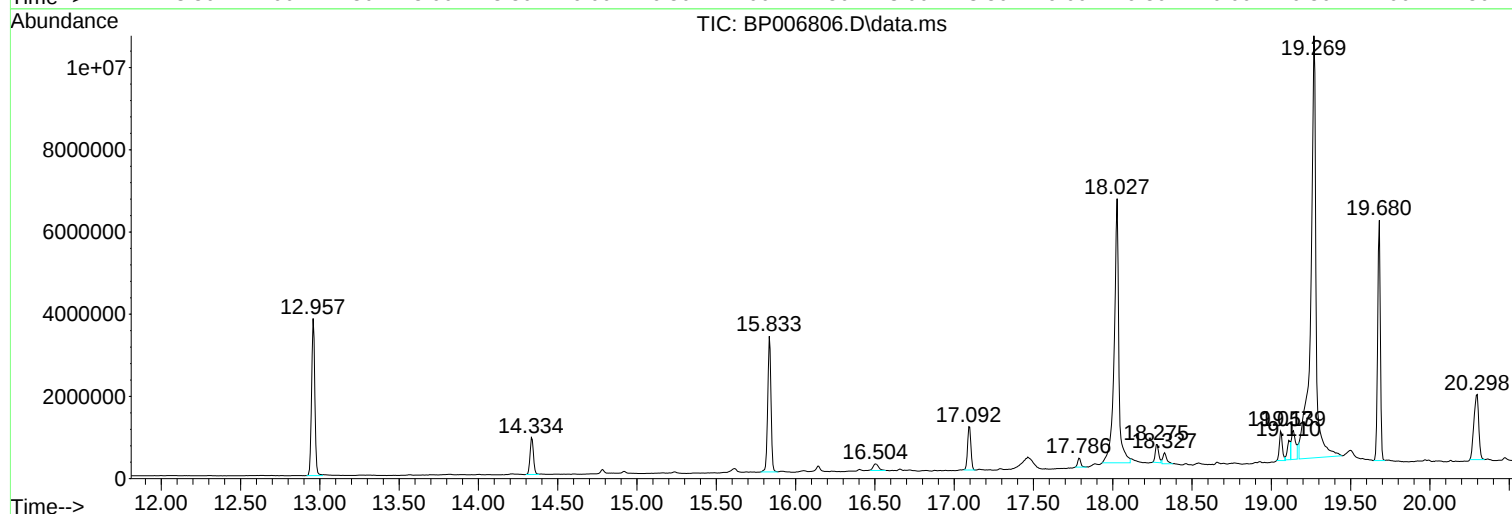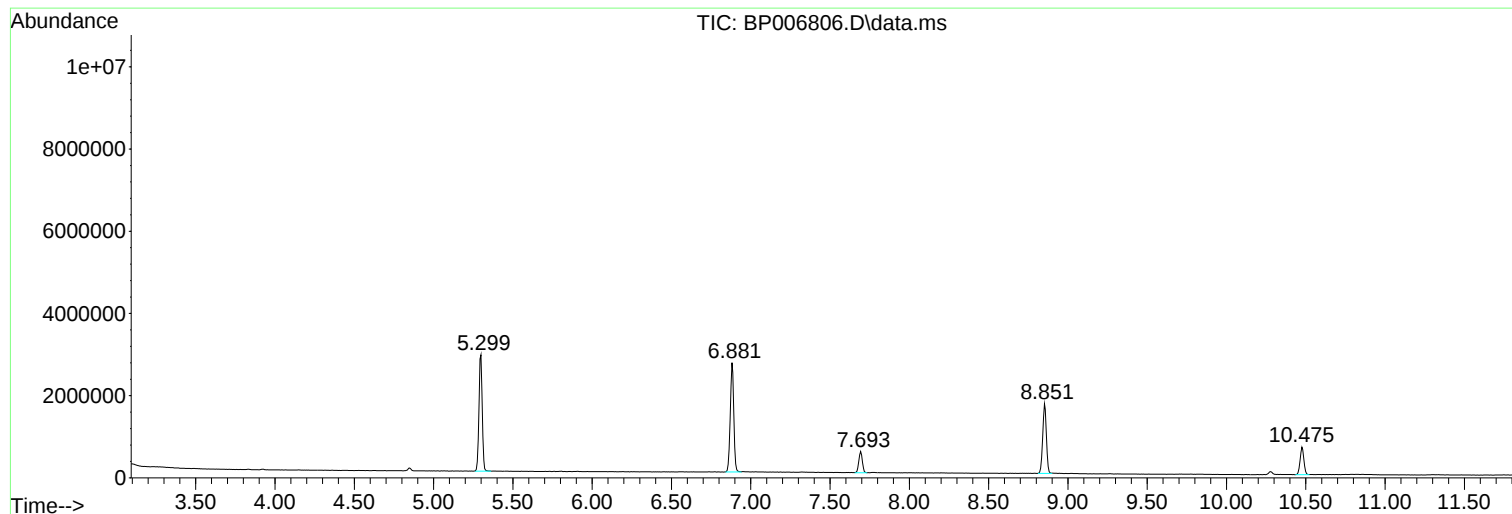

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006806.D
Acq On : 20 Aug 2021 18:37
Operator : CG/JU
Sample : M3426-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006806.D
Acq On : 20 Aug 2021 18:37
Operator : CG/JU
Sample : M3426-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-10-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------