

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006810.D
 Acq On : 20 Aug 2021 20:54
 Operator : CG/JU
 Sample : M3463-27
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-23-0204

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	327	330	335	rVB	56846	75370	1.46%	0.192%
2	5.293	369	375	388	rBV	3137671	4443884	86.15%	11.322%
3	6.881	638	645	659	rBV	2912458	4525904	87.74%	11.531%
4	7.693	777	783	790	rVB	562407	870574	16.88%	2.218%
5	8.852	973	980	987	rBV	1867831	3002920	58.21%	7.651%
6	10.269	1215	1221	1238	rBV	382222	714425	13.85%	1.820%
7	10.475	1249	1256	1269	rVB	779149	1274435	24.71%	3.247%
8	12.957	1670	1678	1693	rBV	3417844	5105189	98.97%	13.007%
9	14.334	1905	1912	1928	rBV	1014680	1528096	29.62%	3.893%
10	15.834	2157	2167	2189	rBV	2918651	4242621	82.25%	10.809%
11	17.092	2375	2381	2389	rBV	1211961	1684812	32.66%	4.292%
12	17.786	2495	2499	2504	rBV	50478	61725	1.20%	0.157%
13	18.004	2531	2536	2552	rBV	253456	447885	8.68%	1.141%
14	19.245	2743	2747	2758	rBV	133463	222212	4.31%	0.566%
15	19.675	2815	2820	2828	rBV	4354401	5158330	100.00%	13.142%
16	20.927	3030	3033	3041	rBV	373492	593133	11.50%	1.511%
17	21.198	3075	3079	3084	rBV	1427973	1698353	32.92%	4.327%
18	21.839	3180	3188	3201	rBV3	346366	887180	17.20%	2.260%
19	22.880	3361	3365	3374	rVB2	255312	499997	9.69%	1.274%
20	23.510	3465	3472	3478	rBV2	1096221	2213668	42.91%	5.640%




Sum of corrected areas: 39250713

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006810.D
Acq On : 20 Aug 2021 20:54
Operator : CG/JU
Sample : M3463-27
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-23-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

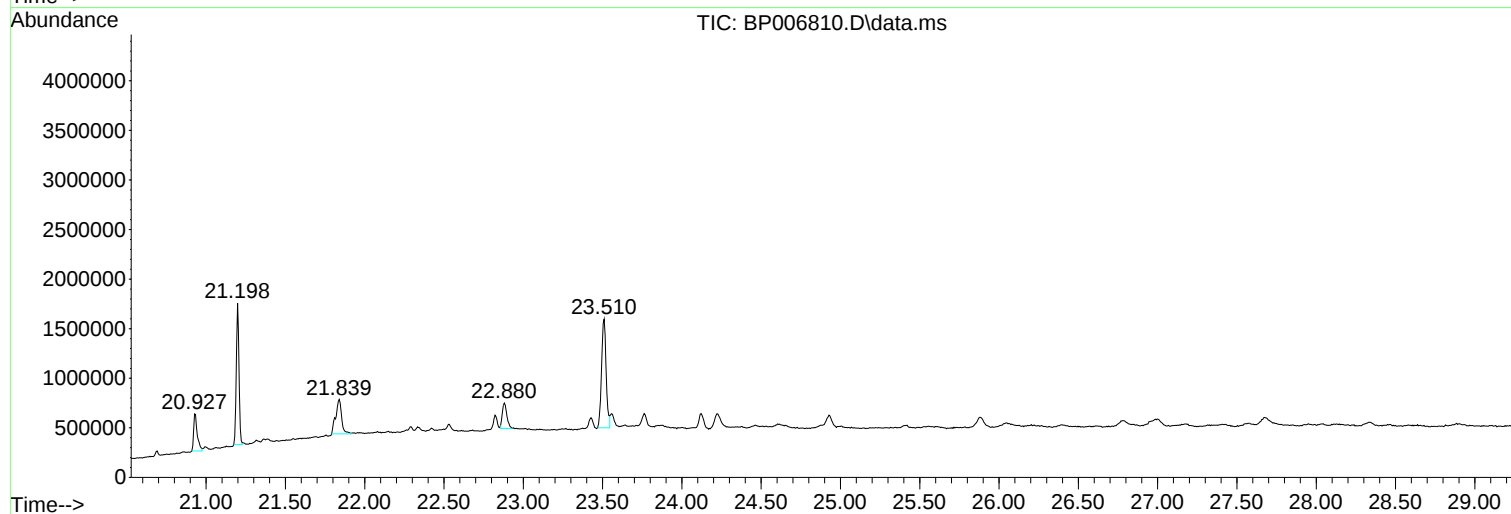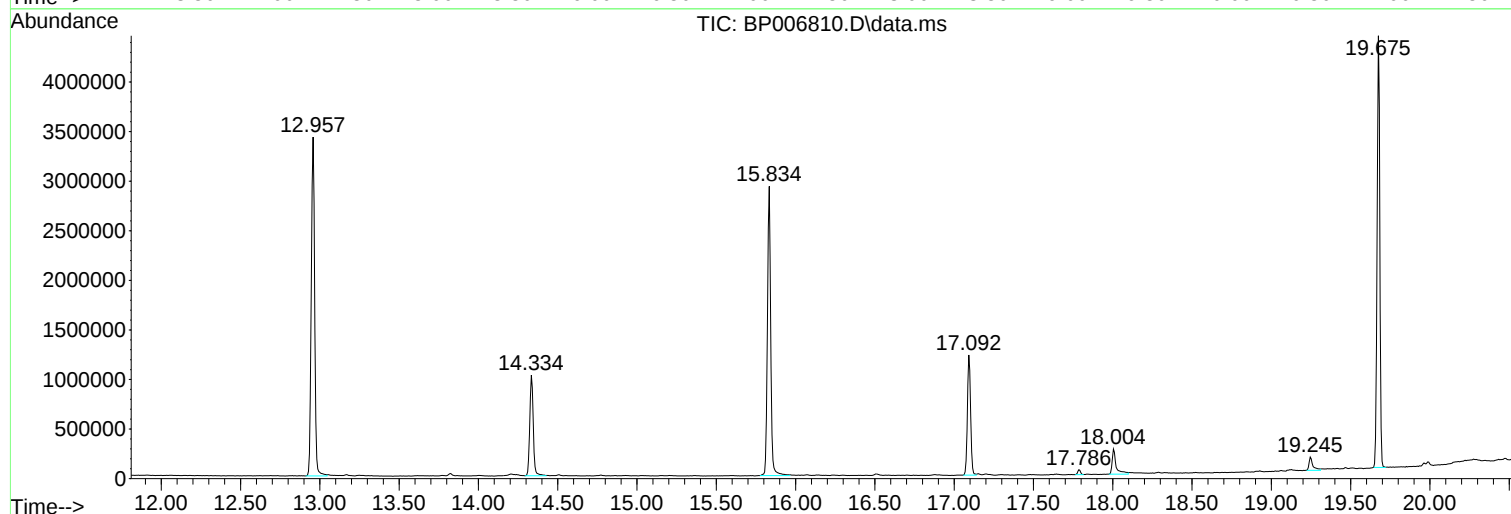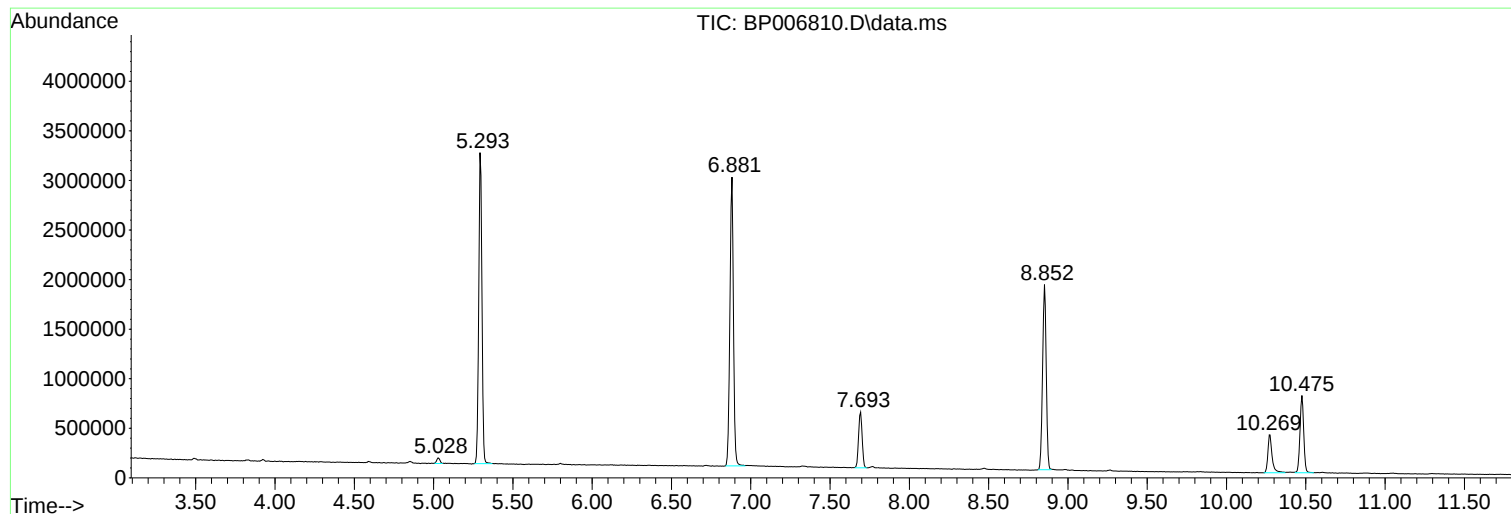

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006810.D
Acq On : 20 Aug 2021 20:54
Operator : CG/JU
Sample : M3463-27
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-23-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006810.D
Acq On : 20 Aug 2021 20:54
Operator : CG/JU
Sample : M3463-27
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-23-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------