

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006811.D
 Acq On : 20 Aug 2021 21:28
 Operator : CG/JU
 Sample : M3434-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.846	295	299	304	rVB2	59461	82753	1.55%	0.125%
2	5.293	369	375	384	rBV	1936024	2682282	50.29%	4.061%
3	6.252	534	538	543	rBV	120543	176971	3.32%	0.268%
4	6.364	553	557	562	rVB	108705	163569	3.07%	0.248%
5	6.593	589	596	601	rVB4	68821	152811	2.86%	0.231%
6	6.828	632	636	638	rVV	101150	158595	2.97%	0.240%
7	6.875	638	644	656	rVB	1716673	2816809	52.81%	4.265%
8	7.140	681	689	691	rBV6	72963	160615	3.01%	0.243%
9	7.175	691	695	703	rVV3	124968	298252	5.59%	0.452%
10	7.246	704	707	717	rVB4	75271	165020	3.09%	0.250%
11	7.405	730	734	740	rBV4	41965	85362	1.60%	0.129%
12	7.581	760	764	766	rBV3	56210	84203	1.58%	0.127%
13	7.693	773	783	788	rVB2	591736	1232828	23.11%	1.867%
14	7.758	788	794	799	rBV3	86640	168077	3.15%	0.254%
15	7.875	810	814	818	rVB3	126353	173303	3.25%	0.262%
16	7.969	822	830	837	rVV4	153737	383816	7.20%	0.581%
17	8.122	852	856	864	rBV4	78334	134480	2.52%	0.204%
18	8.234	864	875	880	rBV5	202810	531325	9.96%	0.804%
19	8.381	896	900	904	rVB3	56393	81525	1.53%	0.123%
20	8.758	959	964	966	rBV2	140237	211833	3.97%	0.321%
21	8.787	966	969	974	rVV3	181952	311511	5.84%	0.472%
22	8.852	974	980	993	rVB	1156194	2038076	38.21%	3.086%
23	8.999	999	1005	1007	rBV3	156673	265626	4.98%	0.402%
24	9.034	1007	1011	1017	rVB3	165874	339232	6.36%	0.514%
25	9.328	1056	1061	1066	rBV3	84630	146867	2.75%	0.222%
26	9.393	1067	1072	1077	rVB4	134530	238111	4.46%	0.361%
27	9.563	1095	1101	1104	rBV5	41962	87459	1.64%	0.132%
28	9.605	1104	1108	1112	rVV	168404	272122	5.10%	0.412%
29	9.652	1112	1116	1124	rVB2	154564	260877	4.89%	0.395%
30	9.928	1152	1163	1168	rBV7	50538	150153	2.81%	0.227%
31	10.069	1181	1187	1198	rVB10	71668	165681	3.11%	0.251%
32	10.205	1201	1210	1215	rBV6	39827	115917	2.17%	0.176%
33	10.269	1216	1221	1228	rBV2	116982	207799	3.90%	0.315%
34	10.475	1243	1256	1262	rBV	829396	1477760	27.70%	2.237%
35	10.646	1280	1285	1290	rVB	75858	118163	2.22%	0.179%
36	10.857	1314	1321	1328	rBV10	34064	98799	1.85%	0.150%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006811.D
 Acq On : 20 Aug 2021 21:28
 Operator : CG/JU
 Sample : M3434-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.063	1349	1356	1364	rBV2	75159	166279	3.12%	0.252%
38	11.175	1365	1375	1385	rVB5	80147	241800	4.53%	0.366%
39	11.510	1425	1432	1441	rBV2	125437	226426	4.24%	0.343%
40	11.757	1469	1474	1483	rBV2	50457	98086	1.84%	0.149%
41	11.875	1489	1494	1508	rVB	196500	396558	7.43%	0.600%
42	12.269	1554	1561	1571	rBV	177514	329753	6.18%	0.499%
43	12.610	1613	1619	1625	rVV4	44506	81971	1.54%	0.124%
44	12.746	1636	1642	1649	rBV2	54206	119659	2.24%	0.181%
45	12.875	1658	1664	1670	rBV	308573	465065	8.72%	0.704%
46	12.957	1670	1678	1684	rVV	2529529	3734670	70.01%	5.655%
47	13.016	1684	1688	1695	rVB3	53932	88626	1.66%	0.134%
48	13.169	1710	1714	1725	rVB4	63257	164744	3.09%	0.249%
49	13.828	1817	1826	1830	rVV2	338790	479721	8.99%	0.726%
50	13.869	1830	1833	1842	rVB4	50944	85518	1.60%	0.129%
51	13.946	1842	1846	1849	rBV3	53843	89704	1.68%	0.136%
52	13.987	1849	1853	1858	rVV	50040	87493	1.64%	0.132%
53	14.051	1858	1864	1871	rVV3	103437	194976	3.66%	0.295%
54	14.246	1892	1897	1902	rVB	227498	301100	5.64%	0.456%
55	14.334	1906	1912	1921	rVB	1074489	1641620	30.78%	2.486%
56	14.751	1978	1983	1989	rBV3	62842	107190	2.01%	0.162%
57	14.893	1999	2007	2012	rBV3	183171	592348	11.10%	0.897%
58	15.204	2056	2060	2070	rBV2	243639	357625	6.70%	0.541%
59	15.610	2123	2129	2134	rVB	167222	266628	5.00%	0.404%
60	15.834	2160	2167	2175	rBV	1977024	2926395	54.86%	4.431%
61	16.069	2201	2207	2209	rBV3	171748	284308	5.33%	0.430%
62	16.092	2209	2211	2216	rVB	222644	257230	4.82%	0.389%
63	16.657	2303	2307	2313	rVB	96238	136422	2.56%	0.207%
64	16.804	2327	2332	2337	rVV	162093	221819	4.16%	0.336%
65	16.863	2337	2342	2347	rVV	400380	534111	10.01%	0.809%
66	16.916	2347	2351	2362	rVB3	73126	141316	2.65%	0.214%
67	17.092	2375	2381	2386	rBV	1290362	1856148	34.80%	2.810%
68	17.134	2386	2388	2392	rVB	168305	194022	3.64%	0.294%
69	17.292	2410	2415	2421	rVB	445749	648330	12.15%	0.982%
70	17.375	2423	2429	2434	rBV	867343	1077175	20.19%	1.631%
71	17.457	2438	2443	2446	rBV3	89607	133294	2.50%	0.202%
72	17.504	2446	2451	2456	rVB3	56523	109266	2.05%	0.165%
73	17.710	2482	2486	2489	rBV2	107358	137139	2.57%	0.208%
74	17.822	2497	2505	2509	rBV2	202510	344779	6.46%	0.522%
75	17.881	2511	2515	2519	rVB	287942	365957	6.86%	0.554%
76	17.963	2524	2529	2533	rBV3	79673	183361	3.44%	0.278%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006811.D
 Acq On : 20 Aug 2021 21:28
 Operator : CG/JU
 Sample : M3434-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	18.010	2533	2537	2546	rVV2	1127943	1817930	34.08%	2.752%
78	18.098	2547	2552	2556	rVV5	295489	499691	9.37%	0.757%
79	18.163	2556	2563	2566	rVV4	385659	739158	13.86%	1.119%
80	18.198	2566	2569	2574	rVV	1485651	1909707	35.80%	2.891%
81	18.245	2574	2577	2581	rVB4	97800	133811	2.51%	0.203%
82	18.369	2592	2598	2604	rVB	3325942	4414309	82.76%	6.684%
83	18.504	2618	2621	2624	rBV3	119275	147697	2.77%	0.224%
84	18.545	2624	2628	2638	rVB	1268769	1743341	32.68%	2.640%
85	18.698	2649	2654	2658	rVB	820729	1072122	20.10%	1.623%
86	18.757	2661	2664	2671	rVB	249085	338947	6.35%	0.513%
87	19.051	2711	2714	2720	rVB	138040	173235	3.25%	0.262%
88	19.122	2722	2726	2730	rBV	554882	802970	15.05%	1.216%
89	19.175	2731	2735	2739	rVB2	574790	835514	15.66%	1.265%
90	19.251	2744	2748	2756	rBV4	781283	1201195	22.52%	1.819%
91	19.469	2782	2785	2789	rVB	332583	388837	7.29%	0.589%
92	19.675	2815	2820	2832	rVB	4343439	5334149	100.00%	8.076%
93	19.881	2850	2855	2859	rBV	917169	1118032	20.96%	1.693%
94	19.992	2871	2874	2878	rVB	252544	310963	5.83%	0.471%
95	20.933	3030	3034	3038	rBV3	387716	502093	9.41%	0.760%
96	21.198	3075	3079	3083	rBV	1620004	2054025	38.51%	3.110%
97	22.216	3250	3252	3254	rBV2	266322	301201	5.65%	0.456%
98	22.251	3255	3258	3263	rVB	595606	802751	15.05%	1.215%
99	22.422	3284	3287	3292	rVB2	450794	696618	13.06%	1.055%
100	23.510	3467	3472	3483	rVB2	1246634	2601863	48.78%	3.939%




Sum of corrected areas: 66047373

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006811.D
Acq On : 20 Aug 2021 21:28
Operator : CG/JU
Sample : M3434-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

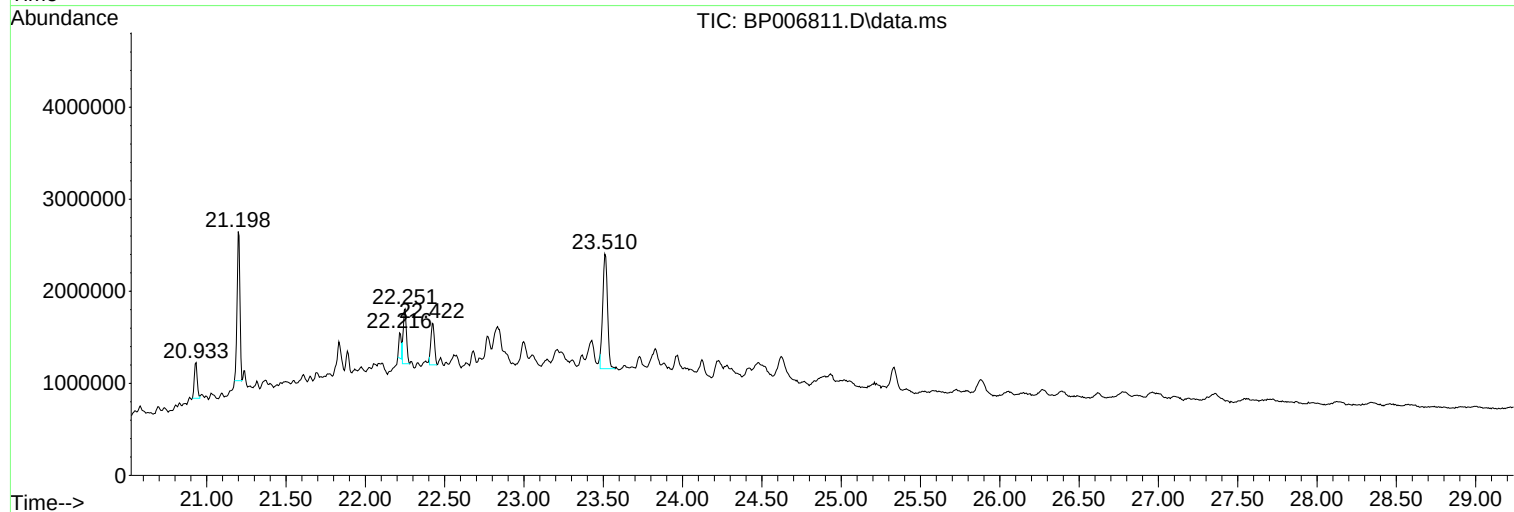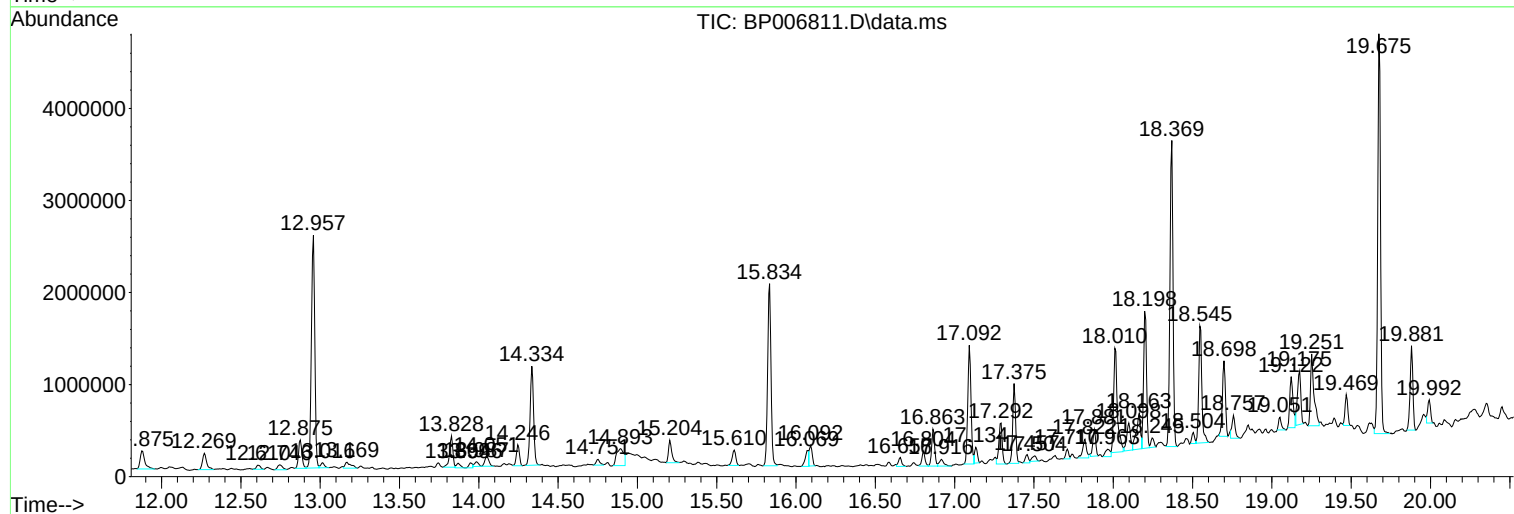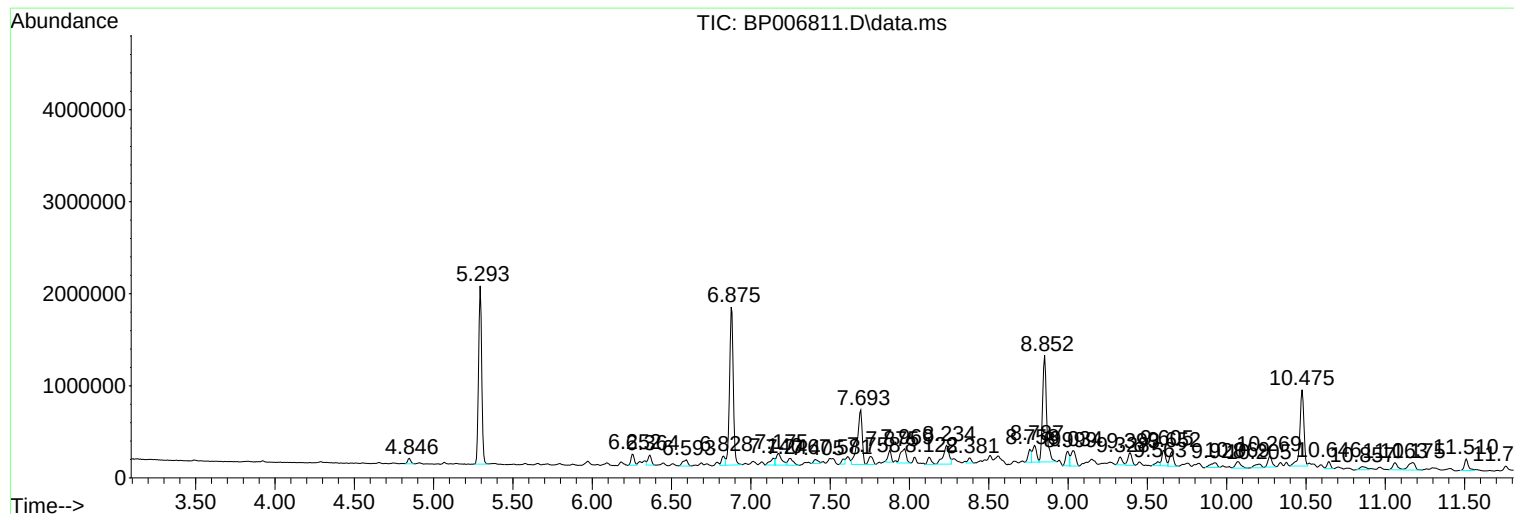

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006811.D
Acq On : 20 Aug 2021 21:28
Operator : CG/JU
Sample : M3434-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006811.D
Acq On : 20 Aug 2021 21:28
Operator : CG/JU
Sample : M3434-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------