

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006812.D
 Acq On : 20 Aug 2021 22:03
 Operator : CG/JU
 Sample : M3434-29
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-14-0515

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.846	295	299	307	rVB	126698	176469	3.04%	0.413%
2	5.293	369	375	383	rBV	3395987	4849139	83.40%	11.340%
3	6.881	638	645	660	rBV	3230755	4964763	85.39%	11.611%
4	7.693	777	783	790	rVB	596988	916838	15.77%	2.144%
5	8.852	973	980	990	rBV	2067563	3375594	58.06%	7.894%
6	10.275	1217	1222	1234	rBV2	88421	158576	2.73%	0.371%
7	10.475	1249	1256	1263	rBV	801545	1318924	22.68%	3.084%
8	12.957	1670	1678	1701	rBV	3879172	5740490	98.73%	13.425%
9	14.334	1905	1912	1921	rBV	1036777	1580780	27.19%	3.697%
10	15.834	2158	2167	2192	rBV	3203278	4761089	81.89%	11.134%
11	17.092	2375	2381	2386	rBV	1223691	1743797	29.99%	4.078%
12	17.134	2386	2388	2396	rVV	183123	271659	4.67%	0.635%
13	17.222	2400	2403	2409	rVB2	42817	66868	1.15%	0.156%
14	18.010	2532	2537	2545	rBV2	392738	602114	10.36%	1.408%
15	19.116	2720	2725	2731	rBV	323587	445070	7.65%	1.041%
16	19.245	2744	2747	2756	rBV3	224495	418665	7.20%	0.979%
17	19.469	2781	2785	2789	rVB	291607	356197	6.13%	0.833%
18	19.675	2815	2820	2829	rVB	4761318	5814259	100.00%	13.597%
19	20.933	3030	3034	3041	rBV	364645	577717	9.94%	1.351%
20	21.198	3074	3079	3083	rBV	1540177	2123494	36.52%	4.966%
21	21.233	3083	3085	3095	rVB2	243467	441070	7.59%	1.031%
22	23.510	3466	3472	3479	rVB2	1076637	2057283	35.38%	4.811%




Sum of corrected areas: 42760855

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006812.D
Acq On : 20 Aug 2021 22:03
Operator : CG/JU
Sample : M3434-29
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-14-0515

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

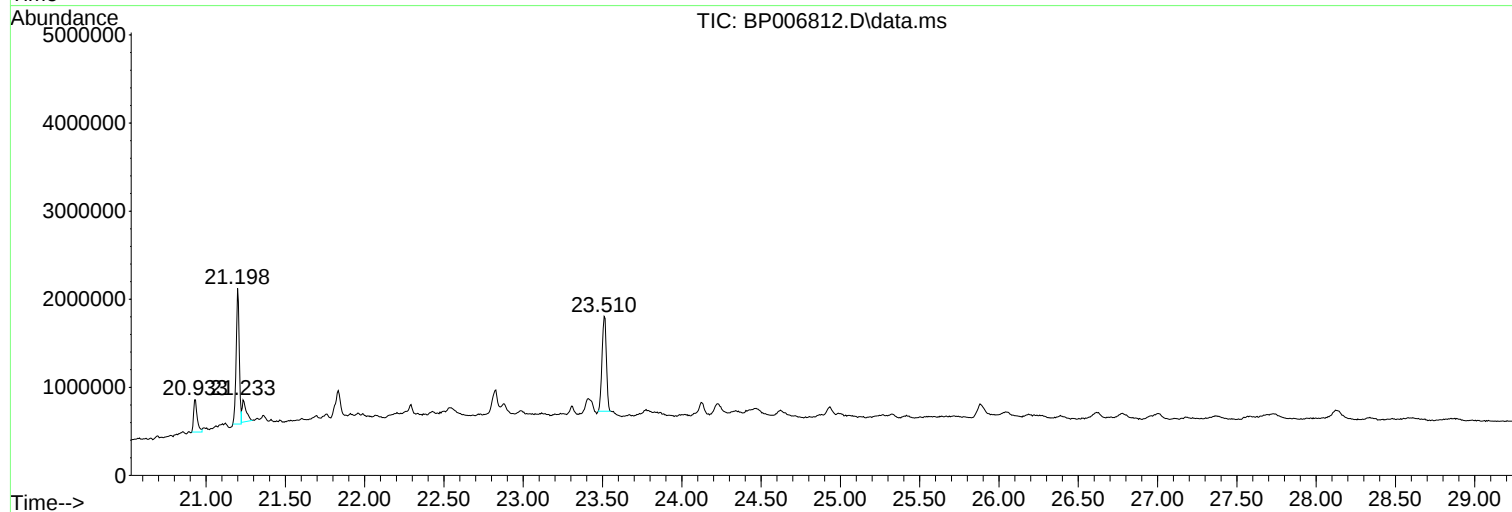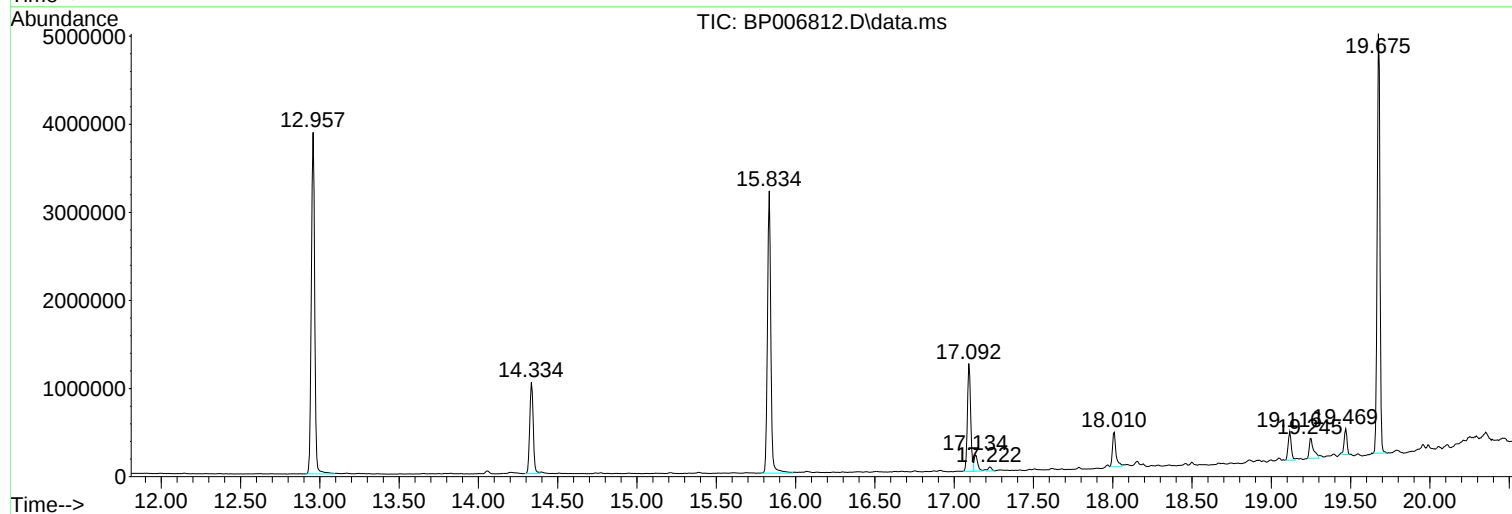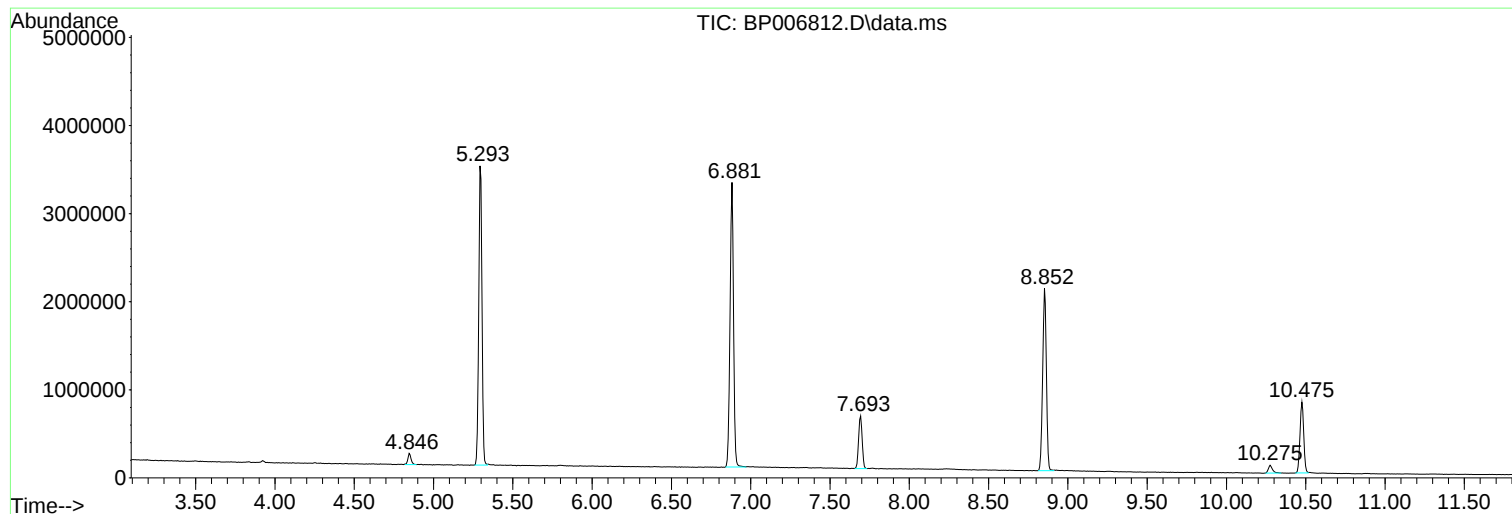

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006812.D
Acq On : 20 Aug 2021 22:03
Operator : CG/JU
Sample : M3434-29
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-14-0515

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006812.D
Acq On : 20 Aug 2021 22:03
Operator : CG/JU
Sample : M3434-29
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-14-0515

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
