

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006813.D
 Acq On : 20 Aug 2021 22:37
 Operator : CG/JU
 Sample : M3426-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-11-FD-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.846	296	299	308	rVB	88784	121106	1.57%	0.297%
2	5.293	369	375	383	rBV	2691437	3837123	49.66%	9.399%
3	6.881	638	645	656	rVB	2489990	3898555	50.45%	9.549%
4	7.693	777	783	790	rVB	592964	908504	11.76%	2.225%
5	8.851	973	980	989	rBV	1673795	2666064	34.50%	6.530%
6	10.275	1216	1222	1234	rBV	80661	160608	2.08%	0.393%
7	10.475	1248	1256	1263	rBV	785410	1295243	16.76%	3.173%
8	12.957	1671	1678	1699	rBV	3652360	5439742	70.40%	13.324%
9	13.563	1775	1781	1788	rBV2	50039	79871	1.03%	0.196%
10	14.334	1905	1912	1921	rBV	971939	1470265	19.03%	3.601%
11	15.833	2158	2167	2187	rBV	2794988	4126784	53.41%	10.108%
12	16.916	2347	2351	2362	rVB2	92245	155294	2.01%	0.380%
13	17.092	2375	2381	2386	rBV	1196081	1710902	22.14%	4.191%
14	17.133	2386	2388	2394	rVB	202620	255484	3.31%	0.626%
15	17.227	2400	2404	2410	rVB	70403	106418	1.38%	0.261%
16	17.533	2452	2456	2461	rVB2	60859	90059	1.17%	0.221%
17	18.004	2532	2536	2542	rBV2	371798	545930	7.07%	1.337%
18	18.739	2658	2661	2665	rVB2	107295	141523	1.83%	0.347%
19	19.116	2721	2725	2730	rBV	372853	474494	6.14%	1.162%
20	19.251	2744	2748	2750	rBV	172911	231615	3.00%	0.567%
21	19.469	2782	2785	2789	rVB	280915	328322	4.25%	0.804%
22	19.674	2815	2820	2832	rVB	5982487	7727141	100.00%	18.927%
23	20.927	3030	3033	3040	rBV2	428395	587220	7.60%	1.438%
24	21.198	3074	3079	3083	rBV	1649553	2263400	29.29%	5.544%
25	23.510	3467	3472	3479	rVB2	1159708	2203848	28.52%	5.398%




Sum of corrected areas: 40825515

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006813.D
Acq On : 20 Aug 2021 22:37
Operator : CG/JU
Sample : M3426-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-11-FD-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

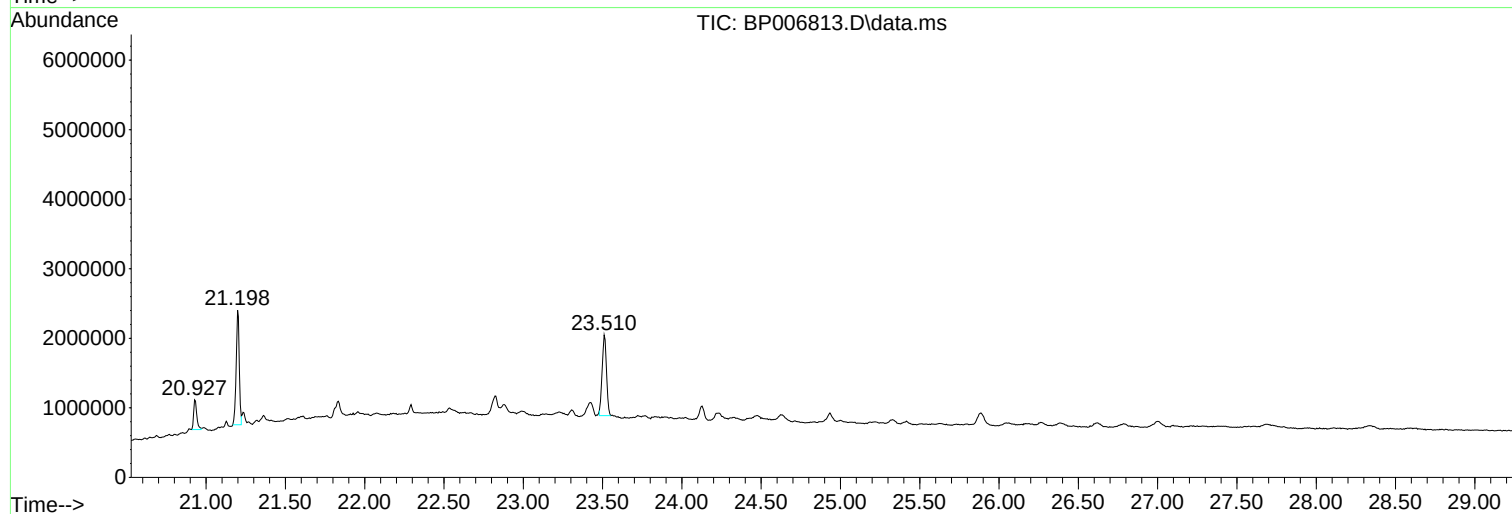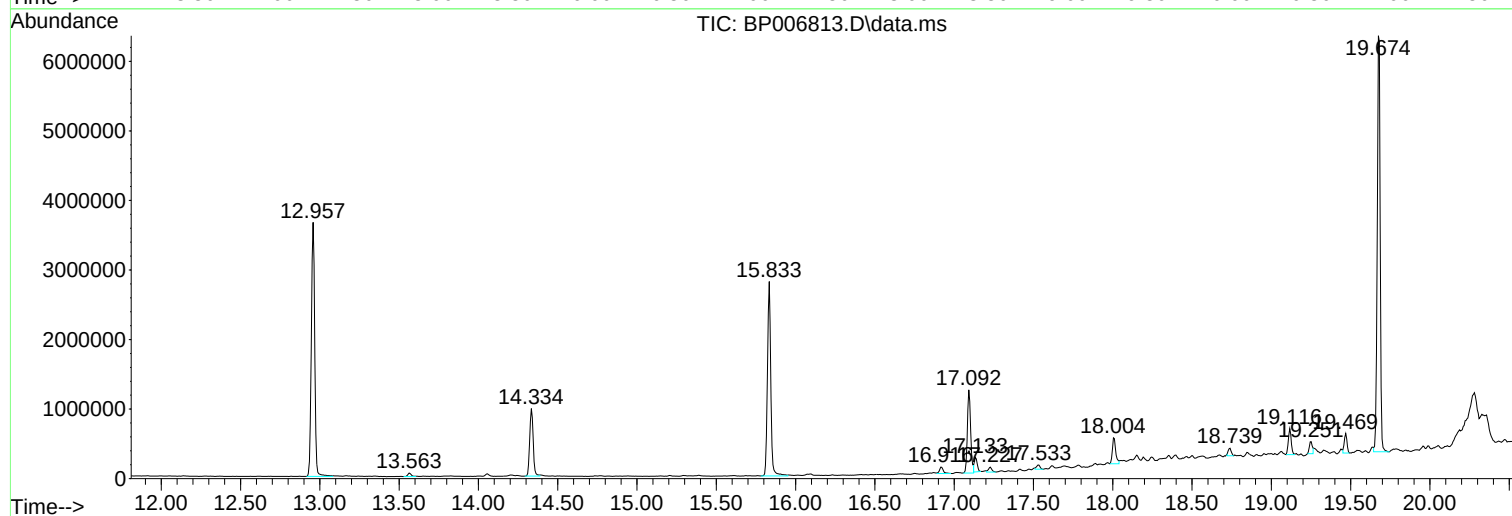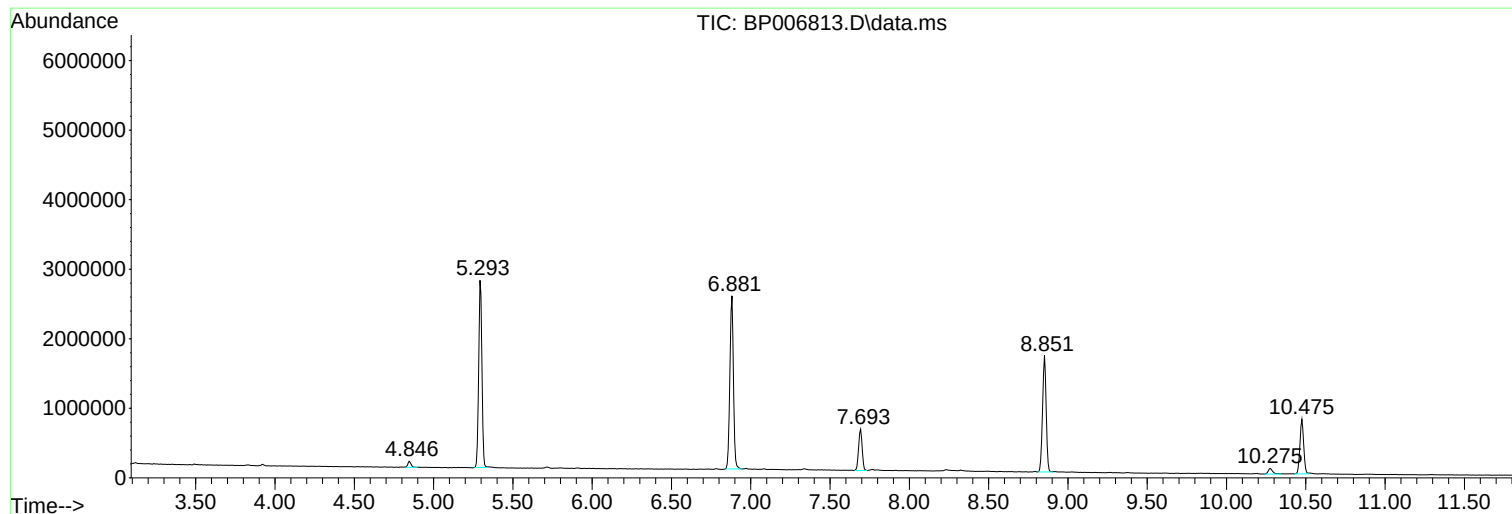

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006813.D
Acq On : 20 Aug 2021 22:37
Operator : CG/JU
Sample : M3426-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-11-FD-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006813.D
Acq On : 20 Aug 2021 22:37
Operator : CG/JU
Sample : M3426-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-11-FD-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc