

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006815.D
 Acq On : 20 Aug 2021 23:46
 Operator : CG/JU
 Sample : M3434-39
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-15-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.846	296	299	306	rVB	78709	109355	2.24%	0.269%
2	5.293	369	375	386	rBV	2236314	3187012	65.28%	7.844%
3	6.881	638	645	659	rVB	2104397	3272229	67.03%	8.054%
4	7.693	777	783	791	rVB	599270	940815	19.27%	2.316%
5	8.852	973	980	991	rBV	1386222	2231094	45.70%	5.492%
6	10.275	1217	1222	1230	rBV	64171	116090	2.38%	0.286%
7	10.475	1249	1256	1263	rBV	828946	1367810	28.02%	3.367%
8	12.957	1669	1678	1694	rBV	2622821	3928319	80.46%	9.669%
9	14.057	1858	1865	1873	rVB	65454	107742	2.21%	0.265%
10	14.210	1883	1891	1905	rVB6	18794	58453	1.20%	0.144%
11	14.334	1905	1912	1920	rBV	1121535	1661769	34.04%	4.090%
12	15.834	2156	2167	2190	rBV	2281038	3411148	69.87%	8.396%
13	17.092	2375	2381	2386	rBV	1362416	1978444	40.53%	4.870%
14	17.134	2386	2388	2396	rVB2	194961	348447	7.14%	0.858%
15	17.228	2401	2404	2410	rVB	55210	76837	1.57%	0.189%
16	18.010	2532	2537	2546	rVV2	416247	590051	12.09%	1.452%
17	18.157	2557	2562	2566	rBV2	65136	110131	2.26%	0.271%
18	18.498	2616	2620	2626	rVB2	50156	63464	1.30%	0.156%
19	18.998	2701	2705	2711	rBV5	30345	62461	1.28%	0.154%
20	19.116	2720	2725	2733	rBV	518996	729941	14.95%	1.797%
21	19.251	2744	2748	2756	rBV3	215615	391791	8.03%	0.964%
22	19.439	2777	2780	2781	rBV	55300	55458	1.14%	0.137%
23	19.469	2781	2785	2789	rVB	477793	586135	12.01%	1.443%
24	19.675	2815	2820	2831	rVB	3975863	4882028	100.00%	12.016%
25	19.957	2865	2868	2871	rBV2	84459	105639	2.16%	0.260%
26	19.986	2871	2873	2877	rVB	84181	88904	1.82%	0.219%
27	20.057	2882	2885	2888	rBV2	64854	70477	1.44%	0.173%
28	20.933	3029	3034	3041	rBV	656480	1010095	20.69%	2.486%
29	21.198	3074	3079	3083	rBV	1987047	2761014	56.55%	6.796%
30	21.233	3083	3085	3094	rVB	269596	354643	7.26%	0.873%
31	21.810	3180	3183	3185	rBV	313522	422079	8.65%	1.039%
32	22.827	3349	3356	3361	rBV2	806455	1590301	32.57%	3.914%
33	22.880	3362	3365	3376	rVB2	339267	616985	12.64%	1.519%
34	23.510	3466	3472	3479	rBV2	1345347	2600215	53.26%	6.400%
35	24.127	3573	3577	3586	rVB	396061	740683	15.17%	1.823%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006815.D
Acq On : 20 Aug 2021 23:46
Operator : CG/JU
Sample : M3434-39
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-15-1015

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 40628059

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006815.D
Acq On : 20 Aug 2021 23:46
Operator : CG/JU
Sample : M3434-39
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-15-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

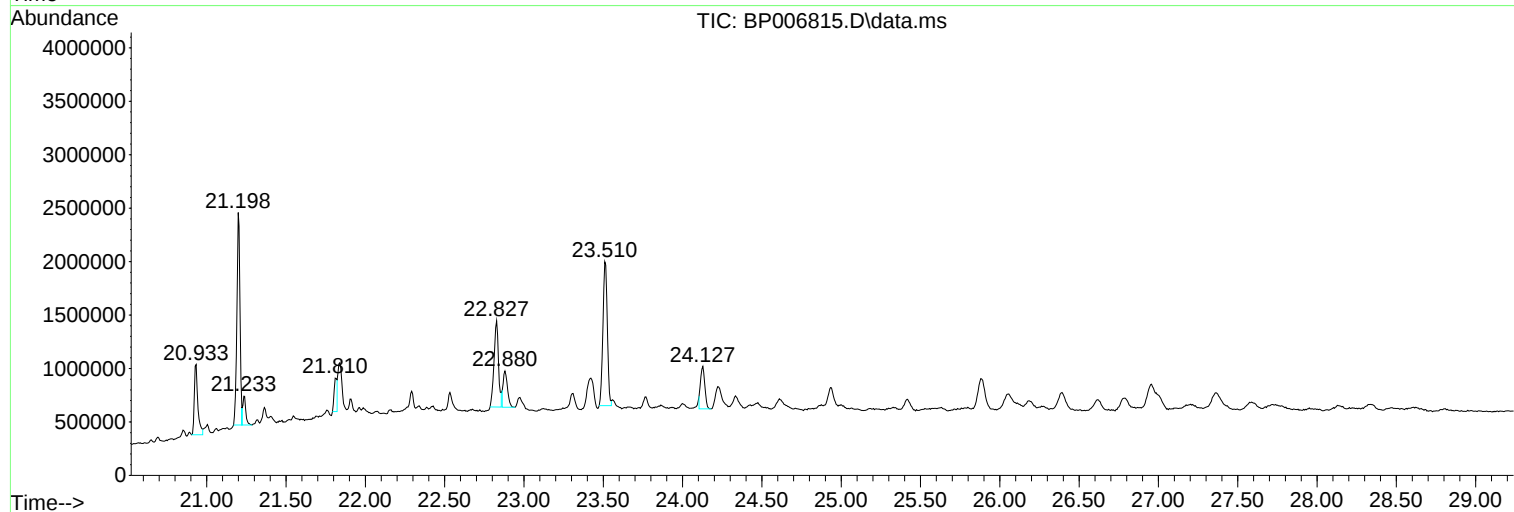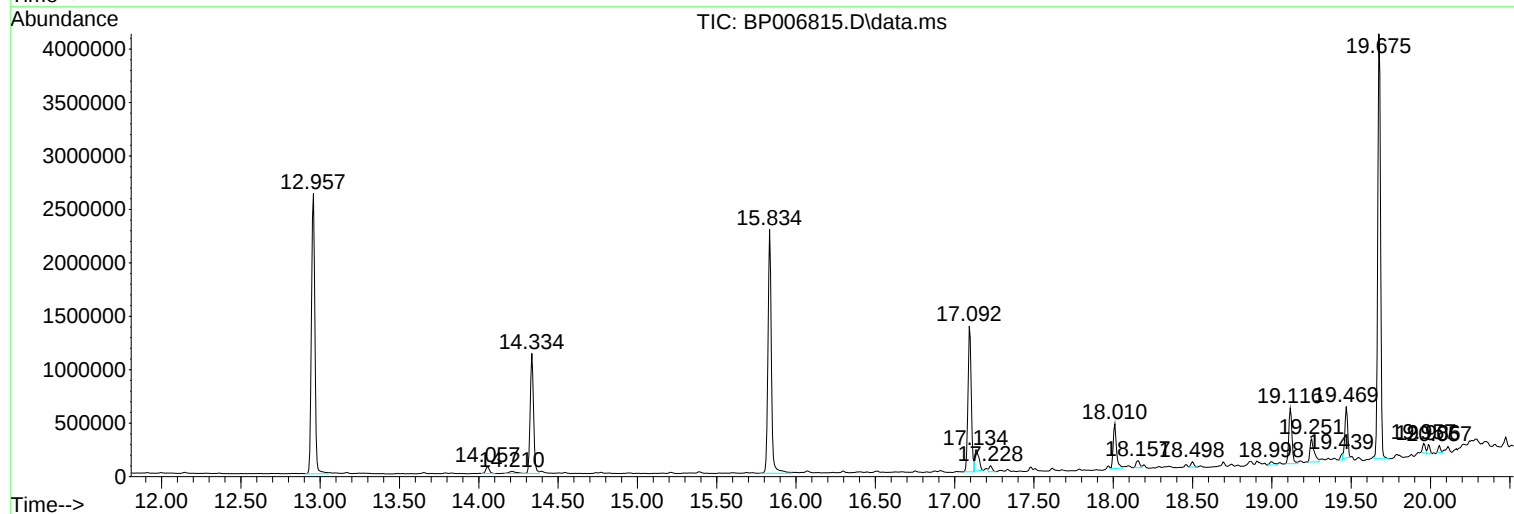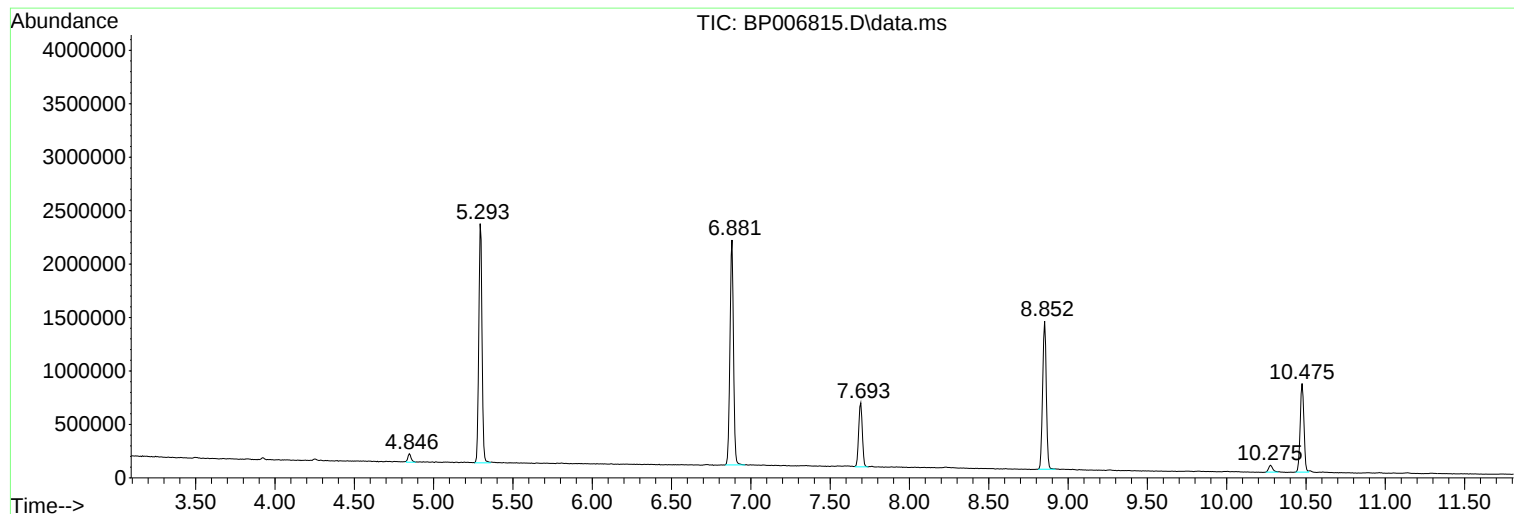

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006815.D
Acq On : 20 Aug 2021 23:46
Operator : CG/JU
Sample : M3434-39
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-15-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006815.D
Acq On : 20 Aug 2021 23:46
Operator : CG/JU
Sample : M3434-39
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-15-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------