

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006816.D
 Acq On : 21 Aug 2021 00:20
 Operator : CG/JU
 Sample : M3434-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.293	369	375	384	rBV	2703387	3878804	31.44%	3.963%
2	6.881	639	645	656	rVB	2463371	3824628	31.00%	3.908%
3	7.175	692	695	703	rVB3	79035	129320	1.05%	0.132%
4	7.245	704	707	716	rVB6	55065	124055	1.01%	0.127%
5	7.692	773	783	789	rVB	693709	1231692	9.98%	1.258%
6	7.969	822	830	837	rVV3	125611	282625	2.29%	0.289%
7	8.234	870	875	881	rVB3	103941	174052	1.41%	0.178%
8	8.757	959	964	966	rBV3	99003	156546	1.27%	0.160%
9	8.792	967	970	974	rVV2	136397	207282	1.68%	0.212%
10	8.851	974	980	993	rVB	1637379	2755785	22.33%	2.816%
11	8.998	1000	1005	1007	rBV3	104401	182900	1.48%	0.187%
12	9.034	1007	1011	1017	rVB4	127374	261902	2.12%	0.268%
13	9.392	1067	1072	1079	rVB3	123944	202419	1.64%	0.207%
14	9.604	1104	1108	1112	rVV	138270	223531	1.81%	0.228%
15	9.651	1112	1116	1124	rVB5	142034	245005	1.99%	0.250%
16	10.069	1181	1187	1196	rVB8	63463	156543	1.27%	0.160%
17	10.269	1215	1221	1229	rBV	145117	275516	2.23%	0.281%
18	10.475	1244	1256	1262	rBV	941207	1575089	12.77%	1.609%
19	11.175	1365	1375	1381	rVB5	77010	218027	1.77%	0.223%
20	11.510	1426	1432	1437	rBV2	159412	264548	2.14%	0.270%
21	11.880	1490	1495	1510	rBV3	80945	189926	1.54%	0.194%
22	12.875	1659	1664	1670	rBV	187543	269973	2.19%	0.276%
23	12.957	1670	1678	1686	rBV	3056137	4401041	35.67%	4.496%
24	13.827	1820	1826	1830	rVV2	225664	355158	2.88%	0.363%
25	14.057	1858	1865	1874	rBV	138926	247995	2.01%	0.253%
26	14.333	1902	1912	1920	rBV	1071727	1666944	13.51%	1.703%
27	14.898	1999	2008	2013	rBV	160977	528574	4.28%	0.540%
28	15.210	2057	2061	2070	rVB3	89180	162229	1.31%	0.166%
29	15.610	2124	2129	2136	rVB	90843	146895	1.19%	0.150%
30	15.833	2161	2167	2176	rVB	2305564	3254307	26.37%	3.325%
31	16.068	2203	2207	2209	rBV3	98443	143289	1.16%	0.146%
32	16.092	2209	2211	2216	rVB	122382	143184	1.16%	0.146%
33	16.868	2338	2343	2347	rBV2	100367	148339	1.20%	0.152%
34	17.092	2376	2381	2385	rBV	1224809	1763882	14.30%	1.802%
35	17.133	2385	2388	2396	rVB	366233	638520	5.17%	0.652%
36	17.292	2411	2415	2419	rVB	118447	161144	1.31%	0.165%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006816.D
 Acq On : 21 Aug 2021 00:20
 Operator : CG/JU
 Sample : M3434-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.374	2425	2429	2433	rBV	178342	223846	1.81%	0.229%
38	18.010	2533	2537	2546	rBV2	745573	1188052	9.63%	1.214%
39	18.198	2565	2569	2574	rVB2	2872661	3821557	30.97%	3.904%
40	18.368	2593	2598	2605	rVB	4222069	5360813	43.45%	5.477%
41	18.545	2625	2628	2633	rBV	841702	1129075	9.15%	1.154%
42	18.698	2650	2654	2658	rVB	614370	750700	6.08%	0.767%
43	19.127	2723	2727	2732	rBV	857813	1111548	9.01%	1.136%
44	19.174	2732	2735	2740	rVB	602038	742879	6.02%	0.759%
45	19.251	2745	2748	2755	rVV4	375545	670359	5.43%	0.685%
46	19.468	2782	2785	2793	rVB	778553	996229	8.07%	1.018%
47	19.674	2816	2820	2830	rVB	4127182	5110301	41.42%	5.221%
48	19.880	2852	2855	2859	rVB	974791	1117028	9.05%	1.141%
49	20.933	3030	3034	3036	rBV	2233463	2658851	21.55%	2.716%
50	21.204	3076	3080	3084	rBV	1741037	2127557	17.24%	2.174%
51	21.392	3110	3112	3118	rVB2	816989	996465	8.08%	1.018%
52	21.815	3181	3184	3185	rBV	1155046	1183145	9.59%	1.209%
53	21.851	3186	3190	3195	rVB2	3315311	5157441	41.80%	5.269%
54	22.345	3271	3274	3279	rBV	721738	986517	8.00%	1.008%
55	22.892	3363	3367	3378	rVB3	2186604	4500324	36.47%	4.598%
56	24.645	3658	3665	3676	rVB2	2434987	7381598	59.82%	7.542%
57	25.344	3777	3784	3793	rVB	3241056	7733607	62.68%	7.901%
58	27.727	4178	4189	4199	rVB	3587001	12338995	100.00%	12.606%




Sum of corrected areas: 97878556

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006816.D
Acq On : 21 Aug 2021 00:20
Operator : CG/JU
Sample : M3434-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

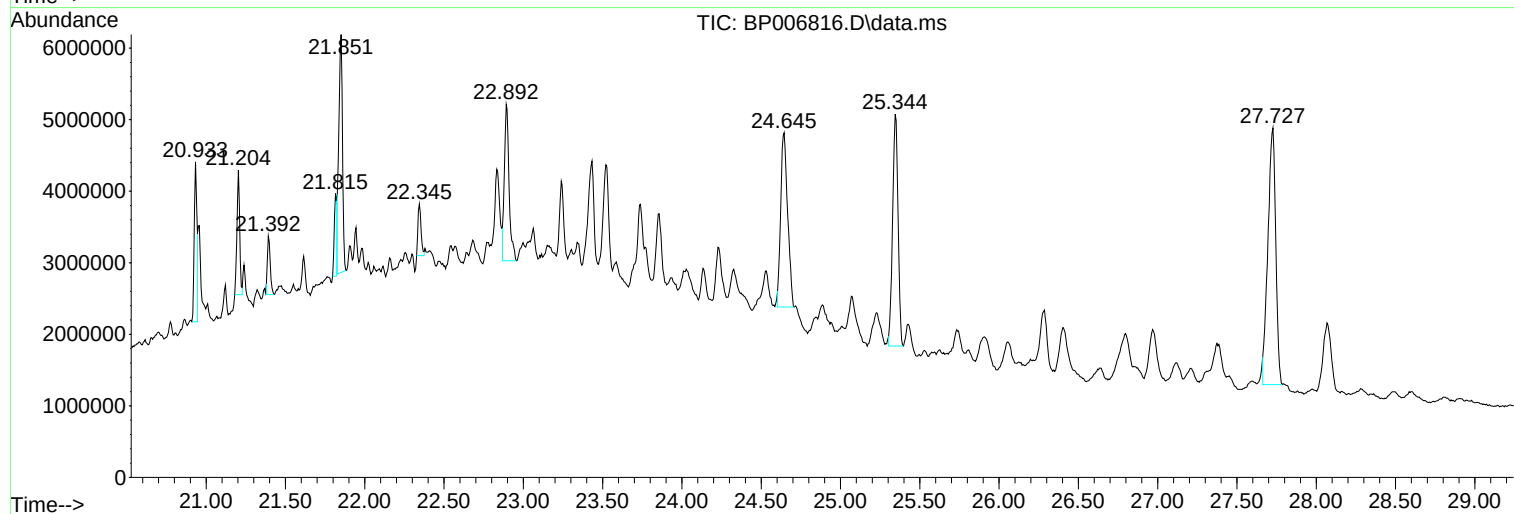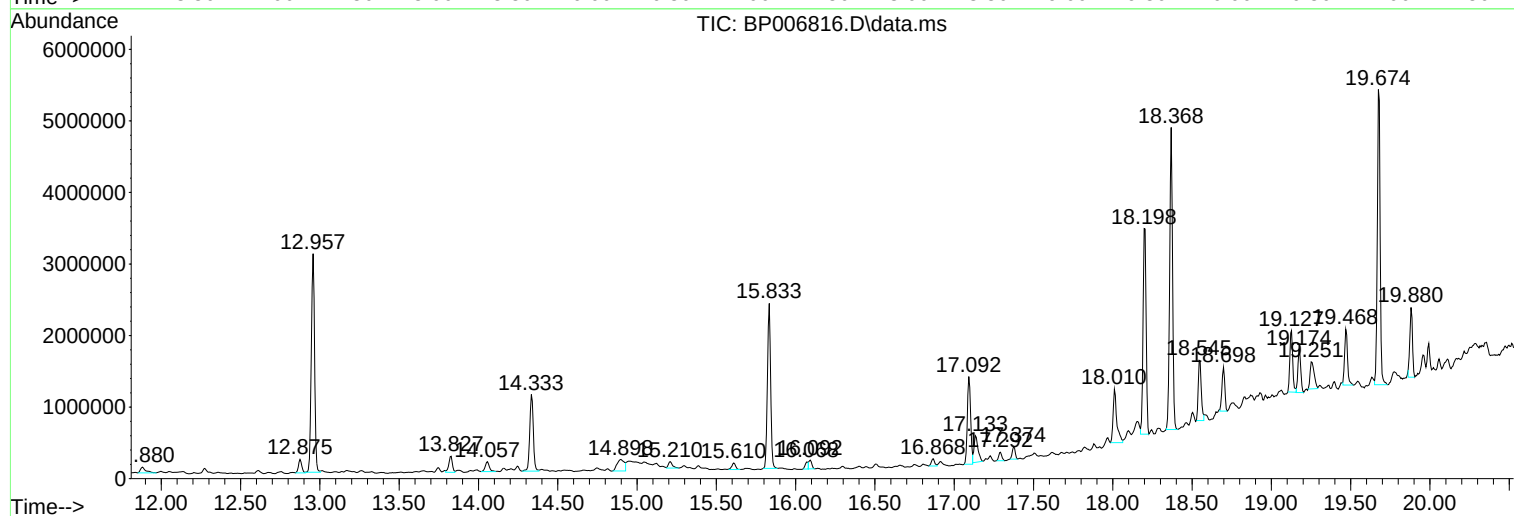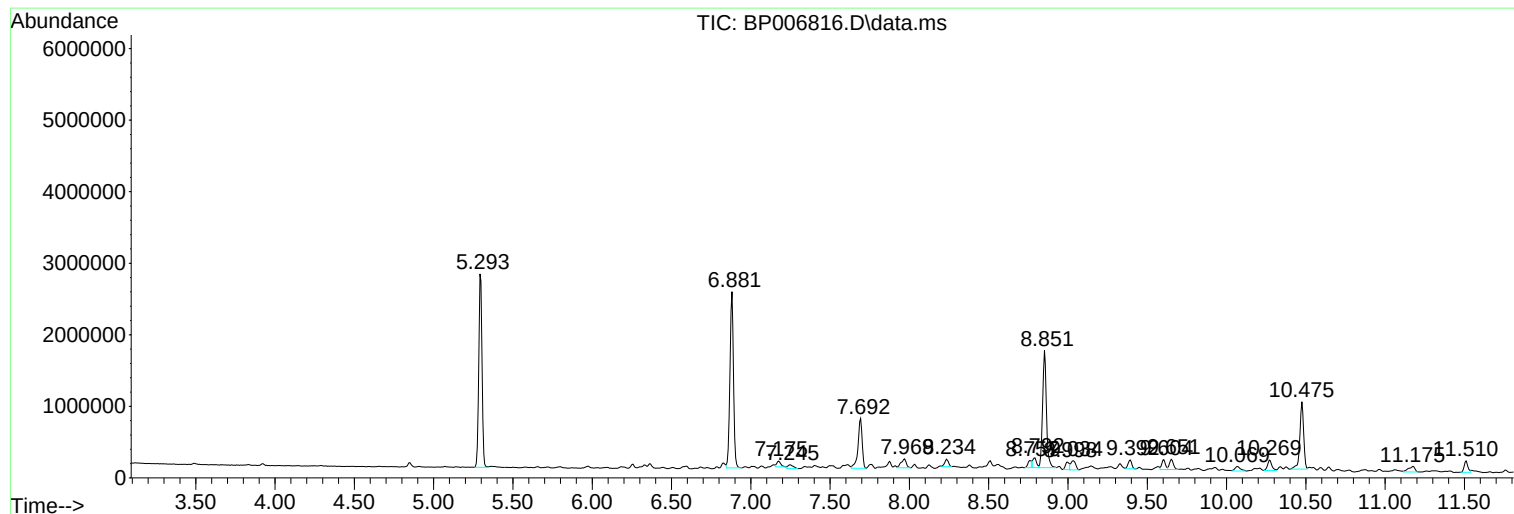

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006816.D
Acq On : 21 Aug 2021 00:20
Operator : CG/JU
Sample : M3434-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006816.D
Acq On : 21 Aug 2021 00:20
Operator : CG/JU
Sample : M3434-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------