

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006818.D
 Acq On : 21 Aug 2021 01:28
 Operator : CG/JU
 Sample : M3434-37
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-15-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.293	370	375	386	rVB	2433039	3543186	3.84%	0.794%
2	6.881	638	645	656	rVB	2317247	3618908	3.92%	0.811%
3	7.693	777	783	790	rVB	711731	1119455	1.21%	0.251%
4	8.852	973	980	994	rBV	1589420	2553161	2.77%	0.572%
5	10.475	1250	1256	1263	rVB	1007428	1645693	1.78%	0.369%
6	12.957	1671	1678	1697	rBV	2699105	4034122	4.37%	0.904%
7	14.334	1905	1912	1921	rBV	1290830	1977553	2.14%	0.443%
8	15.834	2157	2167	2177	rBV	2463453	3629011	3.94%	0.813%
9	17.092	2375	2381	2386	rBV	1611245	2319880	2.52%	0.520%
10	18.010	2532	2537	2549	rBV2	1017214	1456967	1.58%	0.327%
11	18.545	2623	2628	2635	rVB	1077328	1410407	1.53%	0.316%
12	18.839	2674	2678	2686	rBV2	1055608	1822866	1.98%	0.409%
13	19.116	2720	2725	2733	rBV	608817	1002659	1.09%	0.225%
14	19.675	2815	2820	2825	rVB	3652356	4391385	4.76%	0.984%
15	19.963	2864	2869	2872	rBV	2934968	3916961	4.25%	0.878%
16	20.469	2949	2955	2958	rBV2	743893	1492845	1.62%	0.335%
17	20.851	3017	3020	3025	rVV	905568	1064507	1.15%	0.239%
18	20.933	3028	3034	3043	rVV	8782629	12368507	13.41%	2.772%
19	21.057	3051	3055	3060	rVV	2361990	2884609	3.13%	0.647%
20	21.110	3060	3064	3069	rVV	838351	1071141	1.16%	0.240%
21	21.198	3074	3079	3082	rBV	2140412	2905641	3.15%	0.651%
22	21.239	3082	3086	3094	rVB	3003913	3959661	4.29%	0.888%
23	21.363	3101	3107	3110	rBV2	799524	1504389	1.63%	0.337%
24	21.845	3177	3189	3196	rBV4	10718032	23919102	25.94%	5.361%
25	21.910	3196	3200	3205	rVB	1110675	1431889	1.55%	0.321%
26	21.980	3208	3212	3217	rBV	1871382	2546910	2.76%	0.571%
27	22.286	3258	3264	3268	rBV2	1245785	2514864	2.73%	0.564%
28	22.339	3268	3273	3278	rVV	1214559	2125568	2.31%	0.476%
29	22.410	3282	3285	3294	rVB3	633199	1095935	1.19%	0.246%
30	22.533	3302	3306	3313	rVB	735827	1008771	1.09%	0.226%
31	22.833	3349	3357	3361	rBV	7688878	13135745	14.25%	2.944%
32	22.886	3361	3366	3374	rVV	6328248	11459513	12.43%	2.569%
33	22.974	3375	3381	3398	rVB	5416936	9614901	10.43%	2.155%
34	23.427	3453	3458	3464	rVB3	770233	1655449	1.80%	0.371%
35	23.510	3466	3472	3481	rBV2	2043948	4270839	4.63%	0.957%
36	23.604	3483	3488	3496	rVB	785809	1386275	1.50%	0.311%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006818.D
 Acq On : 21 Aug 2021 01:28
 Operator : CG/JU
 Sample : M3434-37
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-15-0510

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.769	3511	3516	3523	rVB	783355	1440033	1.56%	0.323%
38	24.004	3550	3556	3568	rVB	1686823	3651183	3.96%	0.818%
39	24.133	3571	3578	3587	rVB	3352040	7072729	7.67%	1.585%
40	24.227	3588	3594	3605	rVV	3324269	8033174	8.71%	1.801%
41	24.345	3606	3614	3626	rVB	5357950	12593195	13.66%	2.823%
42	24.616	3652	3660	3676	rVB2	2777107	7684926	8.33%	1.723%
43	25.445	3796	3801	3811	rVB2	909906	2428643	2.63%	0.544%
44	25.898	3871	3878	3892	rVB6	980727	3710775	4.02%	0.832%
45	26.080	3900	3909	3925	rBV2	2328726	8344787	9.05%	1.870%
46	26.227	3929	3934	3944	rVB	1002557	2568812	2.79%	0.576%
47	26.410	3955	3965	3973	rBV3	4362076	12971355	14.07%	2.907%
48	26.839	4028	4038	4047	rBV2	2756393	9926974	10.77%	2.225%
49	27.021	4051	4069	4082	rVB2	21446122	91328736	99.04%	20.471%
50	27.215	4091	4102	4120	rBV	5066800	23111737	25.06%	5.180%
51	27.451	4122	4142	4157	rVB2	18732250	92211039	100.00%	20.669%
52	27.627	4161	4172	4184	rBV3	3592508	17200378	18.65%	3.855%




Sum of corrected areas: 446137751

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006818.D
Acq On : 21 Aug 2021 01:28
Operator : CG/JU
Sample : M3434-37
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-15-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

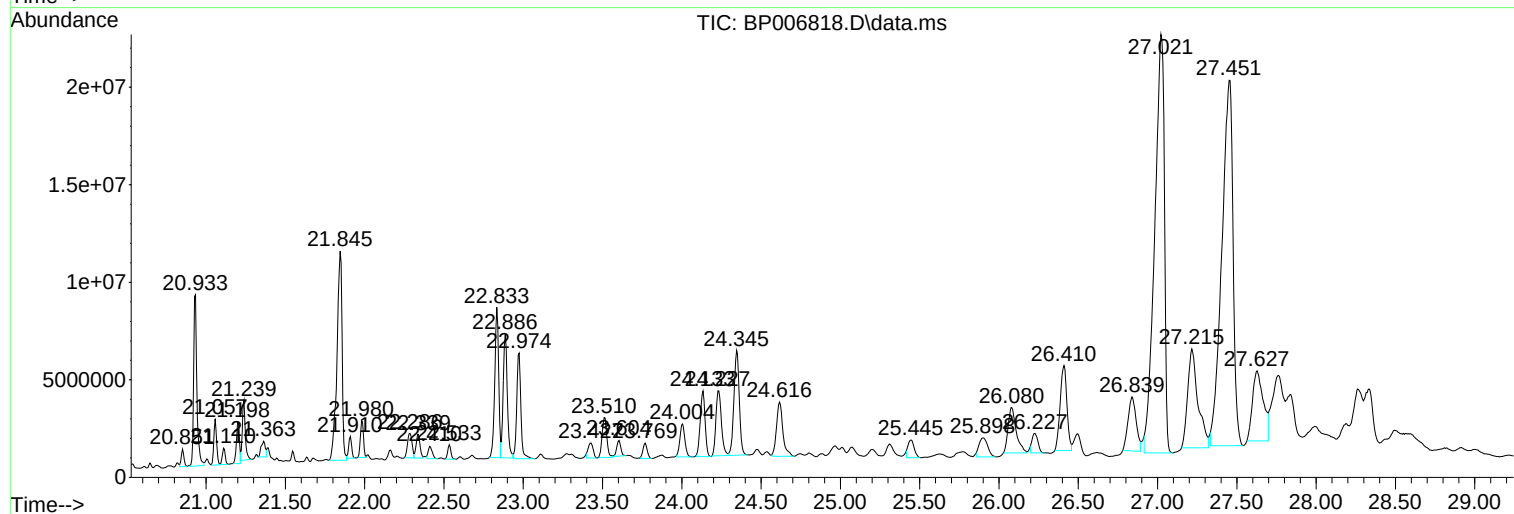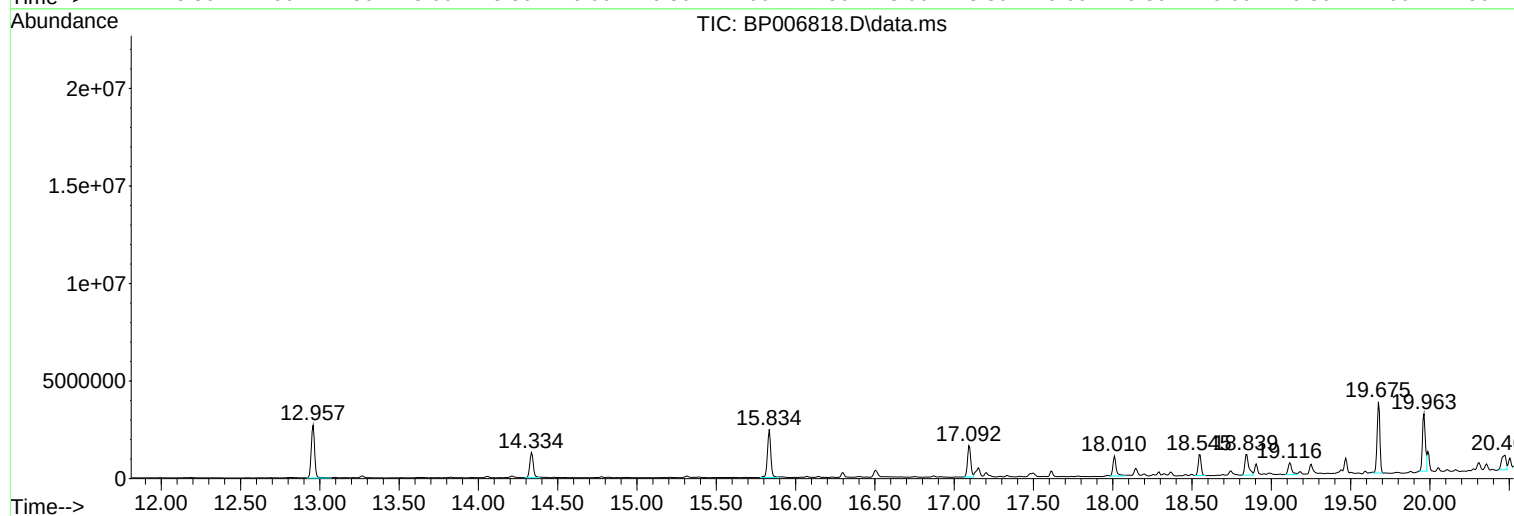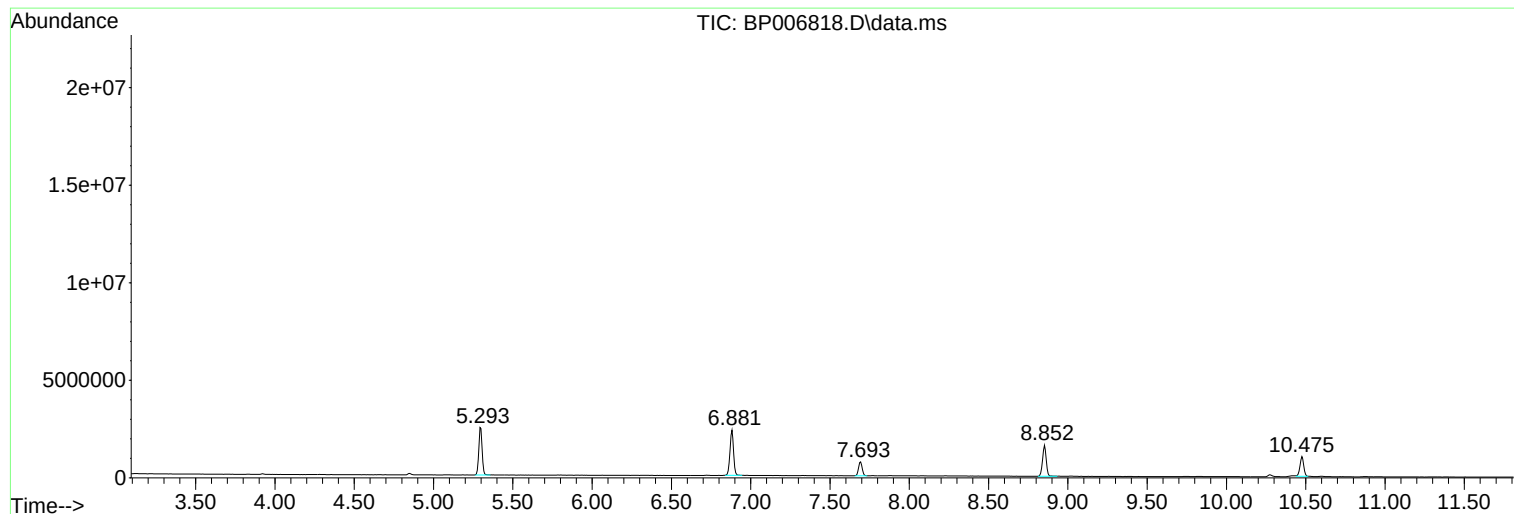

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006818.D
Acq On : 21 Aug 2021 01:28
Operator : CG/JU
Sample : M3434-37
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-15-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006818.D
Acq On : 21 Aug 2021 01:28
Operator : CG/JU
Sample : M3434-37
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-15-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc