

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006819.D
 Acq On : 21 Aug 2021 02:02
 Operator : CG/JU
 Sample : M3434-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	370	376	389	rVB	2503414	3537823	38.34%	2.322%
2	6.881	639	645	661	rVB	2303072	3612439	39.14%	2.371%
3	7.693	777	783	792	rVB	648310	999641	10.83%	0.656%
4	8.222	869	873	881	rVB	53060	96195	1.04%	0.063%
5	8.851	973	980	993	rBV	1521142	2449158	26.54%	1.608%
6	10.275	1216	1222	1231	rBV	178434	315515	3.42%	0.207%
7	10.475	1249	1256	1262	rBV	888526	1453783	15.75%	0.954%
8	11.998	1505	1515	1522	rBV3	41129	94579	1.02%	0.062%
9	12.151	1533	1541	1557	rBV4	51464	141118	1.53%	0.093%
10	12.957	1671	1678	1699	rBV	3458564	5086443	55.12%	3.339%
11	13.792	1814	1820	1825	rBV	203885	324686	3.52%	0.213%
12	14.057	1858	1865	1880	rBV	1172878	1905394	20.65%	1.251%
13	14.334	1906	1912	1919	rBV	1192868	1763875	19.11%	1.158%
14	14.398	1919	1923	1932	rVB	50755	95401	1.03%	0.063%
15	14.739	1973	1981	1985	rBV2	52912	100157	1.09%	0.066%
16	14.945	2010	2016	2021	rBV2	109049	215313	2.33%	0.141%
17	15.210	2056	2061	2067	rBV	202980	299232	3.24%	0.196%
18	15.333	2078	2082	2087	rBV	99344	138800	1.50%	0.091%
19	15.410	2093	2095	2105	rVB	119542	176107	1.91%	0.116%
20	15.598	2122	2127	2136	rVB4	72782	172873	1.87%	0.113%
21	15.728	2147	2149	2158	rVB3	60716	94104	1.02%	0.062%
22	15.833	2158	2167	2177	rBV	3036142	4216823	45.69%	2.768%
23	16.069	2202	2207	2218	rBV	231674	425607	4.61%	0.279%
24	16.392	2256	2262	2268	rBV5	62616	181937	1.97%	0.119%
25	16.669	2305	2309	2314	rBV	109436	156484	1.70%	0.103%
26	16.751	2319	2323	2332	rVB2	180131	281476	3.05%	0.185%
27	16.910	2347	2350	2359	rVB	127472	220363	2.39%	0.145%
28	17.010	2364	2367	2375	rBV	76040	129150	1.40%	0.085%
29	17.098	2376	2382	2385	rBV	1450525	2156011	23.36%	1.415%
30	17.139	2385	2389	2397	rVV	1969504	2800526	30.35%	1.838%
31	17.227	2399	2404	2409	rVB	819593	1133508	12.28%	0.744%
32	17.286	2410	2414	2420	rVV3	142660	255719	2.77%	0.168%
33	17.410	2432	2435	2440	rVB3	84117	120994	1.31%	0.079%
34	17.510	2448	2452	2457	rVB	200467	249109	2.70%	0.164%
35	17.622	2467	2471	2476	rVB2	145669	213380	2.31%	0.140%
36	17.680	2477	2481	2487	rVB3	183320	272094	2.95%	0.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006819.D
 Acq On : 21 Aug 2021 02:02
 Operator : CG/JU
 Sample : M3434-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.892	2513	2517	2521	rBV	91798	134181	1.45%	0.088%
38	17.969	2525	2530	2534	rVV	735194	1039448	11.26%	0.682%
39	18.016	2534	2538	2545	rVV2	1145164	1740216	18.86%	1.142%
40	18.098	2547	2552	2556	rVV	292510	479737	5.20%	0.315%
41	18.157	2556	2562	2566	rVV3	1012521	1895036	20.53%	1.244%
42	18.192	2566	2568	2575	rVB	604127	730090	7.91%	0.479%
43	18.286	2580	2584	2587	rBV3	97198	148678	1.61%	0.098%
44	18.351	2592	2595	2600	rVB2	181838	260189	2.82%	0.171%
45	18.457	2610	2613	2617	rBV	299442	378351	4.10%	0.248%
46	18.498	2617	2620	2630	rVB2	954801	1319984	14.30%	0.866%
47	18.669	2645	2649	2651	rBV	129468	182477	1.98%	0.120%
48	18.698	2651	2654	2658	rVV	264713	375144	4.07%	0.246%
49	18.745	2658	2662	2665	rVV	413587	550947	5.97%	0.362%
50	18.786	2665	2669	2673	rVB	274158	355821	3.86%	0.234%
51	18.863	2675	2682	2687	rVV2	967411	1874226	20.31%	1.230%
52	18.916	2687	2691	2695	rVV3	409001	820166	8.89%	0.538%
53	18.951	2695	2697	2701	rVB	293479	339070	3.67%	0.223%
54	19.004	2701	2706	2712	rBV	622450	1079195	11.69%	0.708%
55	19.122	2718	2726	2732	rBV	6496382	8567462	92.84%	5.624%
56	19.186	2734	2737	2740	rVV	168791	181392	1.97%	0.119%
57	19.216	2740	2742	2745	rVB2	117318	115190	1.25%	0.076%
58	19.263	2745	2750	2755	rVB	716826	1041713	11.29%	0.684%
59	19.316	2756	2759	2763	rBV2	284569	350478	3.80%	0.230%
60	19.357	2763	2766	2768	rBV	193536	215152	2.33%	0.141%
61	19.474	2781	2786	2794	rVB	6383238	9228581	100.00%	6.058%
62	19.551	2794	2799	2803	rBV2	515000	850970	9.22%	0.559%
63	19.592	2803	2806	2808	rBV2	154254	200637	2.17%	0.132%
64	19.680	2816	2821	2830	rBV	6627551	8921317	96.67%	5.856%
65	19.804	2834	2842	2857	rVV7	1730178	7495357	81.22%	4.920%
66	19.927	2858	2863	2865	rVV4	648971	1084427	11.75%	0.712%
67	19.963	2865	2869	2873	rVB	1120249	1525969	16.54%	1.002%
68	20.057	2882	2885	2888	rBV	564610	690774	7.49%	0.453%
69	20.116	2891	2895	2899	rVB	1024978	1341194	14.53%	0.880%
70	20.251	2914	2918	2921	rBV	879072	1325399	14.36%	0.870%
71	20.292	2922	2925	2928	rVV	641829	903557	9.79%	0.593%
72	20.374	2934	2939	2952	rVB4	1973966	6216946	67.37%	4.081%
73	20.692	2989	2993	2999	rVB	832723	1110620	12.03%	0.729%
74	20.892	3024	3027	3030	rVB	686744	715899	7.76%	0.470%
75	20.927	3030	3033	3039	rVV2	1493220	2097618	22.73%	1.377%
76	20.986	3040	3043	3050	rVB	795150	1025696	11.11%	0.673%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006819.D
 Acq On : 21 Aug 2021 02:02
 Operator : CG/JU
 Sample : M3434-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-13-0002

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.198	3073	3079	3084	rBV3	3954539	8415417	91.19%	5.524%
78	21.245	3084	3087	3096	rVB	3781980	4801923	52.03%	3.152%
79	21.410	3112	3115	3124	rVB3	720054	1064447	11.53%	0.699%
80	21.763	3173	3175	3179	rVB	752464	872907	9.46%	0.573%
81	21.827	3181	3186	3192	rVB3	953830	2038634	22.09%	1.338%
82	21.963	3206	3209	3212	rBV2	492362	618152	6.70%	0.406%
83	22.827	3349	3356	3361	rBV	3603904	8464360	91.72%	5.556%
84	23.321	3434	3440	3449	rVB	2339358	4410232	47.79%	2.895%
85	23.421	3451	3457	3465	rVB	3157149	5960400	64.59%	3.913%
86	23.521	3469	3474	3479	rVV2	1178372	2070873	22.44%	1.359%
87	25.909	3873	3880	3893	rVB3	1631695	5108511	55.36%	3.353%
88	26.651	4000	4006	4017	rVB	1290949	3716190	40.27%	2.439%




Sum of corrected areas: 152337167

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006819.D
Acq On : 21 Aug 2021 02:02
Operator : CG/JU
Sample : M3434-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

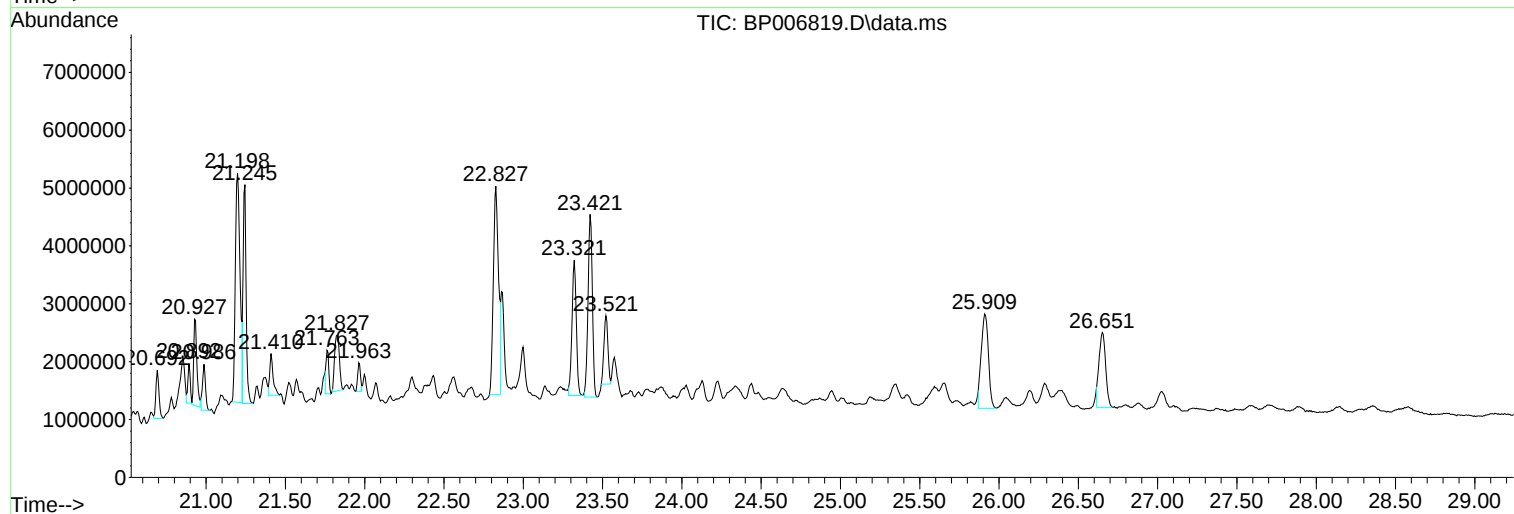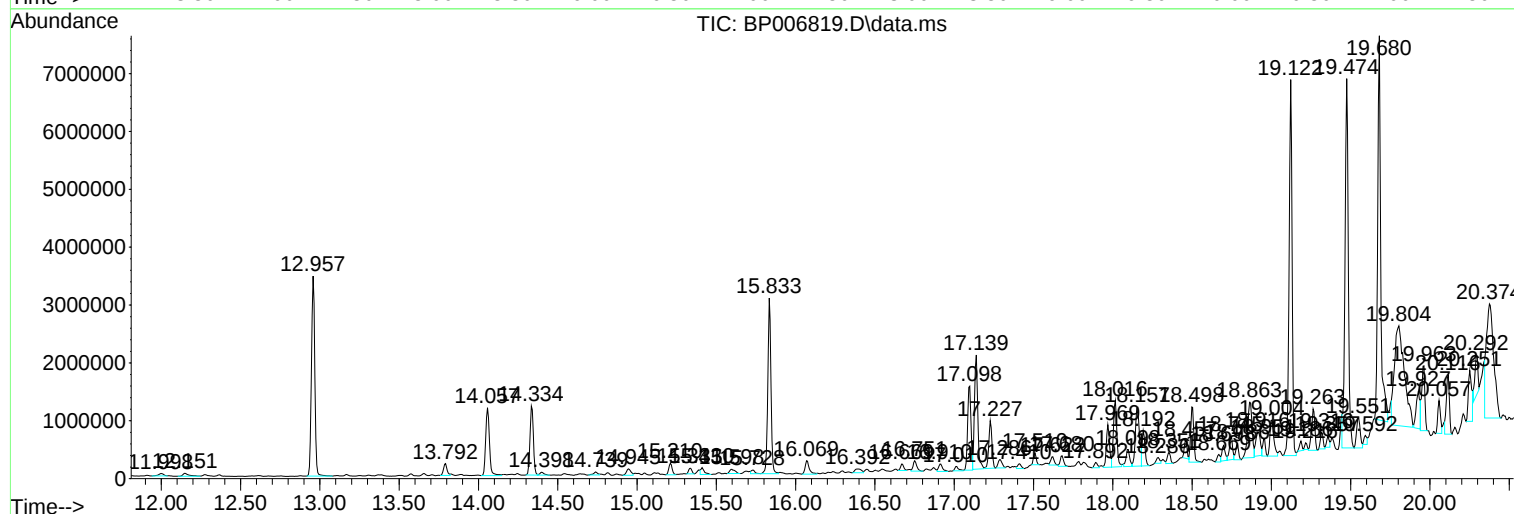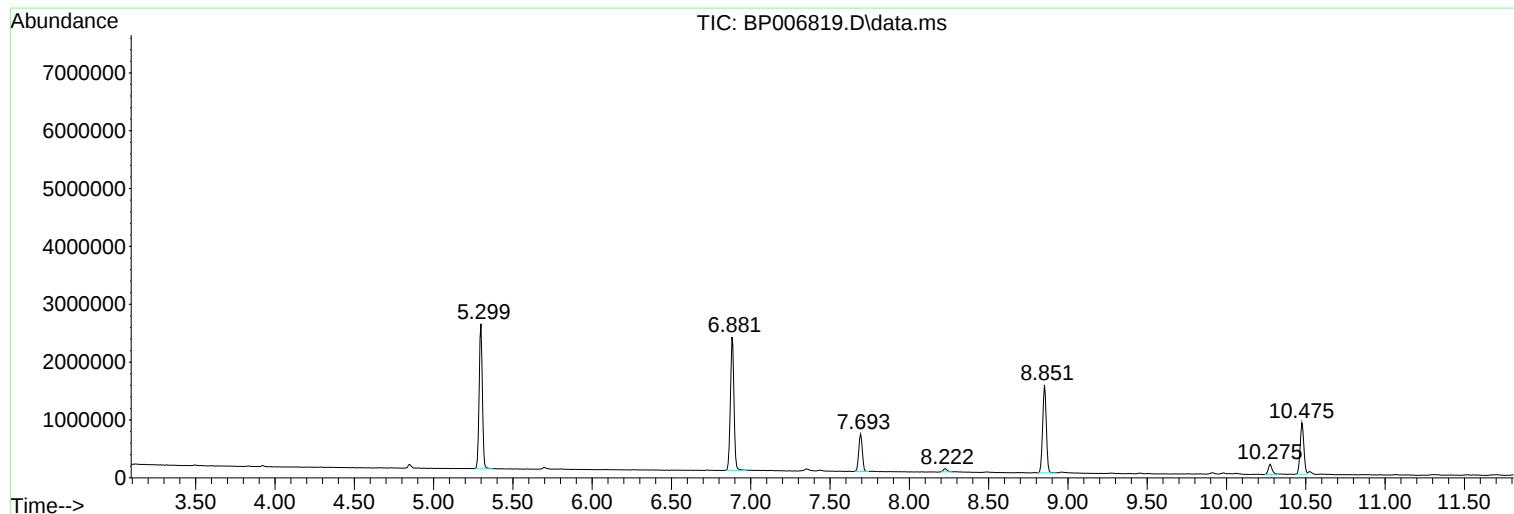

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006819.D
Acq On : 21 Aug 2021 02:02
Operator : CG/JU
Sample : M3434-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006819.D
Acq On : 21 Aug 2021 02:02
Operator : CG/JU
Sample : M3434-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-13-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
