

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006820.D
 Acq On : 21 Aug 2021 02:36
 Operator : CG/JU
 Sample : M3434-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-11-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	307	rVB	81597	112186	1.38%	0.215%
2	5.299	370	376	387	rVB	2906821	4063308	49.93%	7.793%
3	6.887	639	646	656	rBV	2665439	4127492	50.72%	7.916%
4	7.693	777	783	790	rVB	739446	1136235	13.96%	2.179%
5	8.851	973	980	997	rVB	1678573	2767523	34.01%	5.308%
6	10.275	1217	1222	1230	rBV	63801	121878	1.50%	0.234%
7	10.475	1249	1256	1263	rBV	955905	1639009	20.14%	3.144%
8	12.957	1669	1678	1693	rBV	3767992	5567367	68.42%	10.678%
9	14.057	1859	1865	1872	rBV	136363	207690	2.55%	0.398%
10	14.339	1906	1913	1920	rBV	1346356	2036004	25.02%	3.905%
11	15.839	2160	2168	2187	rBV	3325305	4892355	60.12%	9.383%
12	17.098	2376	2382	2386	rBV	1695902	2526945	31.05%	4.846%
13	17.139	2386	2389	2396	rVV	318336	416796	5.12%	0.799%
14	17.227	2400	2404	2410	rVB	217900	302348	3.72%	0.580%
15	17.969	2526	2530	2533	rBV	132466	184382	2.27%	0.354%
16	18.010	2533	2537	2546	rVV2	380131	616680	7.58%	1.183%
17	18.092	2548	2551	2556	rVV	84791	145879	1.79%	0.280%
18	18.157	2557	2562	2566	rVV2	195838	373766	4.59%	0.717%
19	18.192	2566	2568	2574	rVB	124311	160637	1.97%	0.308%
20	18.457	2610	2613	2617	rVV	98676	110266	1.36%	0.211%
21	18.498	2617	2620	2625	rVB2	99946	131707	1.62%	0.253%
22	18.863	2676	2682	2687	rBV3	160465	340186	4.18%	0.652%
23	18.910	2687	2690	2692	rBV4	68635	96138	1.18%	0.184%
24	18.998	2702	2705	2711	rBV4	89162	144706	1.78%	0.278%
25	19.121	2721	2726	2732	rVB	835514	1119322	13.76%	2.147%
26	19.263	2745	2750	2755	rBV	200753	355890	4.37%	0.683%
27	19.468	2781	2785	2795	rVB	1093583	1555412	19.11%	2.983%
28	19.680	2816	2821	2830	rVB	6825803	8137364	100.00%	15.607%
29	19.957	2866	2868	2872	rVB2	246569	264580	3.25%	0.507%
30	20.927	3030	3033	3040	rBV2	692019	969437	11.91%	1.859%
31	21.204	3074	3080	3084	rBV2	2568070	4003205	49.20%	7.678%
32	21.239	3084	3086	3092	rVB	664018	768721	9.45%	1.474%
33	23.515	3468	3473	3479	rVB2	1484530	2744185	33.72%	5.263%




Sum of corrected areas: 52139599

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006820.D
Acq On : 21 Aug 2021 02:36
Operator : CG/JU
Sample : M3434-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-11-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

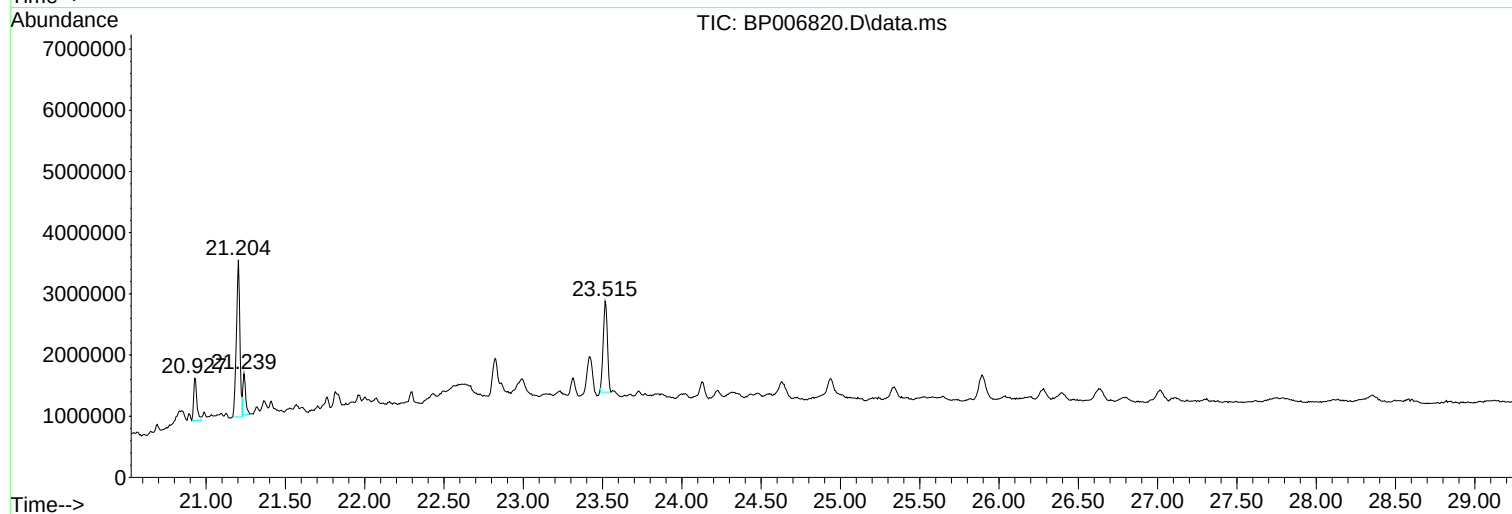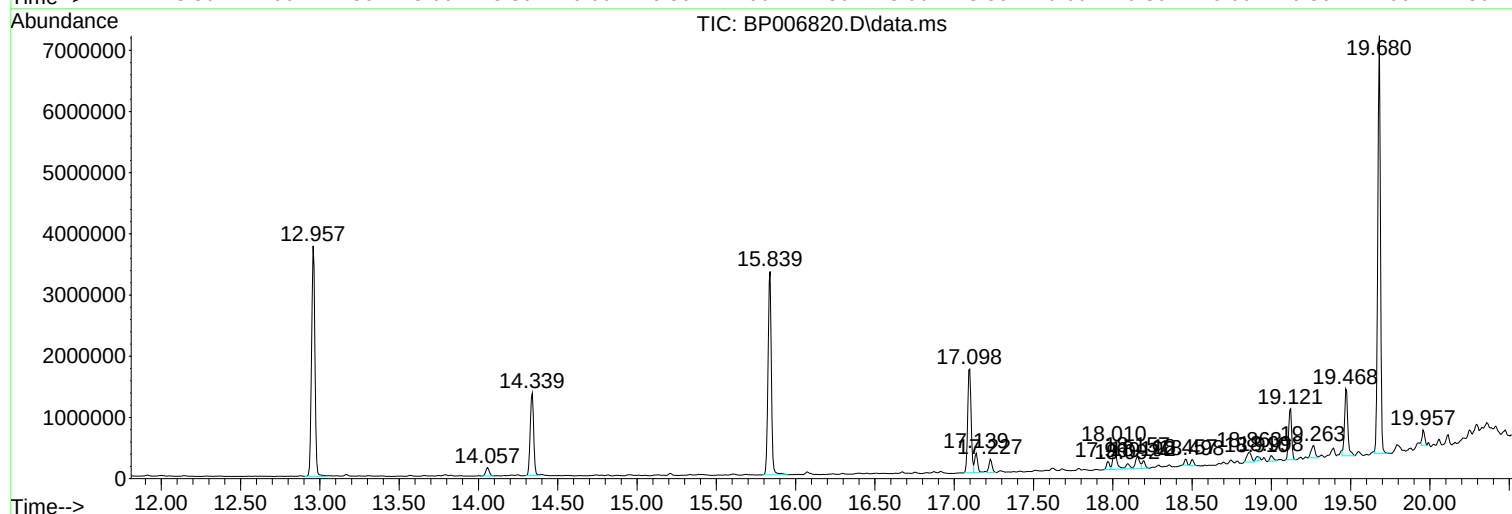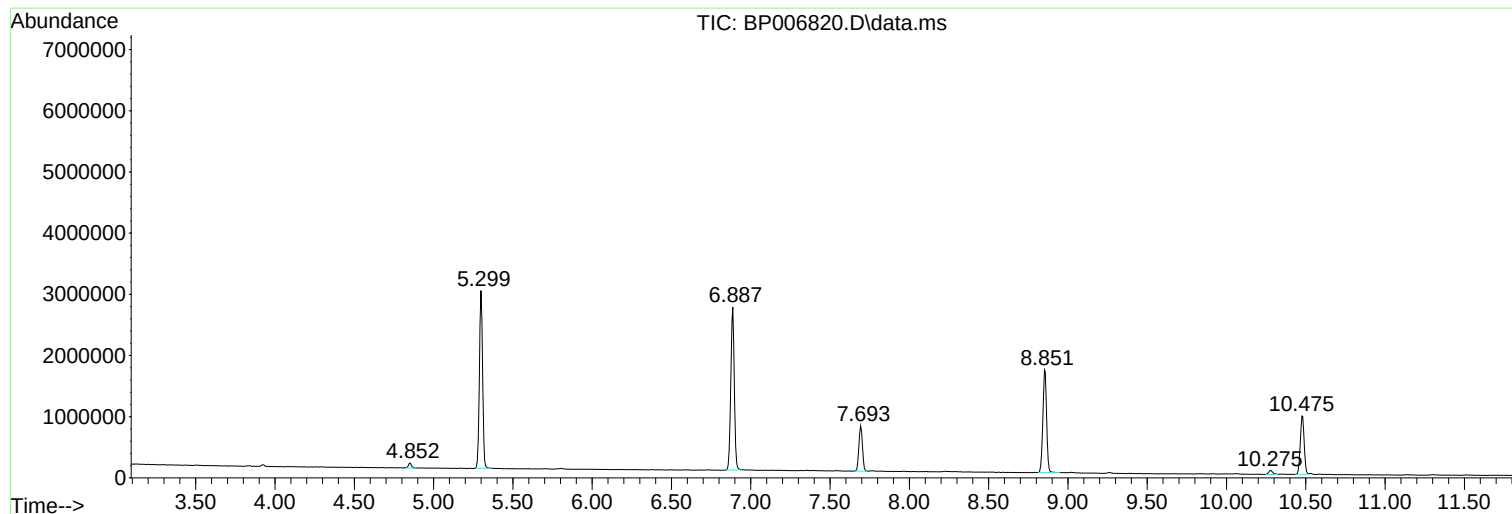

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006820.D
Acq On : 21 Aug 2021 02:36
Operator : CG/JU
Sample : M3434-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-11-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006820.D
Acq On : 21 Aug 2021 02:36
Operator : CG/JU
Sample : M3434-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-11-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------