

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006821.D
 Acq On : 21 Aug 2021 03:10
 Operator : CG/JU
 Sample : M3419-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-08-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	306	rVB	87883	125169	1.65%	0.251%
2	5.299	370	376	392	rVB	3075422	4376948	57.84%	8.763%
3	6.887	639	646	656	rVB	2897536	4476703	59.16%	8.962%
4	7.693	777	783	791	rVB	849069	1286719	17.00%	2.576%
5	8.858	974	981	988	rBV	1830998	3026359	39.99%	6.059%
6	10.275	1214	1222	1232	rBV	501019	840256	11.10%	1.682%
7	10.481	1249	1257	1263	rBV	1146026	1893251	25.02%	3.790%
8	12.957	1669	1678	1694	rBV	4139061	6162545	81.43%	12.337%
9	14.057	1860	1865	1871	rVB	108325	160538	2.12%	0.321%
10	14.340	1906	1913	1920	rBV	1549784	2284352	30.19%	4.573%
11	15.840	2161	2168	2178	rBV	3116272	4583905	60.57%	9.177%
12	16.057	2200	2205	2217	rVB	178101	353934	4.68%	0.709%
13	16.751	2319	2323	2331	rVB3	45003	78962	1.04%	0.158%
14	17.098	2376	2382	2387	rBV	1814044	2588390	34.20%	5.182%
15	17.139	2387	2389	2394	rVB	209916	240802	3.18%	0.482%
16	17.234	2401	2405	2410	rVB	90706	131331	1.74%	0.263%
17	17.786	2496	2499	2507	rBV	107068	143527	1.90%	0.287%
18	17.975	2527	2531	2533	rBV	65071	94026	1.24%	0.188%
19	18.010	2533	2537	2546	rVV2	433051	645309	8.53%	1.292%
20	18.157	2558	2562	2566	rBV2	72347	101370	1.34%	0.203%
21	18.292	2581	2585	2589	rBV2	70140	98172	1.30%	0.197%
22	18.863	2676	2682	2687	rBV3	111027	283989	3.75%	0.569%
23	18.910	2687	2690	2695	rVB3	85332	122688	1.62%	0.246%
24	19.122	2722	2726	2732	rBV	435975	559833	7.40%	1.121%
25	19.251	2745	2748	2756	rBV3	172580	360159	4.76%	0.721%
26	19.475	2782	2786	2796	rVB	419376	579802	7.66%	1.161%
27	19.681	2816	2821	2831	rVB	6592004	7567577	100.00%	15.150%
28	20.933	3030	3034	3040	rBV	851855	1157970	15.30%	2.318%
29	21.204	3076	3080	3084	rBV	2138052	2769536	36.60%	5.545%
30	23.527	3470	3475	3482	rVB2	1513333	2856100	37.74%	5.718%




Sum of corrected areas: 49950222

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006821.D
Acq On : 21 Aug 2021 03:10
Operator : CG/JU
Sample : M3419-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

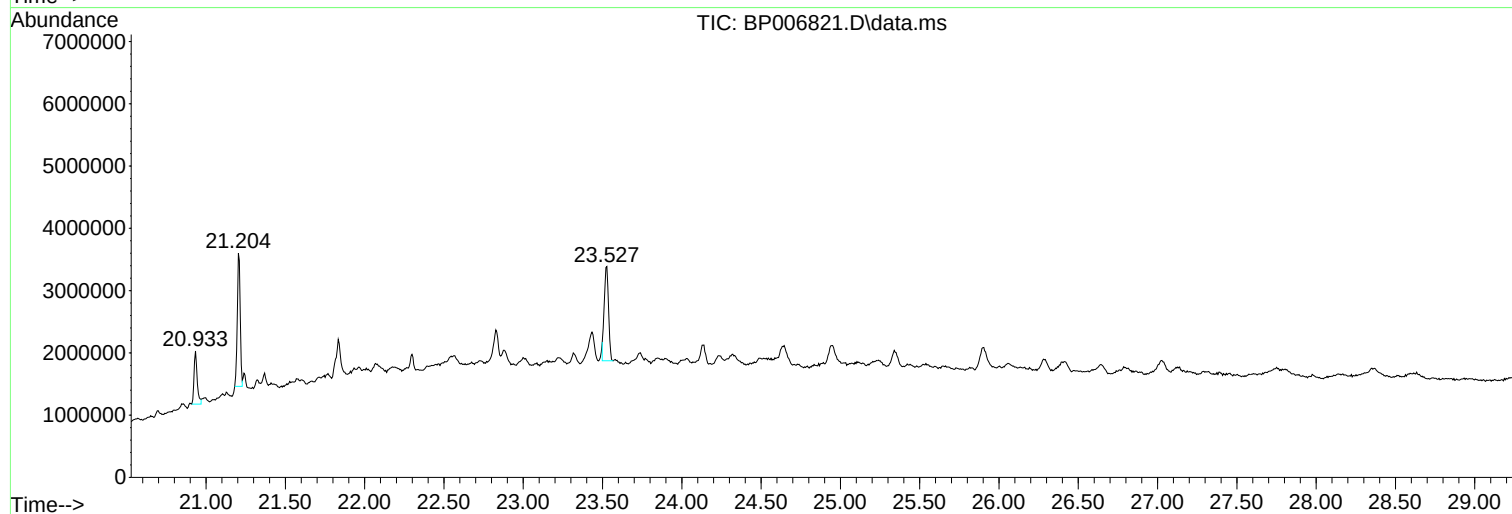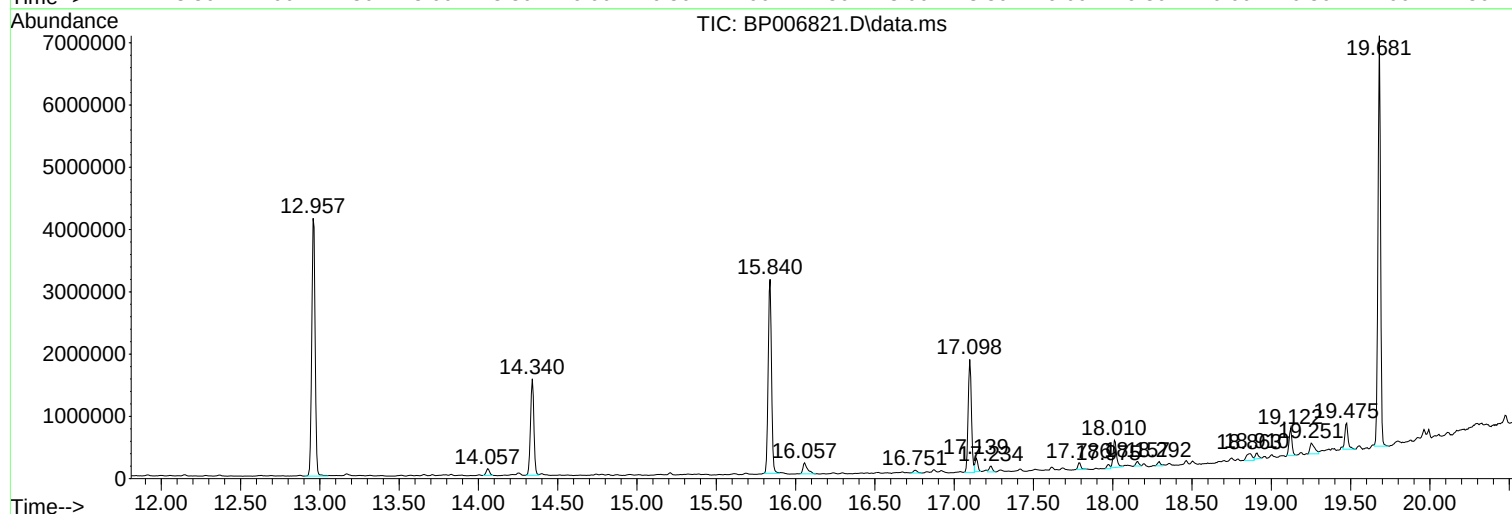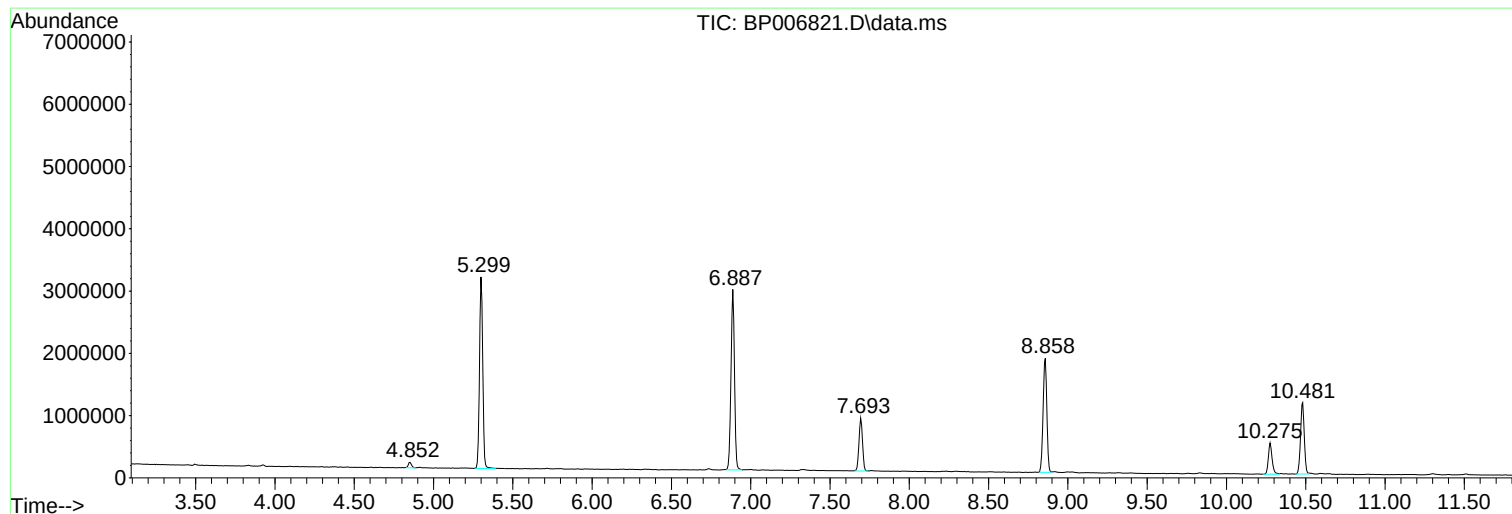

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006821.D
Acq On : 21 Aug 2021 03:10
Operator : CG/JU
Sample : M3419-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
Data File : BP006821.D
Acq On : 21 Aug 2021 03:10
Operator : CG/JU
Sample : M3419-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
