
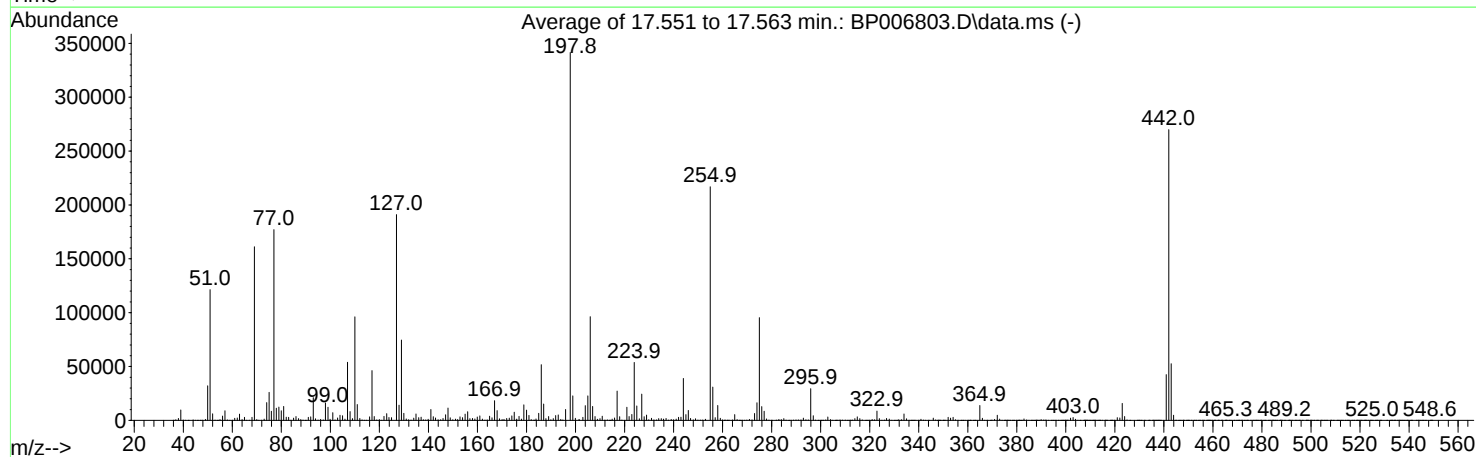


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006803.D
 Acq On : 20 Aug 2021 16:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 20 11:25:25 2021

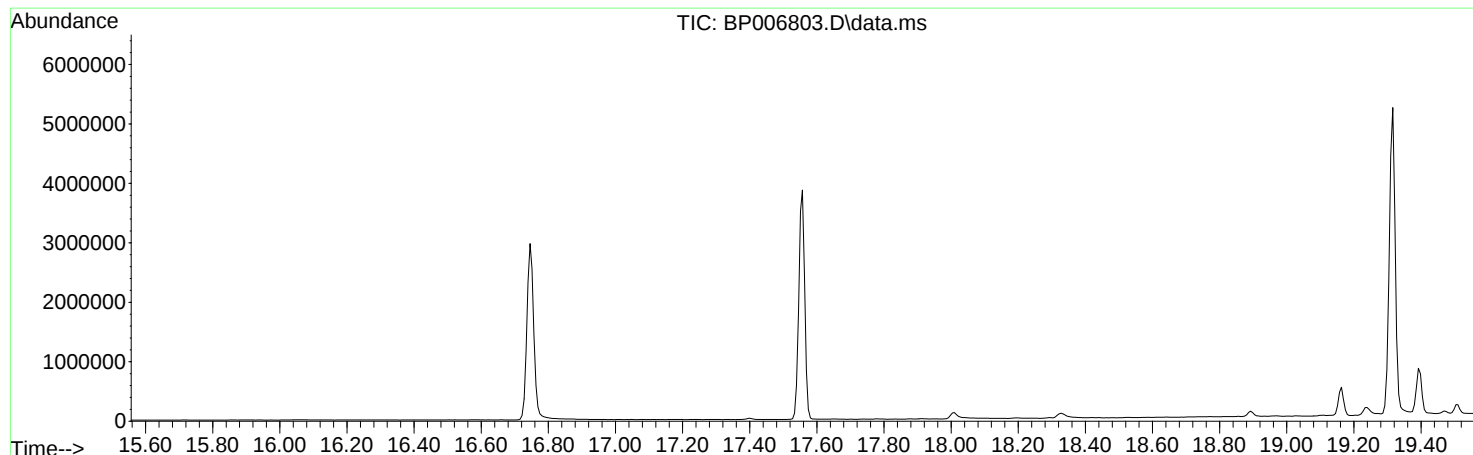




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	121417	PASS
68	69	0.00	2	1.8	2844	PASS
69	198	0.00	100	47.2	161206	PASS
70	69	0.00	2	0.5	781	PASS
127	198	10	80	55.9	191049	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	341517	PASS
199	198	5	9	6.7	22718	PASS
275	198	10	60	27.9	95427	PASS
365	198	1	100	4.0	13804	PASS
441	198	0.01	100	12.5	42546	PASS
442	442	100	100	100.0	269909	PASS
443	442	15	24	19.5	52568	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006803.D
 Acq On : 20 Aug 2021 16:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 21 04:39:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 11:25:25 2021
 Response via : Initial Calibration

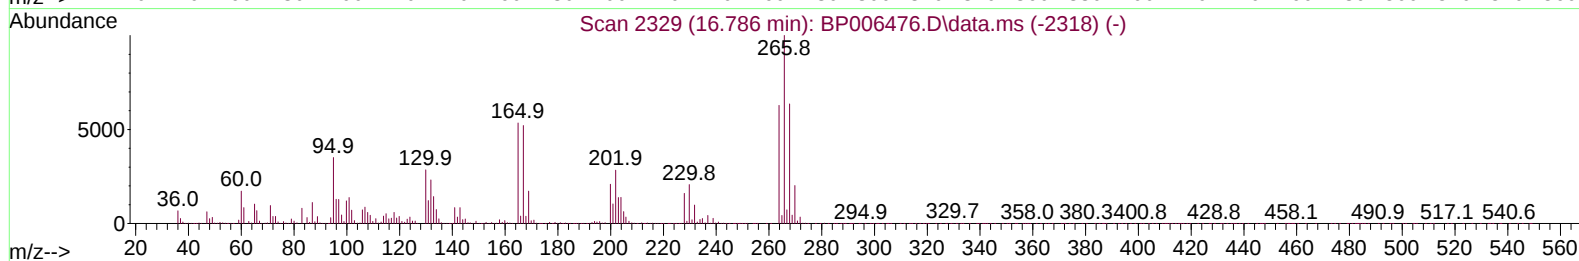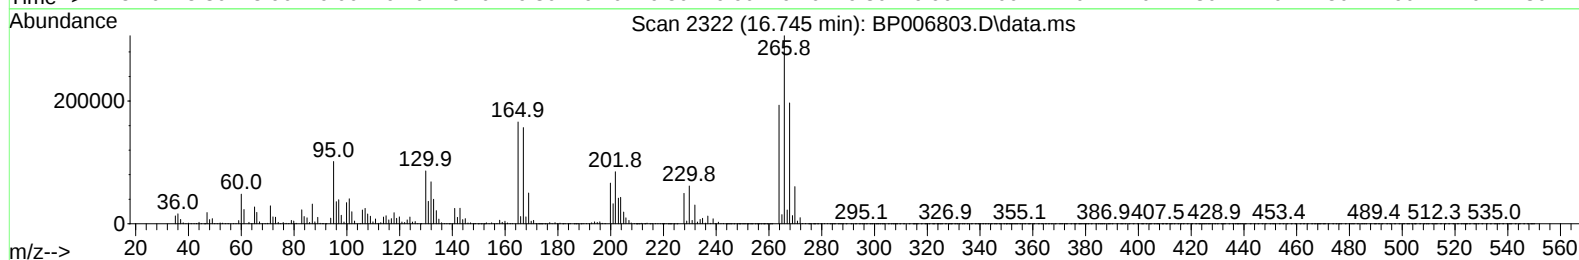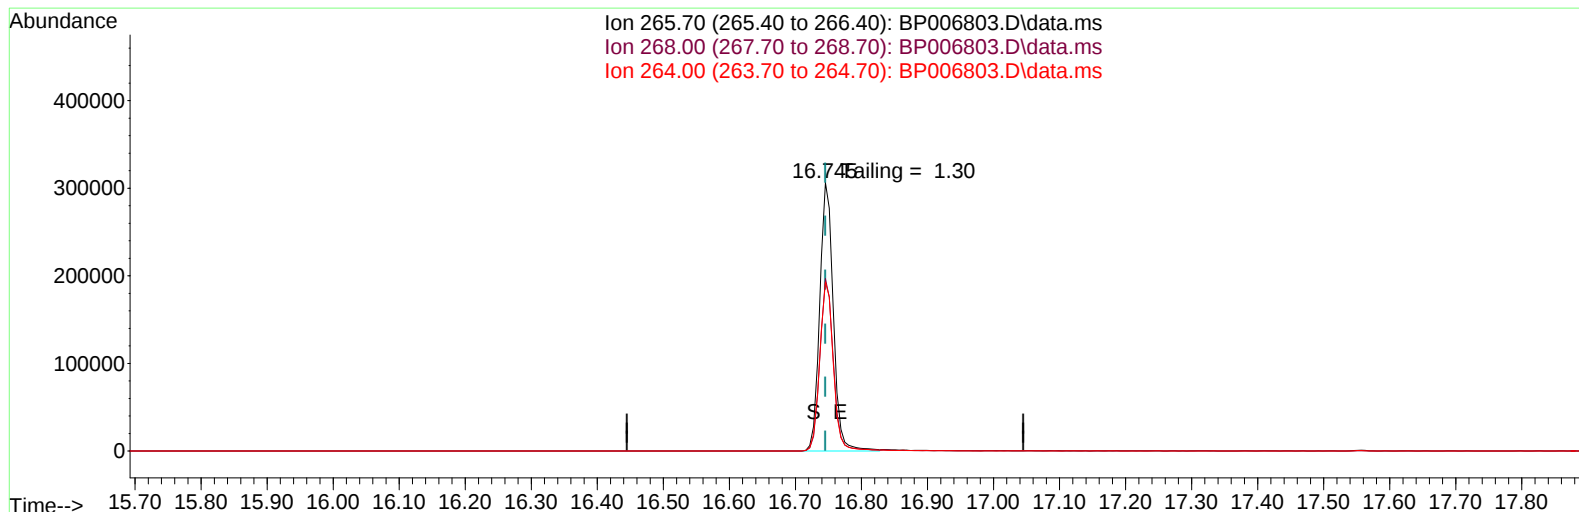

TIC: BP006803.D\data.ms

(70) Pentachlorophenol (C)

16.745min (+ 0.000) 1449037.93 ng




response 441698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.22
264.00	62.90	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082021\
 Data File : BP006803.D
 Acq On : 20 Aug 2021 16:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 21 04:39:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 11:25:25 2021
 Response via : Initial Calibration

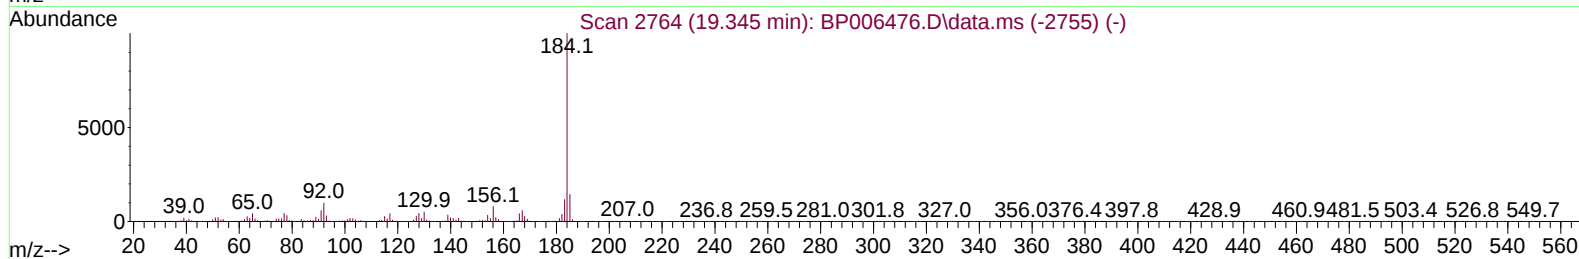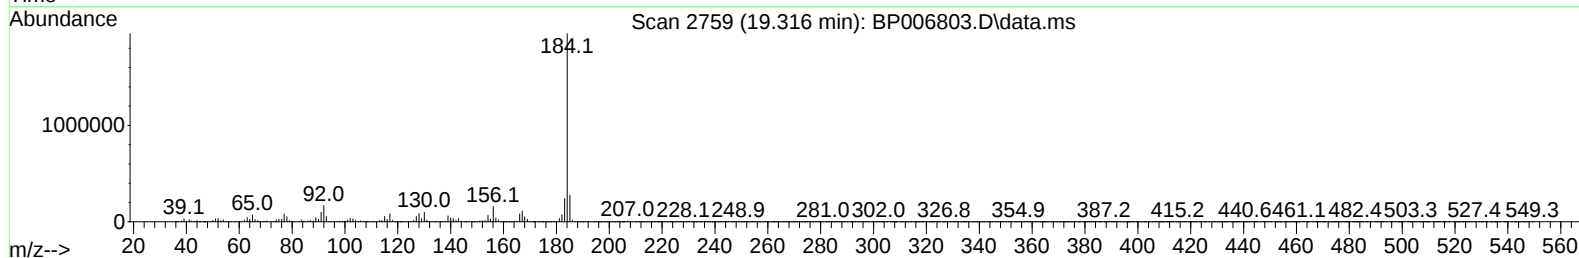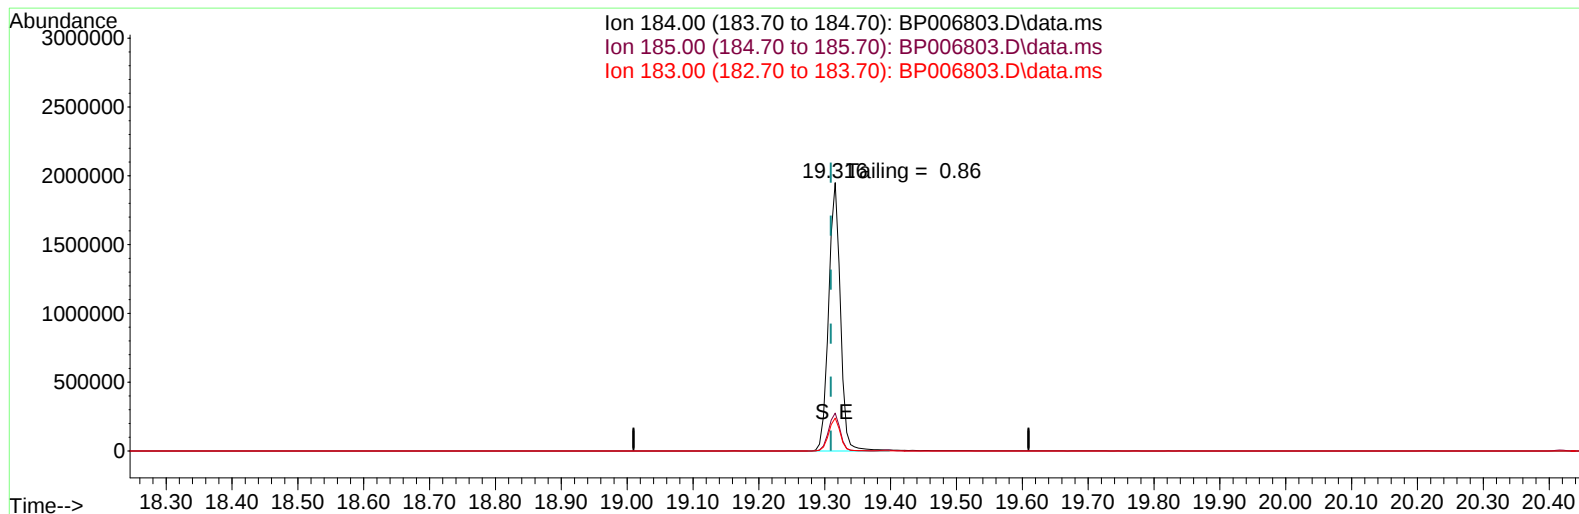

TIC: BP006803.D\data.ms

(77) Benzidine

19.316min (+ 0.006) 646139.55 ng

response 2425284

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.12
183.00	11.90	12.30
0.00	0.00	0.00

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2021	BNA_P	<u>BP006803.D</u>
Compound Name	Response	Retention Time
DDT	1231617	20.516
DDD	21363	20.086
DDE	2937	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24300	1255917	1.93