
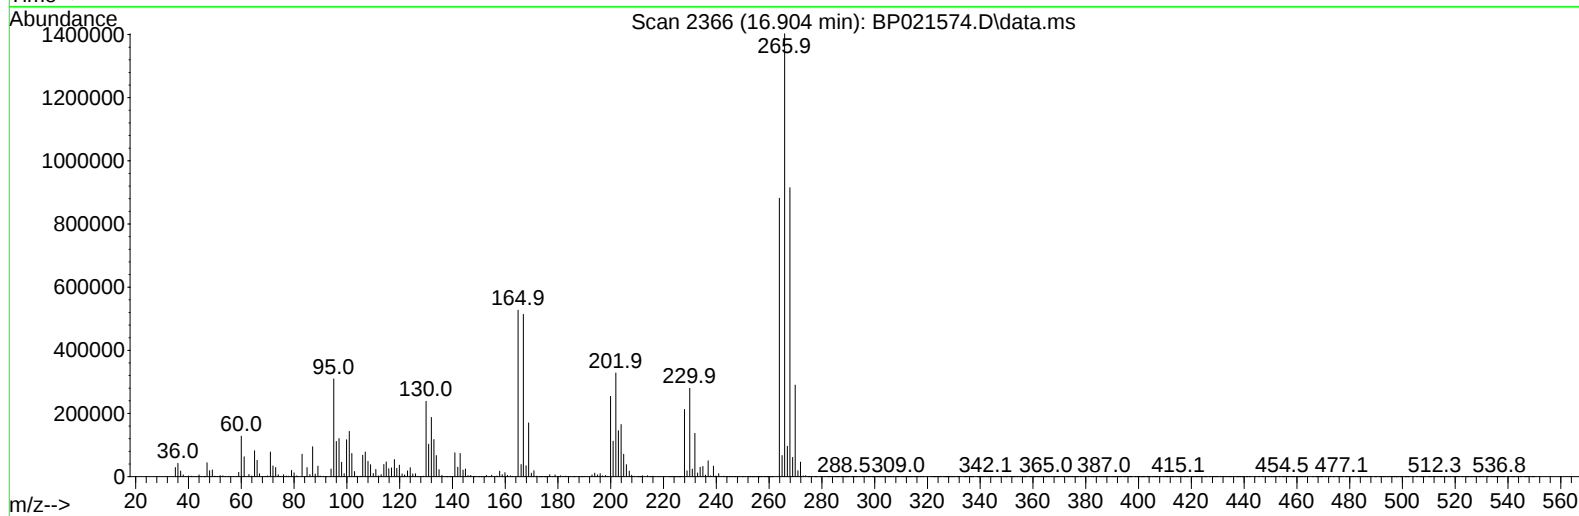


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021574.D
Acq On : 20 Aug 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 16:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

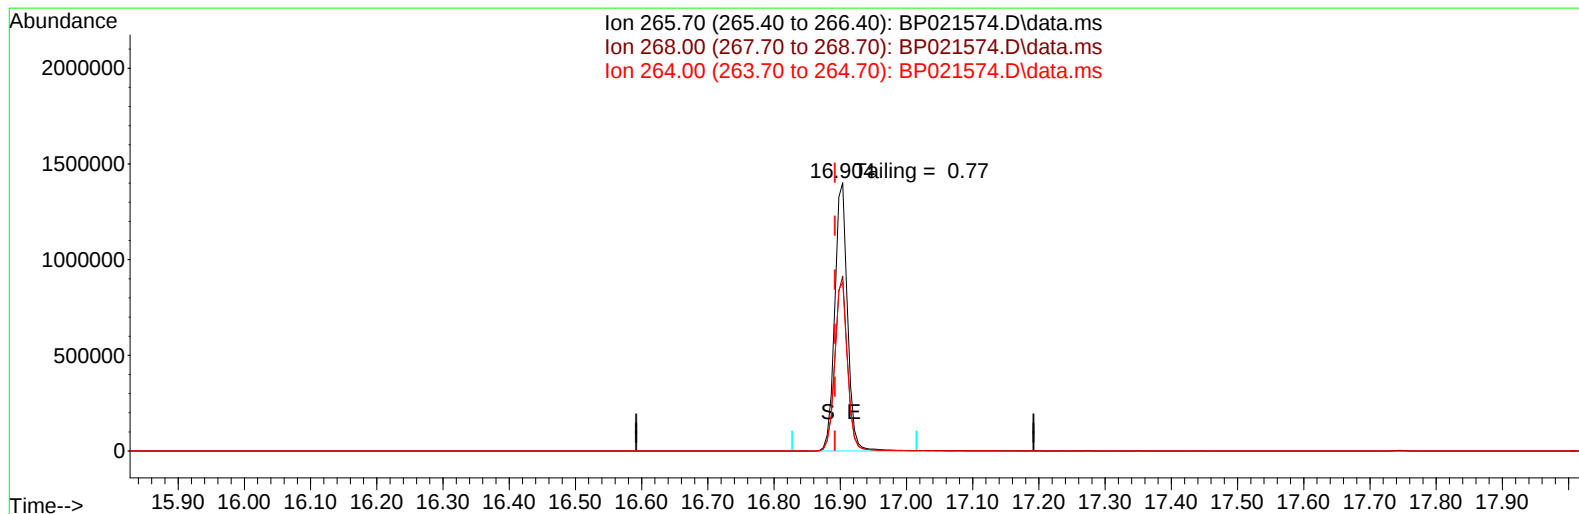

TIC: BP021574.D\data.ms

(70) Pentachlorophenol (C)



16.904min (+ 0.012) 1466831.19 ng

response 1882505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	65.26
264.00	63.10	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021574.D
Acq On : 20 Aug 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 16:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

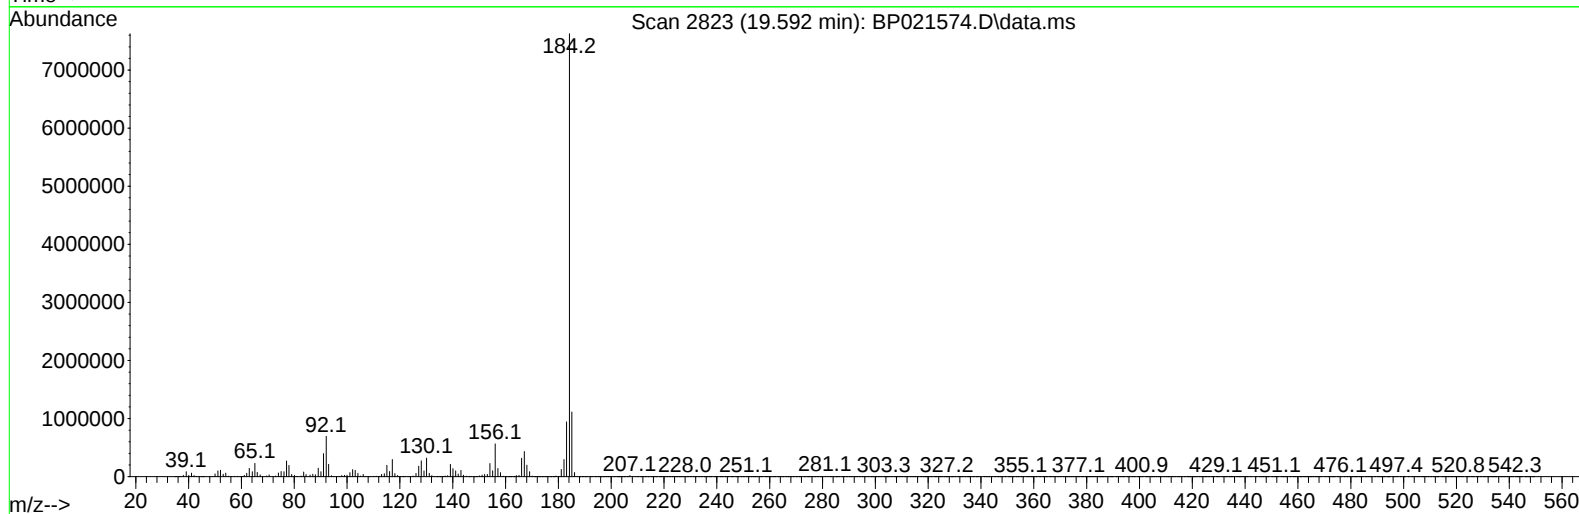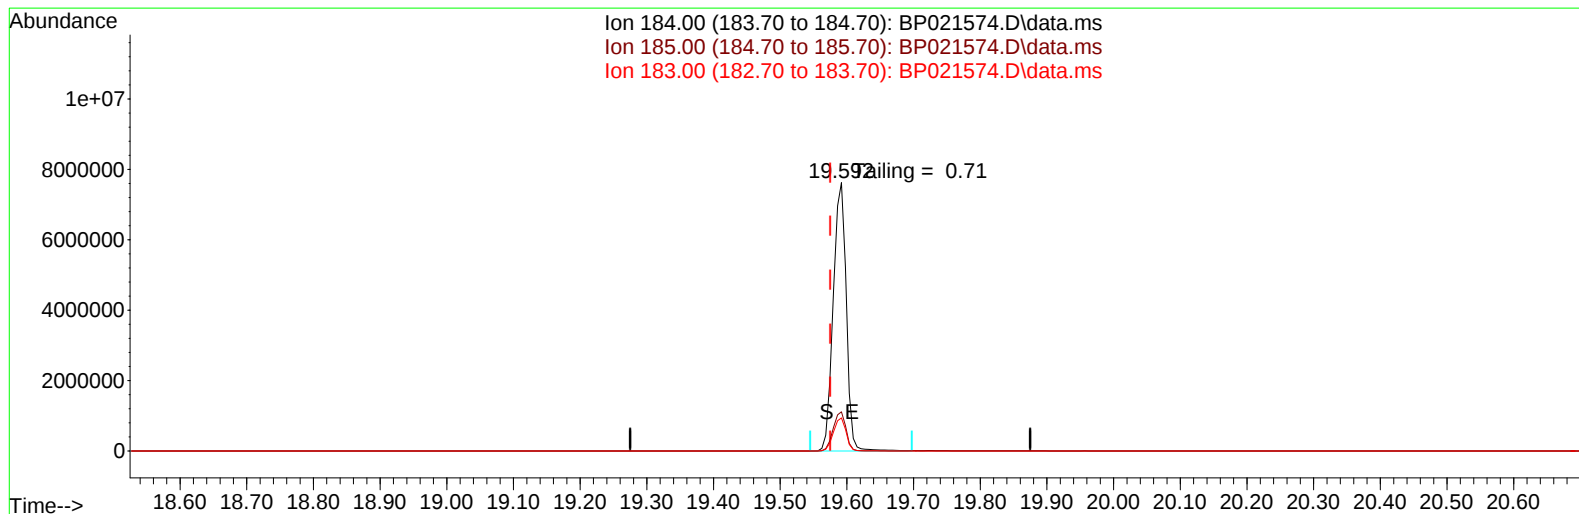

TIC: BP021574.D\data.ms

(77) Benzidine**19.592min (+ 0.017) -20.00 ng****response 10375641**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.60
183.00	11.60	12.36
0.00	0.00	0.00