
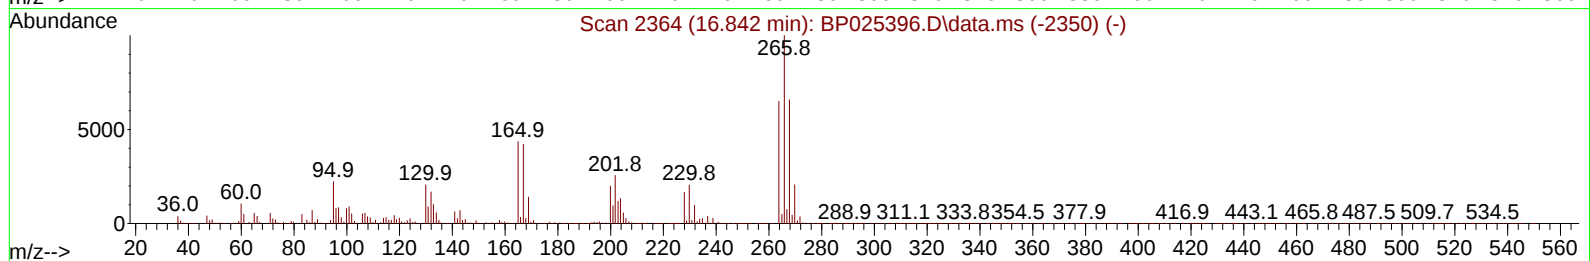
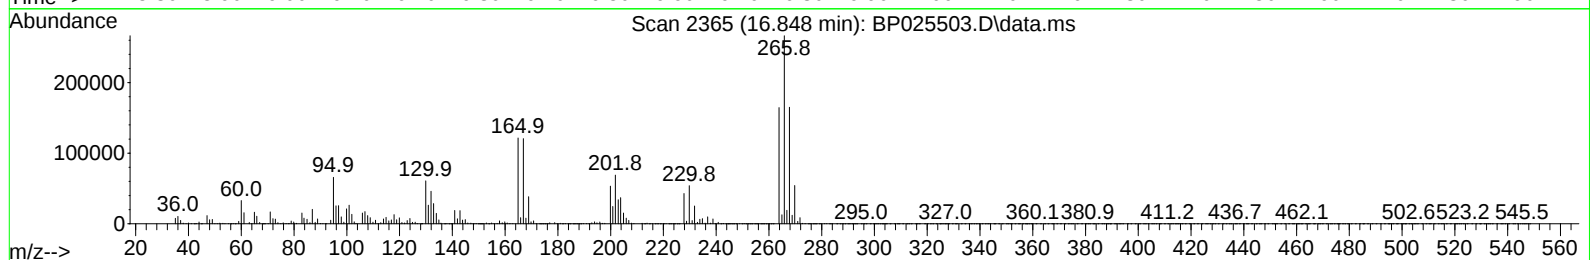


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025503.D
Acq On : 20 Aug 2025 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 12:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

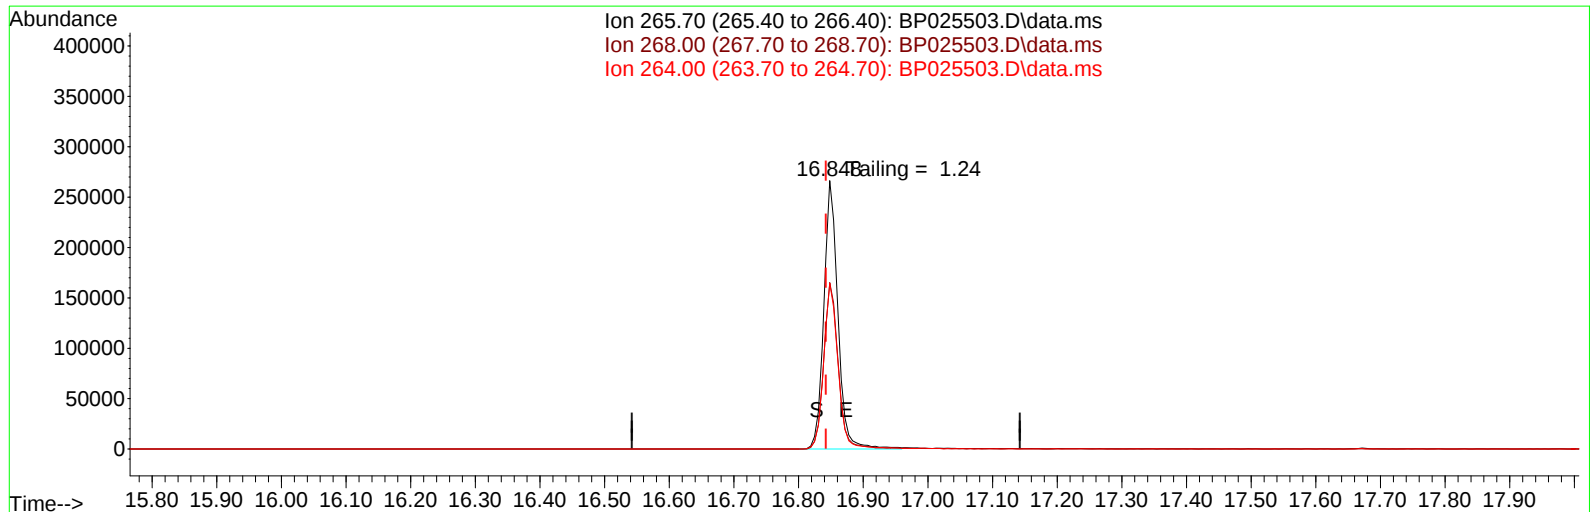

TIC: BP025503.D\data.ms

(70) Pentachlorophenol (C)




16.848min (+ 0.006) 11966.43 ng

response 406984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	61.99
264.00	65.00	61.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025503.D
Acq On : 20 Aug 2025 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 12:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

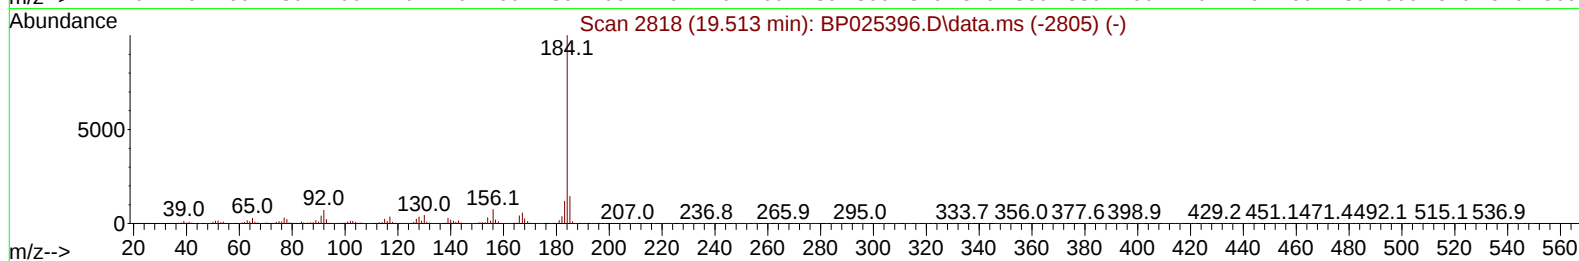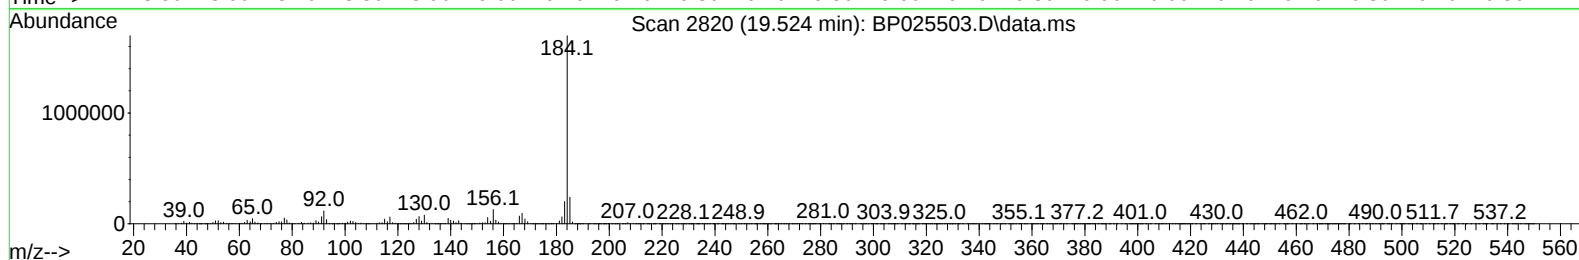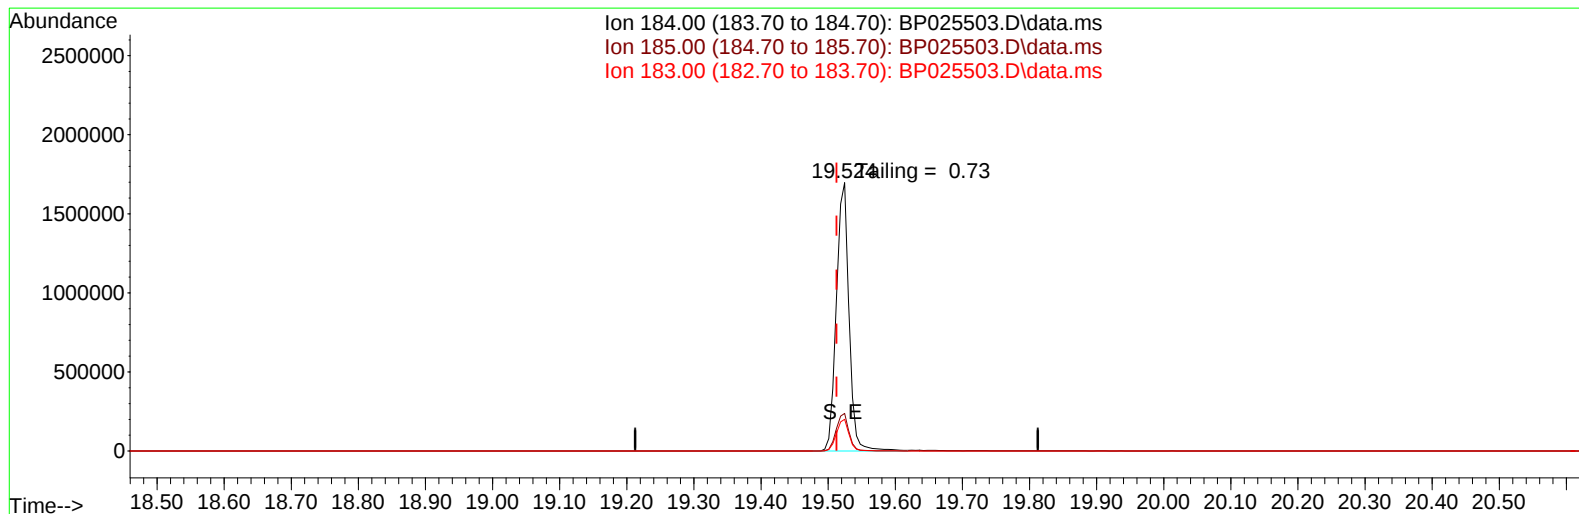

TIC: BP025503.D\data.ms

(77) Benzidine**19.524min (+ 0.012) 12639.84 ng****response 2228895**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.03
183.00	11.80	11.81
0.00	0.00	0.00