
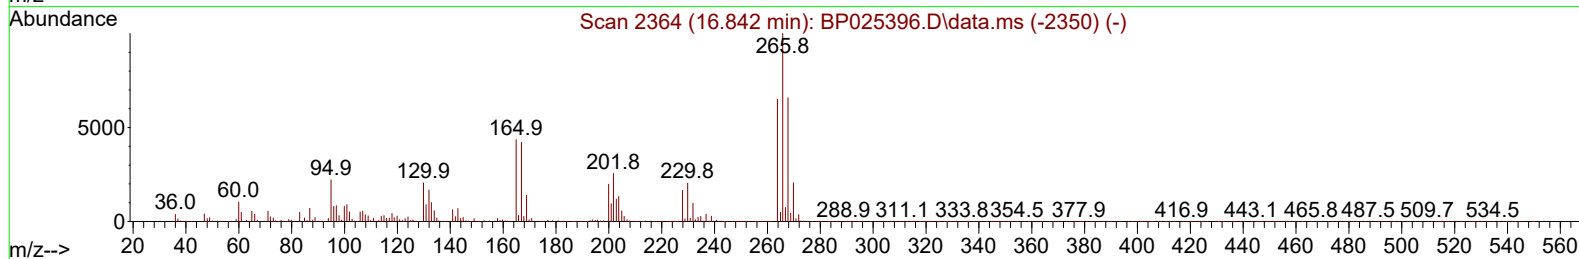
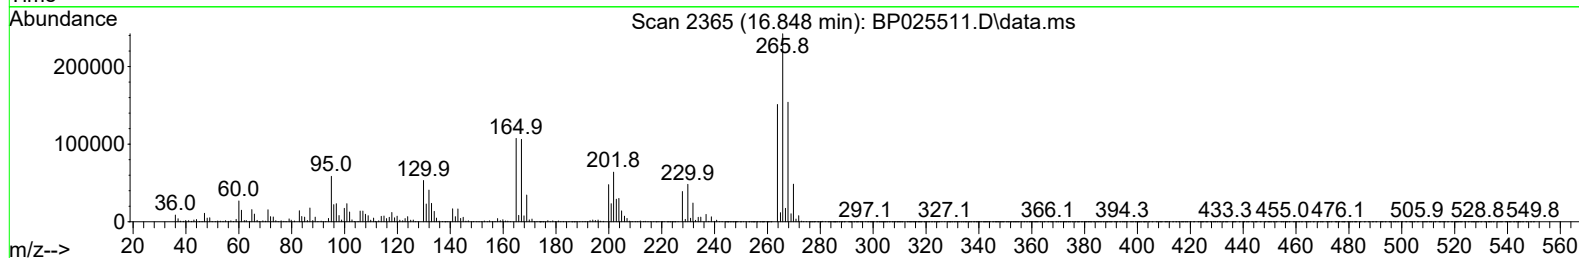


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025511.D
Acq On : 20 Aug 2025 17:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 01:41:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

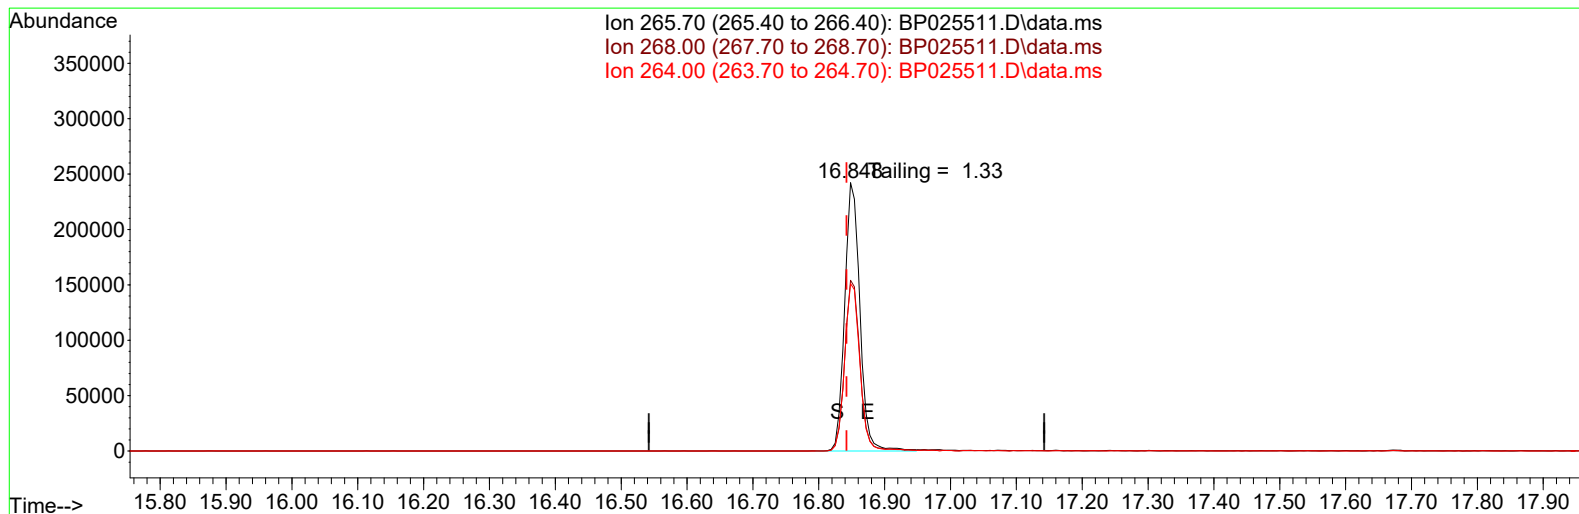

TIC: BP025511.D\data.ms

(70) Pentachlorophenol (C)




16.848min (+ 0.006) 19981.54 ng

response 390285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	63.60
264.00	65.00	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025511.D
Acq On : 20 Aug 2025 17:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 01:41:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

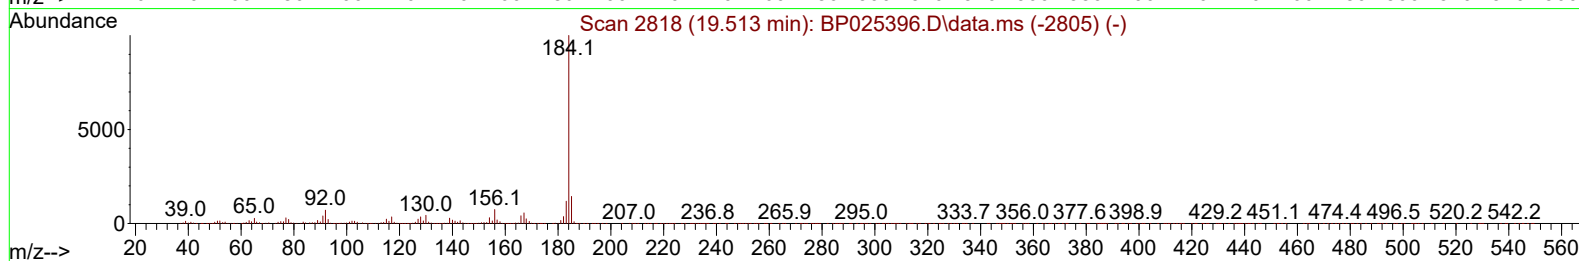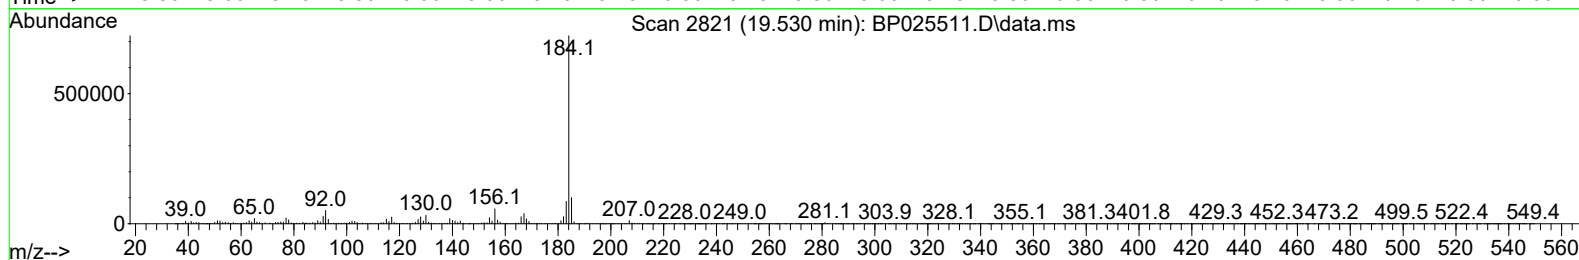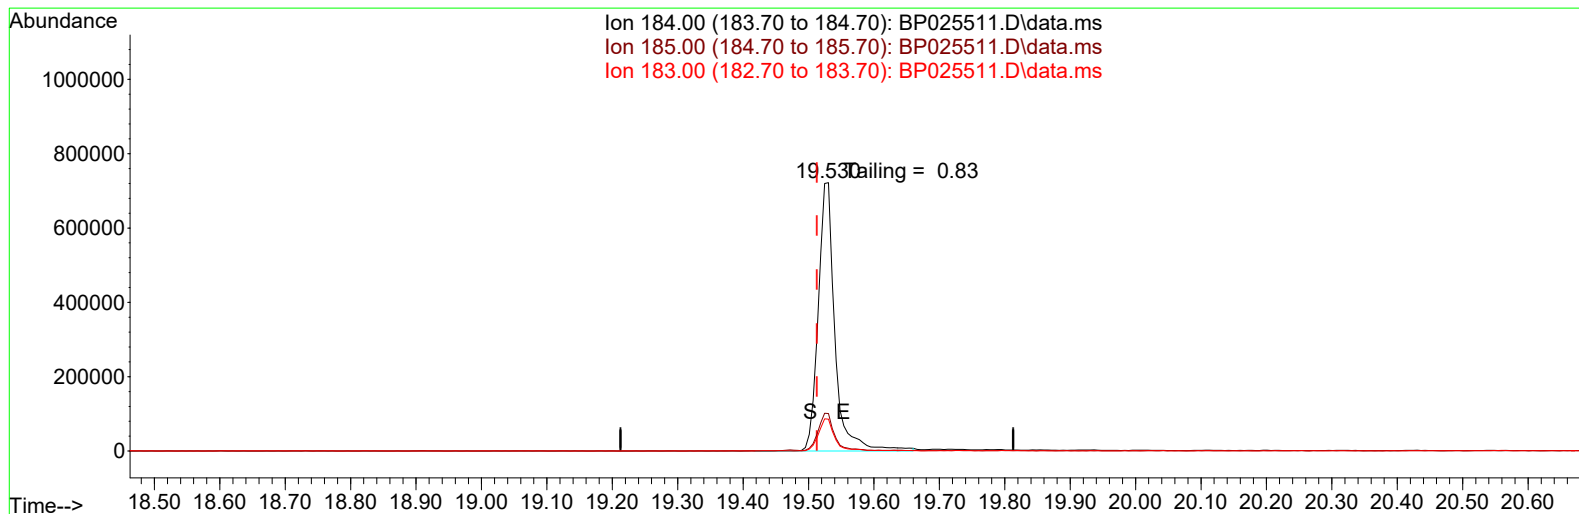

TIC: BP025511.D\data.ms

(77) Benzidine

19.530min (+ 0.018) 12499.23 ng

response 1286969

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	11.80	11.89
0.00	0.00	0.00