
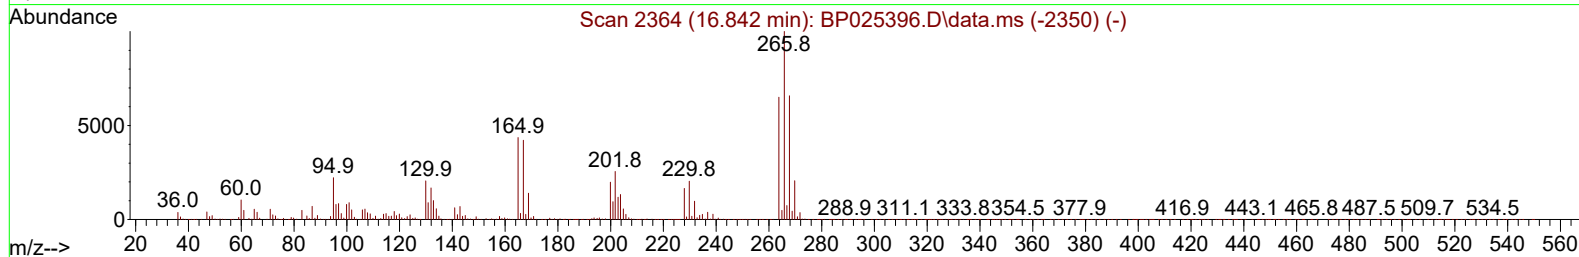
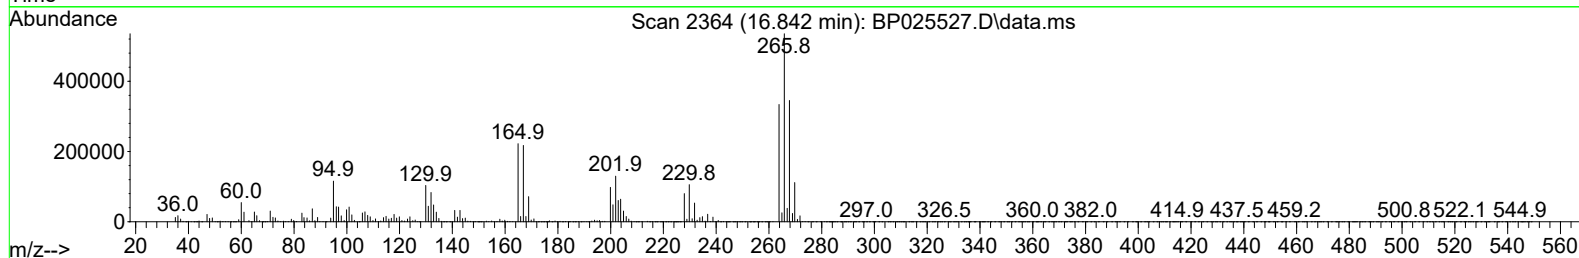


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025527.D
Acq On : 21 Aug 2025 05:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 21 06:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

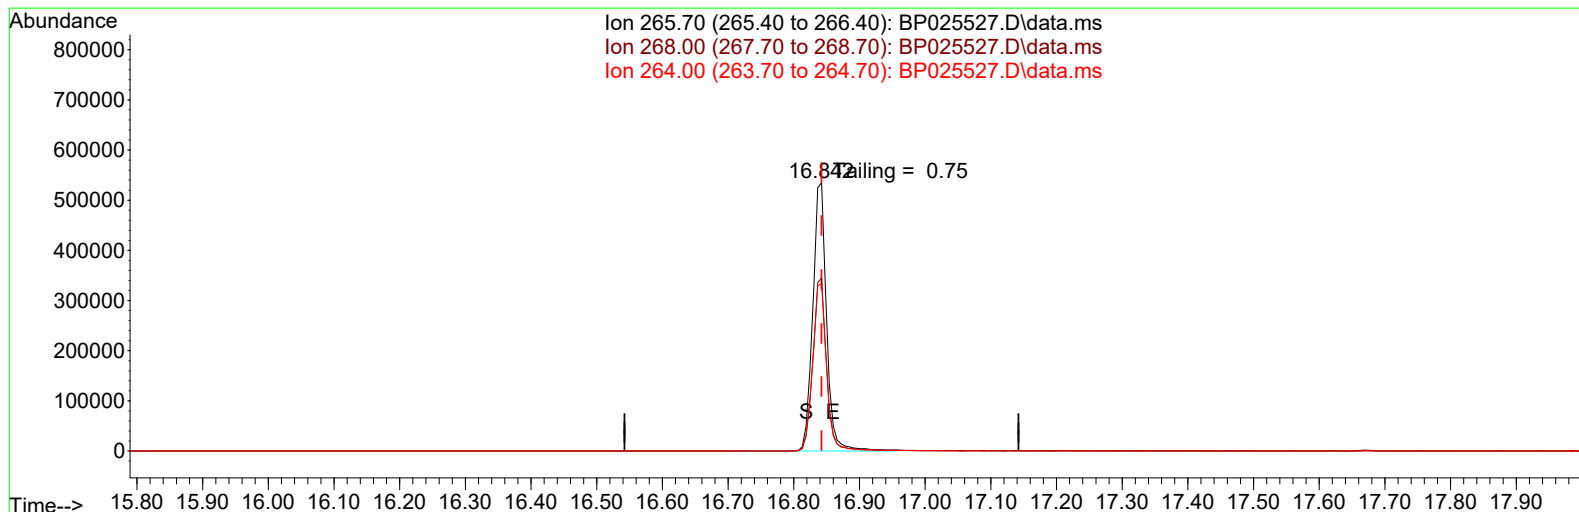

TIC: BP025527.D\data.ms

(70) Pentachlorophenol (C)




16.842min (+ 0.000) 14024.53 ng

response 784998

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.48
264.00	65.00	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025527.D
Acq On : 21 Aug 2025 05:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 21 06:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

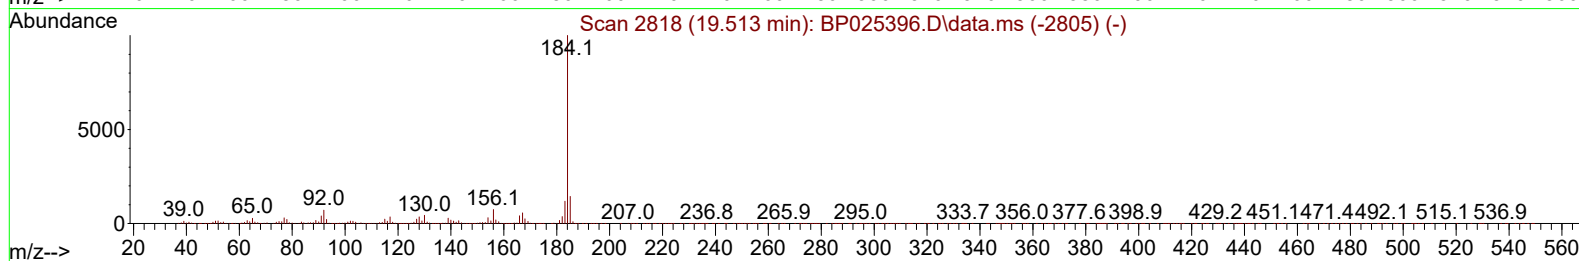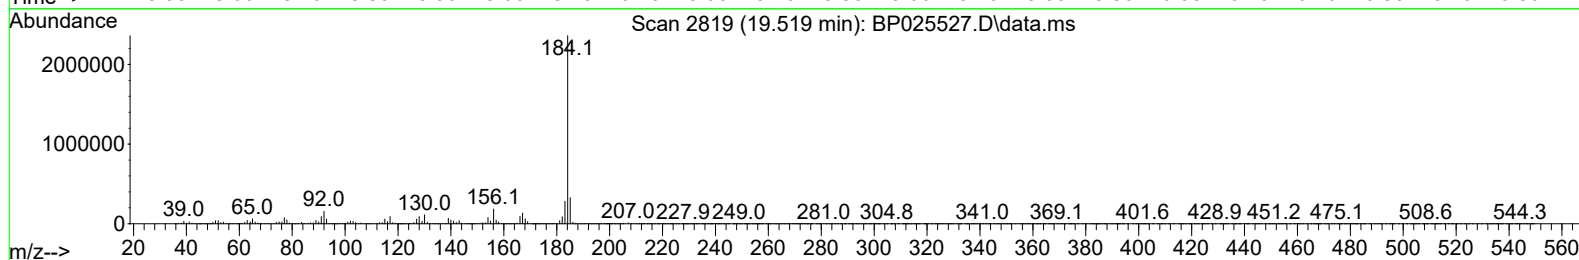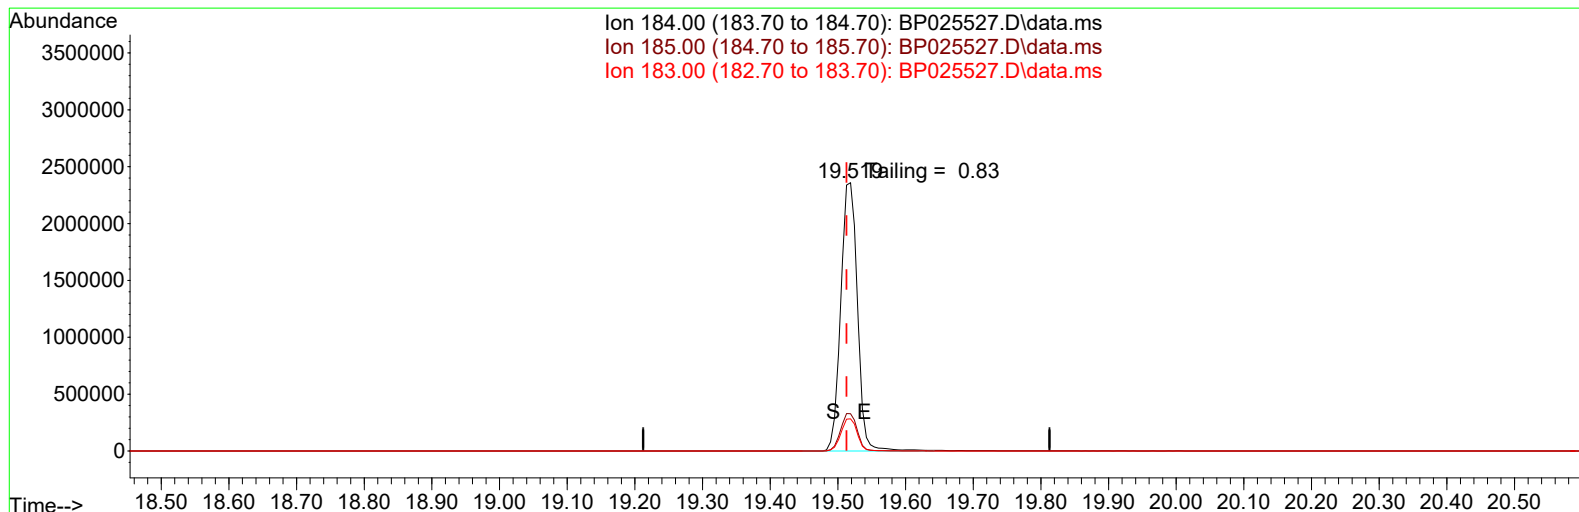

TIC: BP025527.D\data.ms

(77) Benzidine**19.519min (+ 0.006) 13689.91 ng****response 4033404**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.90
183.00	11.80	11.97
0.00	0.00	0.00