

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
 Data File : BP025509.D
 Acq On : 20 Aug 2025 15:34
 Operator : CG/JU
 Sample : Q2865-02 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ARS10-0047

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

Quant Time: Aug 20 15:58:33 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 14 18:14:31 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.784	152	168781	20.000	ng	-0.01
21) Naphthalene-d8	10.548	136	625274	20.000	ng	-0.01
39) Acenaphthene-d10	14.401	164	358397	20.000	ng	0.00
64) Phenanthrene-d10	17.195	188	672674	20.000	ng	0.00
76) Chrysene-d12	21.642	240	748470	20.000	ng	0.00
86) Perylene-d12	25.024	264	942424	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.402	112	152270	14.982	ng	0.00
7) Phenol-d6	6.960	99	202909	15.572	ng	0.00
23) Nitrobenzene-d5	8.919	82	129051	10.440	ng	-0.02
42) 2,4,6-Tribromophenol	15.907	330	76060	15.767	ng	0.00
45) 2-Fluorobiphenyl	13.013	172	272557	10.393	ng	0.00
79) Terphenyl-d14	19.919	244	388162	9.488	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	17.236	178	550040	14.885	ng	98
72) Anthracene	17.330	178	147024	3.896	ng	97
73) Carbazole	17.613	167	86880	2.444	ng	# 91
75) Fluoranthene	19.324	202	1058459	24.014	ng	97
78) Pyrene	19.701	202	866608	17.814	ng	99
81) Benzo(a)anthracene	21.624	228	463496	9.390	ng	97
83) Chrysene	21.683	228	541963	11.724	ng	95
84) Bis(2-ethylhexyl)phtha...	21.571	149	760632	23.436	ng	98
87) Indeno(1,2,3-cd)pyrene	28.853	276	346779	5.018	ng	92
88) Benzo(b)fluoranthene	23.954	252	748624	13.471	ng	# 90
89) Benzo(k)fluoranthene	24.024	252	240648m	4.327	ng	
90) Benzo(a)pyrene	24.865	252	427435	7.902	ng	# 87
92) Benzo(g,h,i)perylene	30.053	276	328540	5.918	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025509.D
Acq On : 20 Aug 2025 15:34
Operator : CG/JU
Sample : Q2865-02 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
ARS10-0047

Quant Time: Aug 20 15:58:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

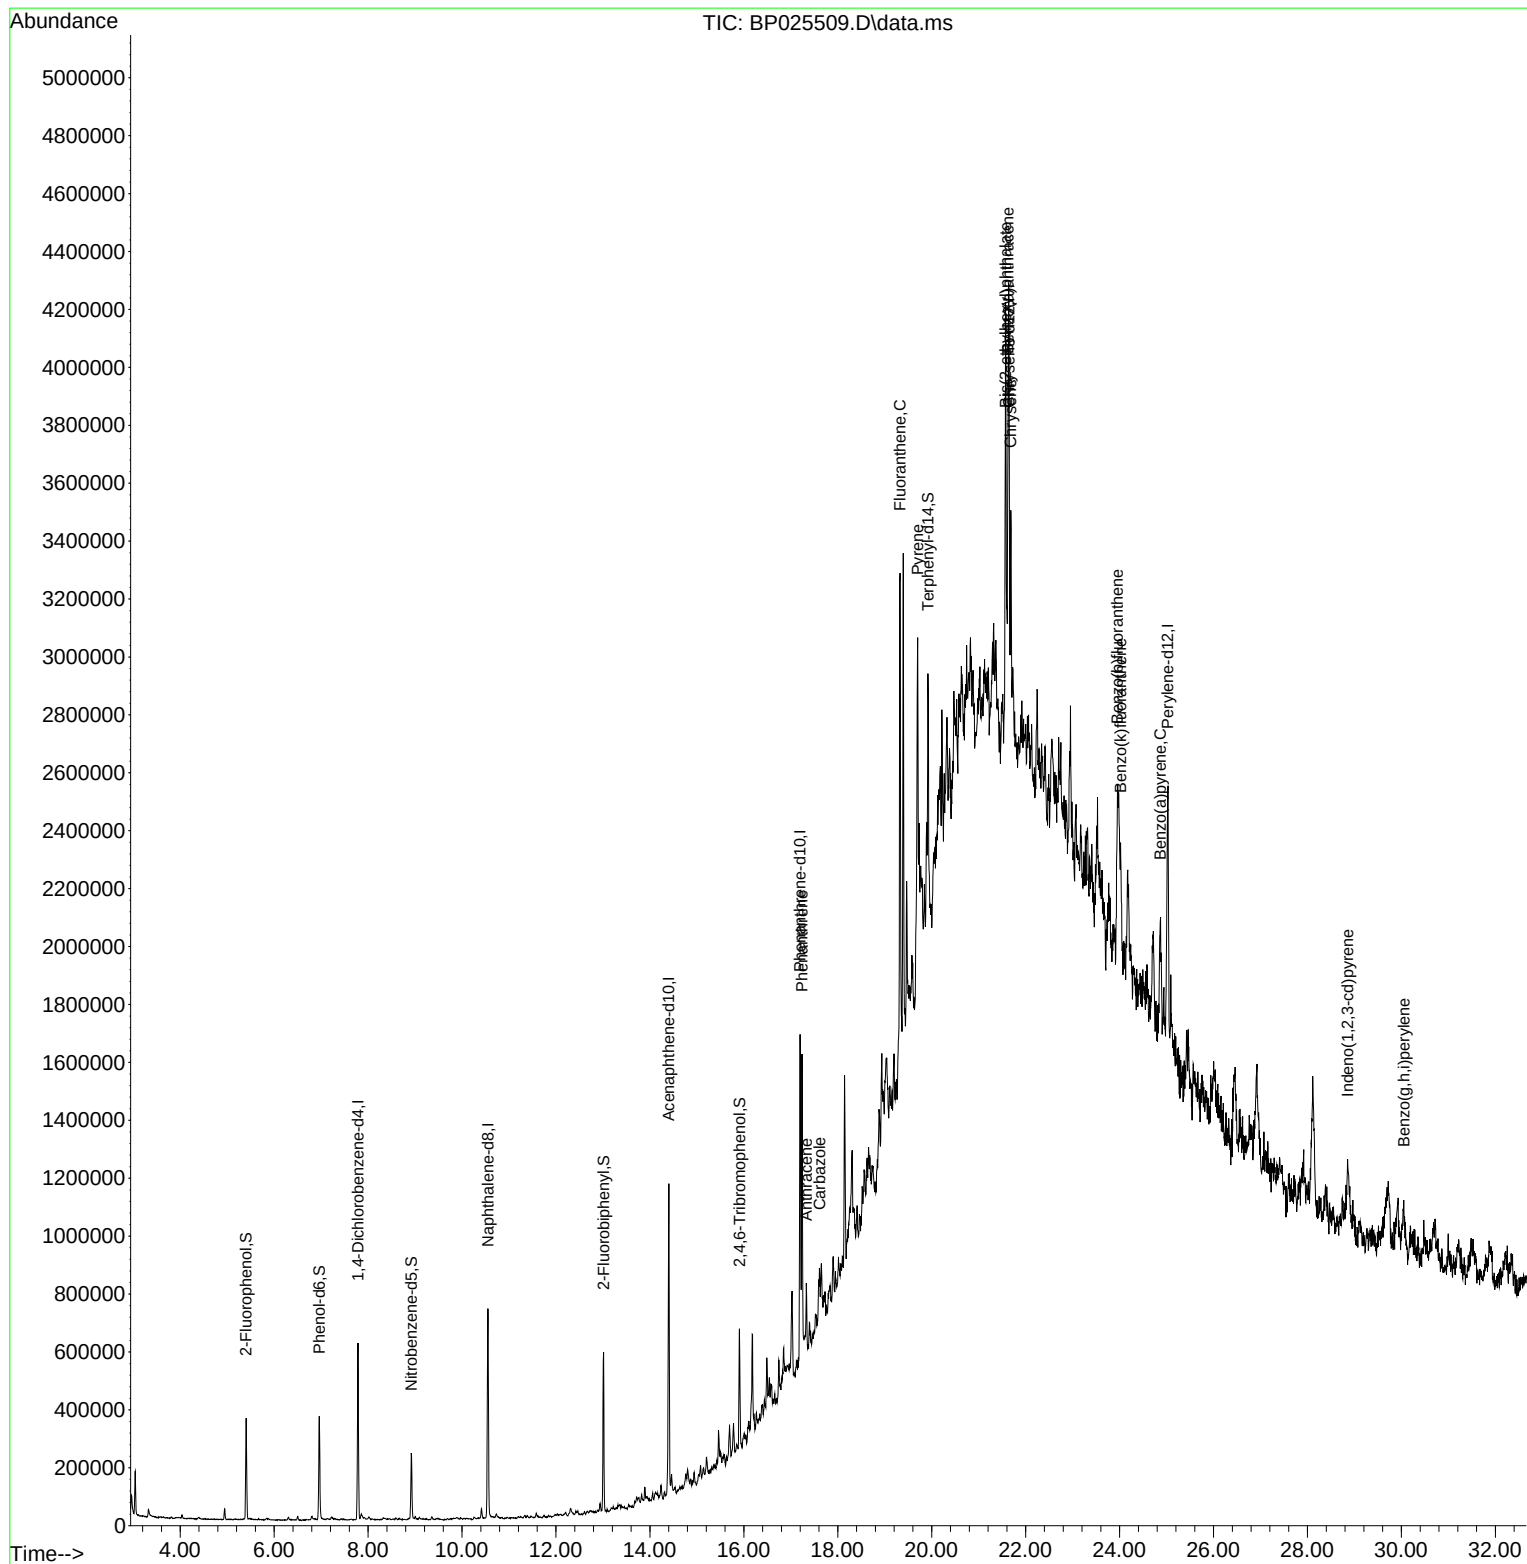



#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.784 min Scan# 81
 Delta R.T. -0.012 min
 Lab File: BP025509.D
 Acq: 20 Aug 2025 15:34




Instrument :
 BNA_P
 ClientSampleId :
 ARS10-0047




Tgt Ion:152 Resp: 16878
 Ion Ratio Lower Upper
 152 100
 150 157.9 125.9 188.9
 115 63.3 48.5 72.7

Manual Integrations
 APPROVED



Reviewed By :Rahul Chavli 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

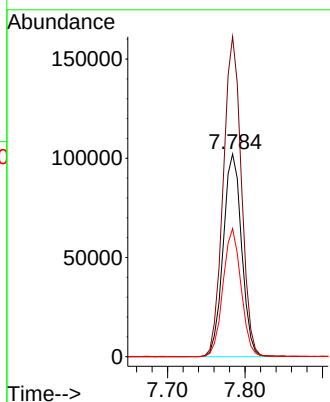


#5
 2-Fluorophenol
 Concen: 14.982 ng
 RT: 5.402 min Scan# 419
 Delta R.T. -0.006 min
 Lab File: BP025509.D
 Acq: 20 Aug 2025 15:34




Tgt Ion:112 Resp: 152270
 Ion Ratio Lower Upper
 112 100
 64 57.7 43.8 65.8
 63 31.2 22.7 34.1

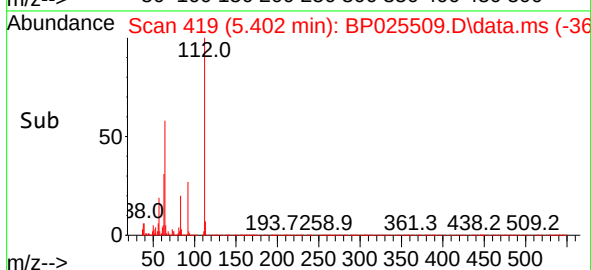



#7
Phenol-d6
Concen: 15.572 ng
RT: 6.960 min Scan# 685
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Instrument :
BNA_P
ClientSampleId :
ARS10-0047




Tgt Ion: 99 Resp: 202909
Ion Ratio Lower Upper
99 100
42 17.2 13.7 20.5
71 36.8 28.2 42.4

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

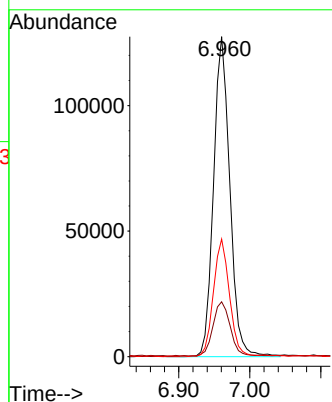


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.548 min Scan# 1294
Delta R.T. -0.012 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Tgt Ion:136 Resp: 625274
Ion Ratio Lower Upper
136 100
137 10.9 9.2 13.8
54 8.1 6.0 9.0
68 5.9 4.3 6.5

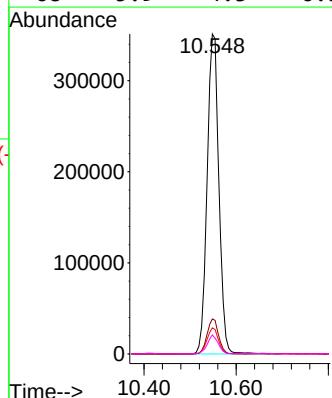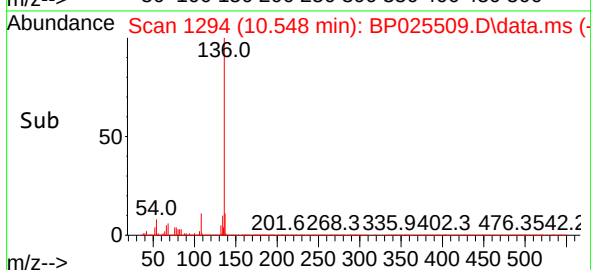



#23
Nitrobenzene-d5
Concen: 10.440 ng
RT: 8.919 min Scan# 1020
Delta R.T. -0.018 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Instrument :
BNA_P
ClientSampleId :
ARS10-0047




Tgt Ion: 82 Resp: 12905
Ion Ratio Lower Upper
82 100
128 44.5 37.7 56.5
54 53.2 39.8 59.6

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.401 min Scan# 1949
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Tgt Ion:164 Resp: 358397
Ion Ratio Lower Upper
164 100
162 101.9 81.0 121.6
160 45.0 35.4 53.2

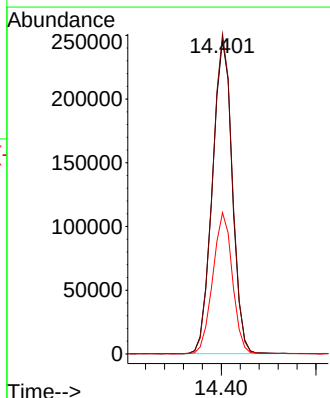



#42
2,4,6-Tribromophenol
Concen: 15.767 ng
RT: 15.907 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Instrument :
BNA_P
ClientSampleId :
ARS10-0047



Tgt Ion:330 Resp: 76060
Ion Ratio Lower Upper
330 100
332 96.9 77.3 115.9
141 35.1 26.6 39.8




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

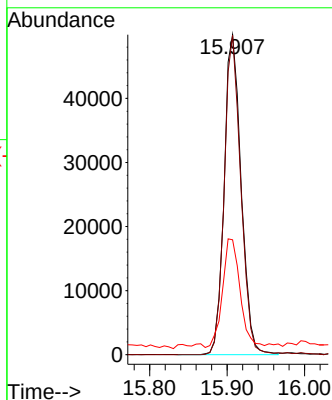

#45
2-Fluorobiphenyl
Concen: 10.393 ng
RT: 13.013 min Scan# 1713
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34

Tgt Ion:172 Resp: 272557
Ion Ratio Lower Upper
172 100
171 33.8 28.1 42.1
170 22.6 18.6 28.0

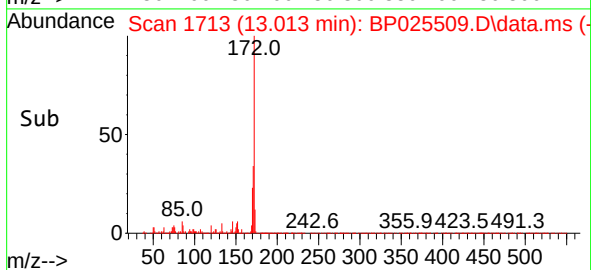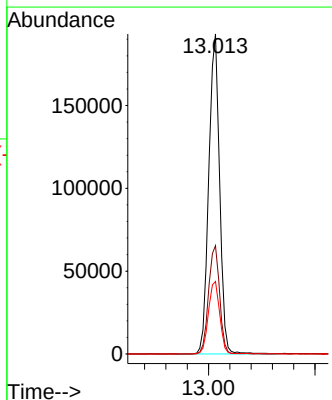







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.195 min Scan# 2425
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34

Instrument :
BNA_P
ClientSampleId :
ARS10-0047

Tgt Ion:188 Resp: 672674
Ion Ratio Lower Upper
188 100
94 9.1 6.6 10.0
80 9.8 6.7 10.1




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

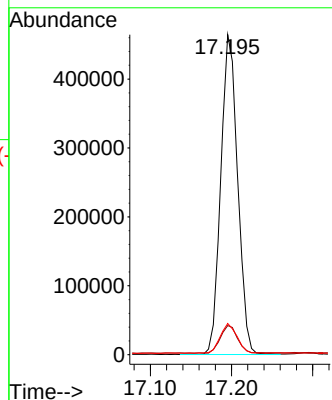

#71
Phenanthrene
Concen: 14.885 ng
RT: 17.236 min Scan# 2431
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34

Tgt Ion:178 Resp: 550040
Ion Ratio Lower Upper
178 100
176 18.6 15.5 23.3
179 16.6 12.2 18.4

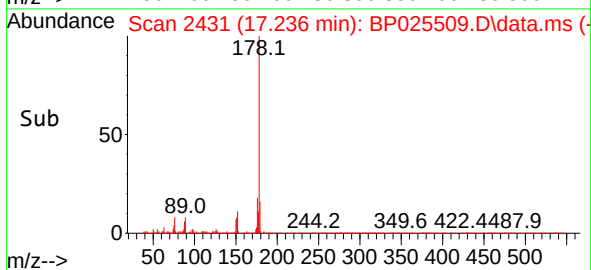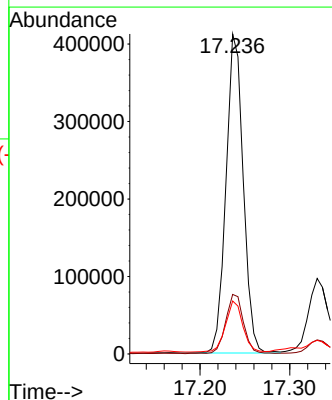

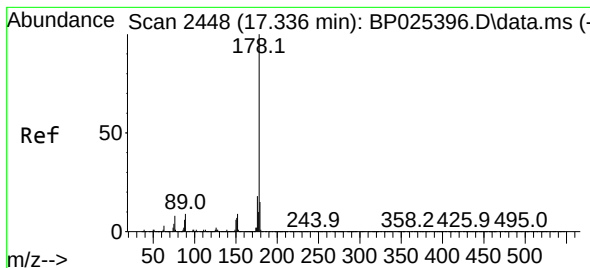

#72

Anthracene

Concen: 3.896 ng

RT: 17.330 min Scan# 2448

Delta R.T. -0.006 min

Lab File: BP025509.D

Acq: 20 Aug 2025 15:34

Instrument :

BNA_P

ClientSampleId :

ARS10-0047





Tgt Ion:178	Resp: 147024
Ion Ratio	Lower Upper
178 100	
176 18.6	14.7 22.1
179 18.1	12.2 18.2

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/21/2025

Supervised By :mohammad ahmed 08/22/2025

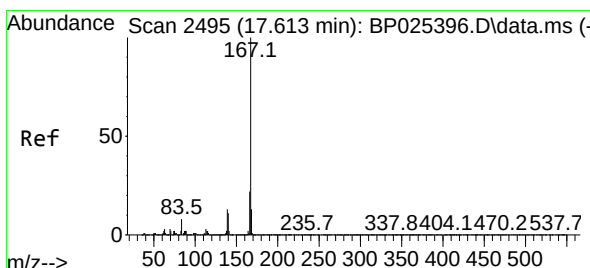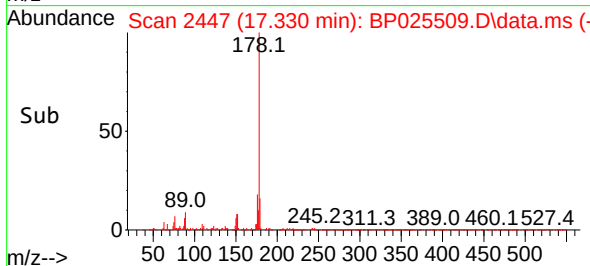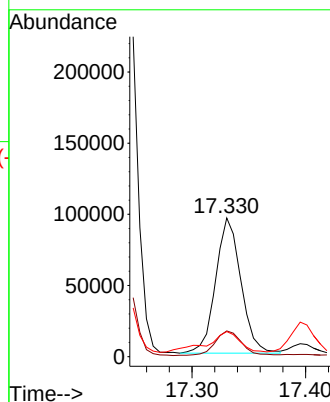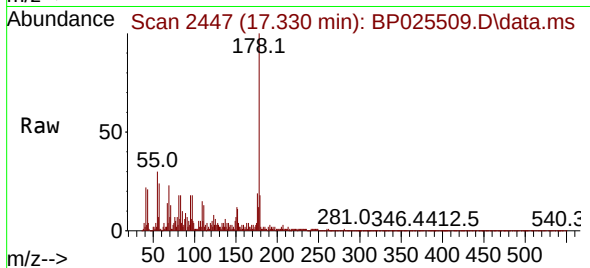

#73

Carbazole

Concen: 2.444 ng




RT: 17.613 min Scan# 2495


Delta R.T. 0.000 min

Lab File: BP025509.D

Acq: 20 Aug 2025 15:34


Tgt Ion:167	Resp: 86880
Ion Ratio	Lower Upper
167 100	
166 25.5	17.5 26.3
139 18.4	10.6 16.0

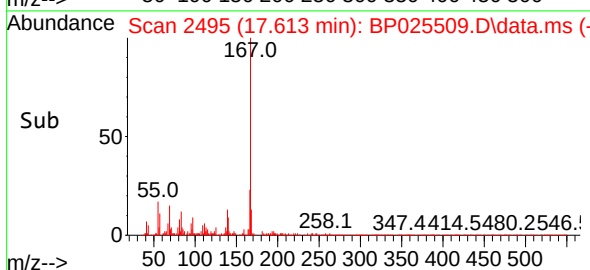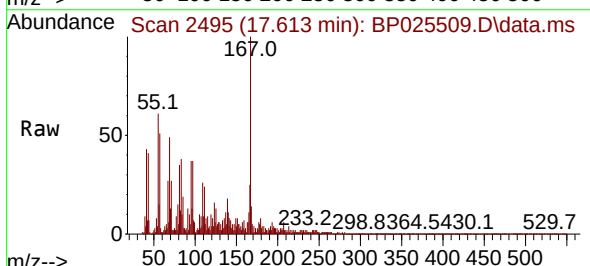



#75
Fluoranthene
Concen: 24.014 ng
RT: 19.324 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Instrument :
BNA_P
ClientSampleId :
ARS10-0047



Tgt Ion:202 Resp: 105845
Ion Ratio Lower Upper
202 100
101 9.7 0.0 31.1
203 18.1 0.0 37.3




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

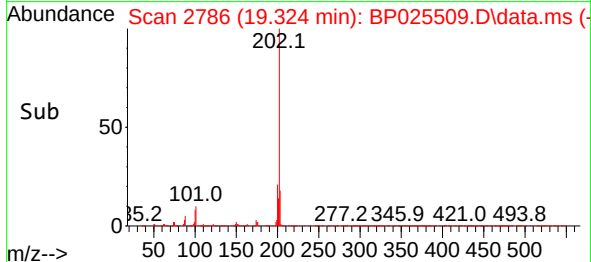

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.642 min Scan# 3180
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34

Tgt Ion:240 Resp: 748470
Ion Ratio Lower Upper
240 100
120 10.0 8.9 13.3
236 26.6 19.8 29.8

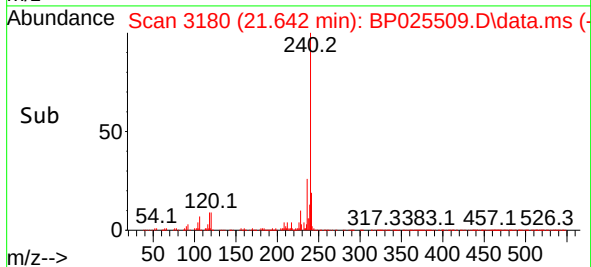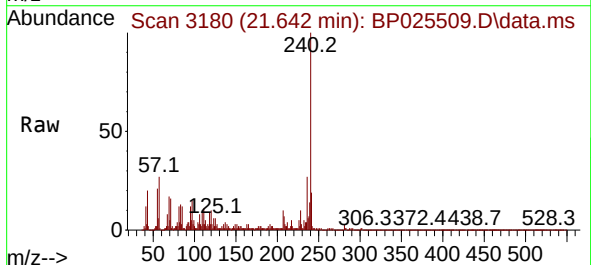



#78

Pyrene

Concen: 17.814 ng

RT: 19.701 min Scan# 2850

Delta R.T. 0.000 min

Lab File: BP025509.D

Acq: 20 Aug 2025 15:34

Instrument :

BNA_P

ClientSampleId :





ARS10-0047

Tgt Ion:	202	Resp:	866608
Ion Ratio	Lower	Upper	
202	100		
200	20.3	16.9	25.3
203	17.9	14.2	21.2

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025



#79

Terphenyl-d14

Concen: 9.488 ng




RT: 19.919 min Scan# 2887


Delta R.T. 0.000 min

Lab File: BP025509.D

Acq: 20 Aug 2025 15:34


Tgt Ion:	244	Resp:	388162
Ion Ratio	Lower	Upper	
244	100		
212	8.1	5.8	8.6
122	12.3	7.4	11.2

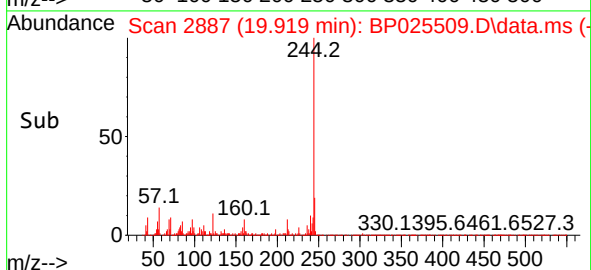

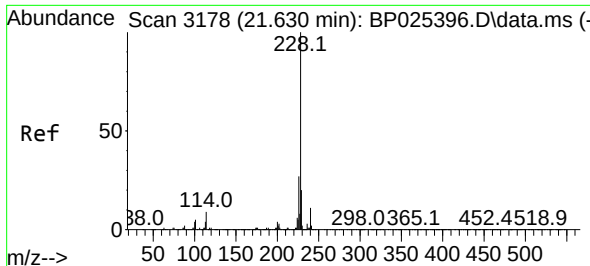

#81
Benzo(a)anthracene
Concen: 9.390 ng
RT: 21.624 min Scan# 3177
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Instrument :
BNA_P
ClientSampleId :
ARS10-0047

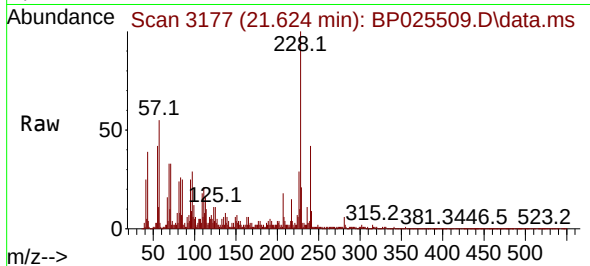

Tgt Ion:228 Resp: 463490
Ion Ratio Lower Upper
228 100
226 28.7 21.7 32.5
229 21.3 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

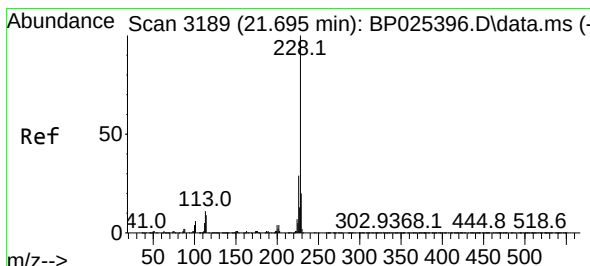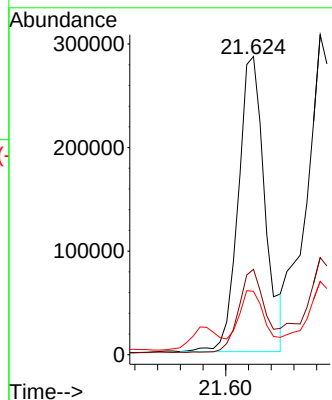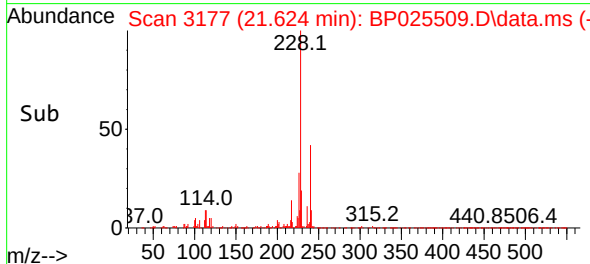

#83
Chrysene
Concen: 11.724 ng
RT: 21.683 min Scan# 3187
Delta R.T. -0.012 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34

Tgt Ion:228 Resp: 541963
Ion Ratio Lower Upper
228 100
226 30.4 23.2 34.8
229 22.9 15.6 23.4

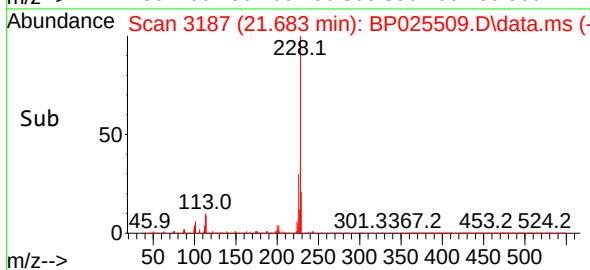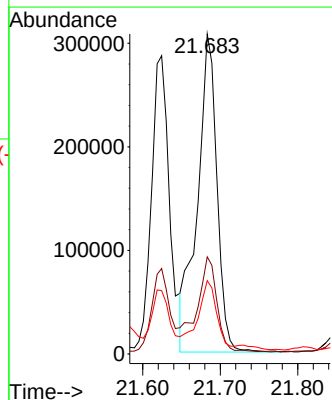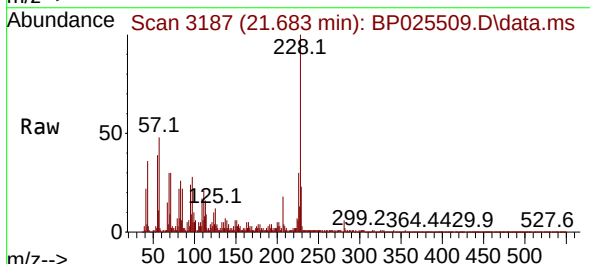



#84

Bis(2-ethylhexyl)phthalate

Concen: 23.436 ng

RT: 21.571 min Scan# 31

Delta R.T. -0.012 min

Lab File: BP025509.D

Acq: 20 Aug 2025 15:34

Instrument :

BNA_P

ClientSampleId :

ARS10-0047





Tgt Ion:	149	Resp:	76063
Ion Ratio	Lower	Upper	
149	100		
167	28.7	22.1	33.1
279	4.9	3.8	5.6

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/21/2025

Supervised By :mohammad ahmed 08/22/2025



#86

Perylene-d12

Concen: 20.000 ng




RT: 25.024 min Scan# 3755


Delta R.T. -0.006 min

Lab File: BP025509.D

Acq: 20 Aug 2025 15:34


Tgt Ion:	264	Resp:	942424
Ion Ratio	Lower	Upper	
264	100		
260	23.7	19.3	28.9
265	22.9	17.4	26.0

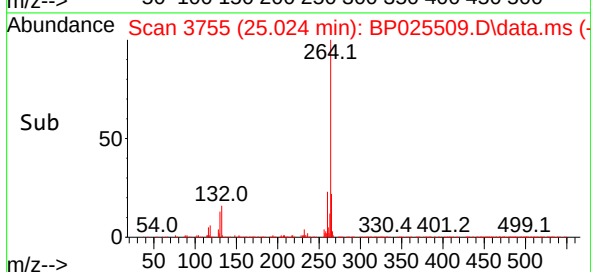



#87
Indeno(1,2,3-cd)pyrene
Concen: 5.018 ng
RT: 28.853 min Scan# 4408
Delta R.T. -0.012 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Instrument :
BNA_P
ClientSampleId :
ARS10-0047



Tgt Ion: 276 Resp: 346779
Ion Ratio Lower Upper
276 100
138 19.3 12.9 19.3
277 25.4 17.0 25.6




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025



#88
Benzo(b)fluoranthene
Concen: 13.471 ng
RT: 23.954 min Scan# 3573
Delta R.T. 0.000 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34


Tgt Ion: 252 Resp: 748624
Ion Ratio Lower Upper
252 100
253 23.8 17.7 26.5
125 18.9 7.9 11.9#

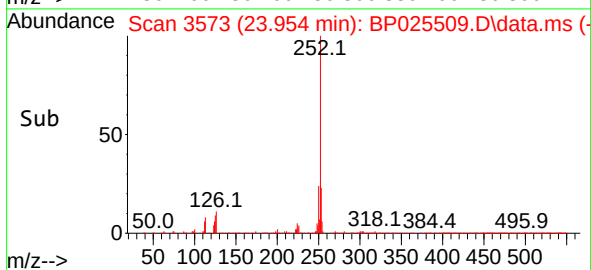



#89
Benzo(k)fluoranthene
Concen: 4.327 ng m
RT: 24.024 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34




Instrument :
BNA_P
ClientSampleId :
ARS10-0047



Tgt Ion:252 Resp: 24064
Ion Ratio Lower Upper
252 100
253 27.4 17.1 25.7
125 24.9 7.8 11.6




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

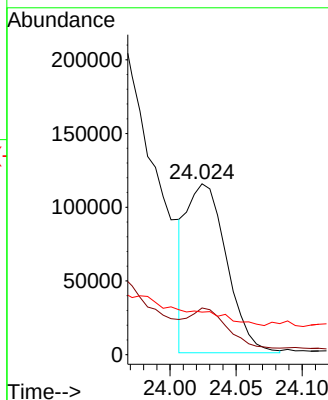

#90
Benzo(a)pyrene
Concen: 7.902 ng
RT: 24.865 min Scan# 3728
Delta R.T. 0.012 min
Lab File: BP025509.D
Acq: 20 Aug 2025 15:34


Tgt Ion:252 Resp: 427435
Ion Ratio Lower Upper
252 100
253 24.8 17.5 26.3
125 20.9 8.7 13.1

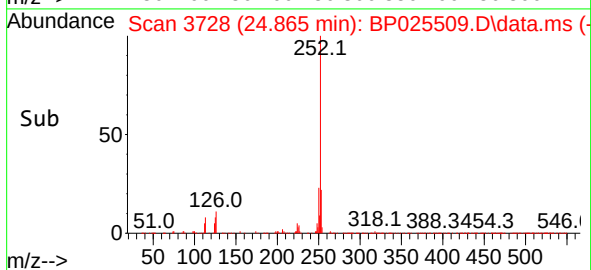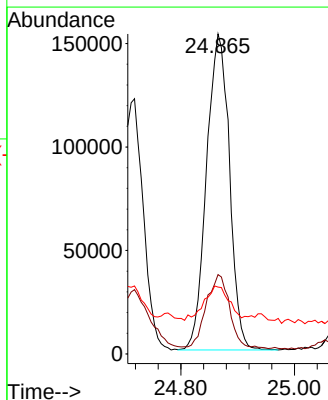

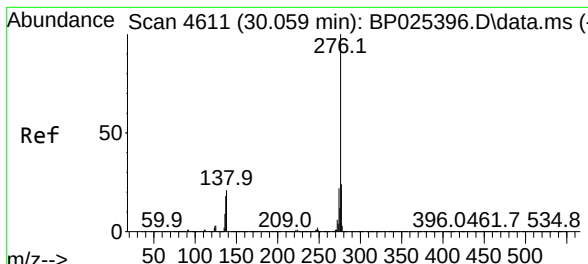

#92
 Benzo(g,h,i)perylene
 Concen: 5.918 ng
 RT: 30.053 min Scan# 40
 Delta R.T. -0.006 min
 Lab File: BP025509.D
 Acq: 20 Aug 2025 15:34

Instrument :
 BNA_P
 ClientSampleId :
 ARS10-0047

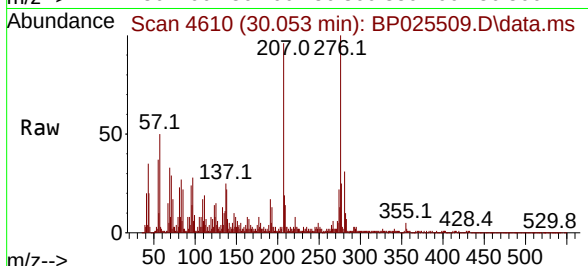

Tgt Ion: 276 Resp: 328540
 Ion Ratio Lower Upper
 276 100
 277 24.7 19.4 29.0
 138 22.0 16.7 25.1

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

