


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025503.D
Acq On : 20 Aug 2025 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

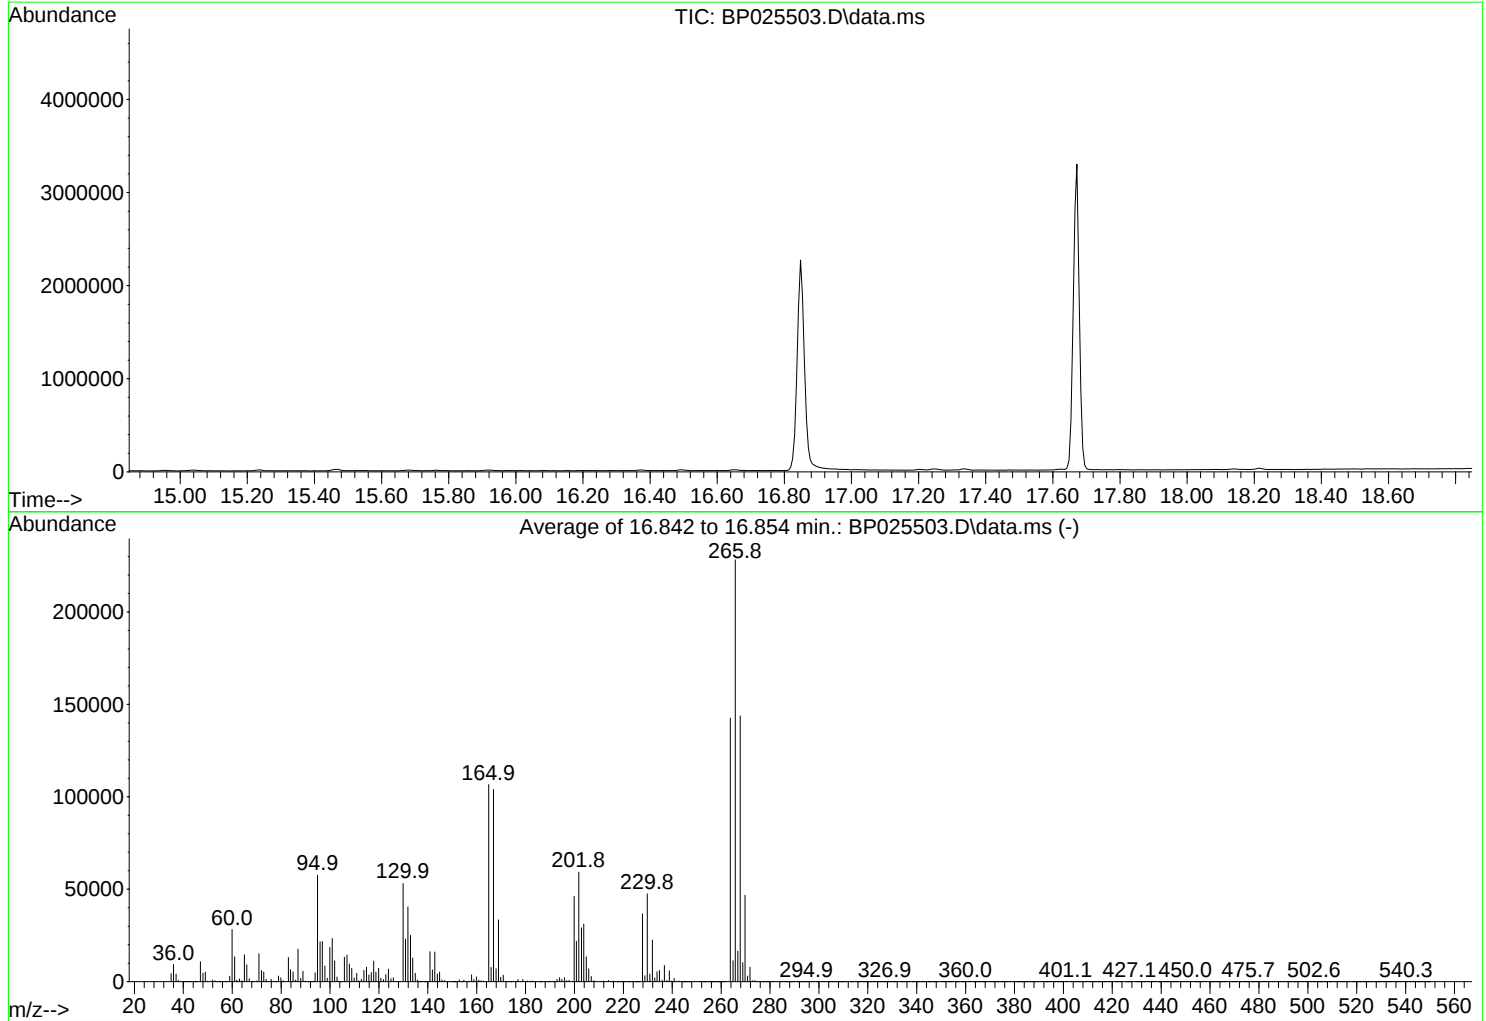




AutoFind: Scans 2364, 2365, 2366; Background Corrected with Scan 2355

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	0.5	298	FAIL*
75	95	30	60	0.1	65	FAIL*
95	95	100	100	100.0	57581	PASS
96	95	5	9	37.5	21574	FAIL*
173	174	0.00	2	50.0	4	FAIL*
174	95	50	100	0.0	8	FAIL*
175	174	5	9	650.0	52	FAIL*
176	174	95	101	125.0	10	FAIL*
177	176	5	9	11200.0	1120	FAIL*

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025503.D
Acq On : 20 Aug 2025 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 12:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

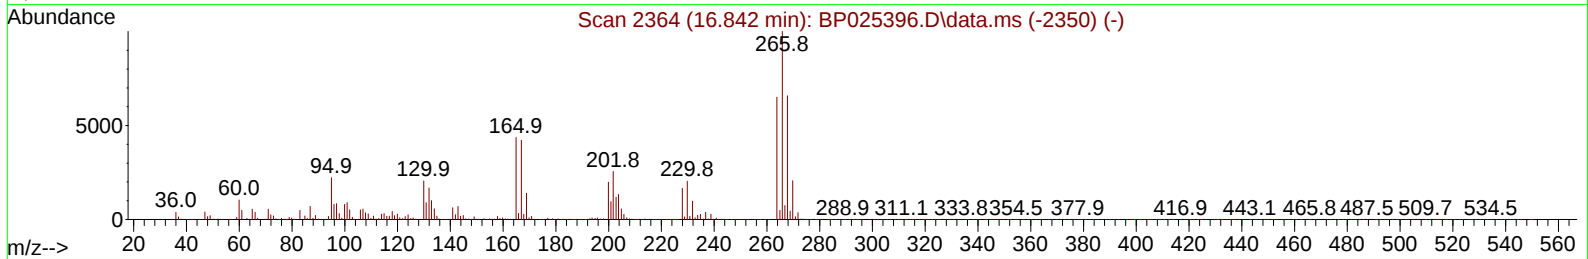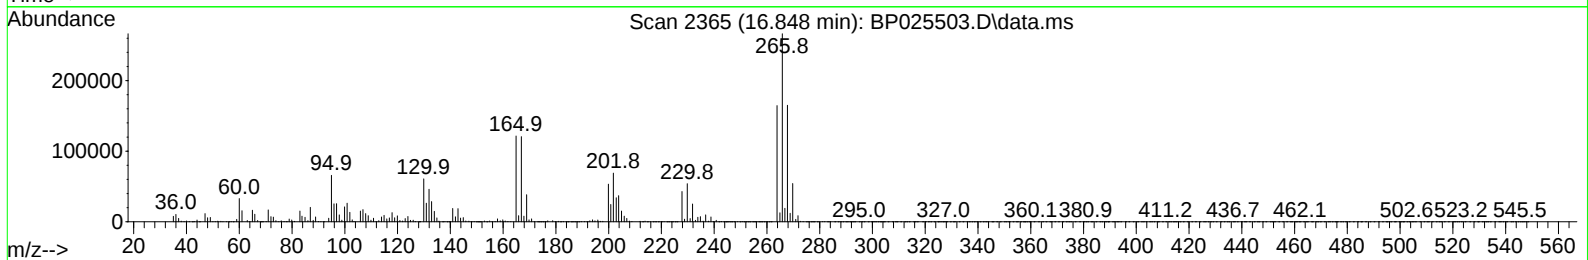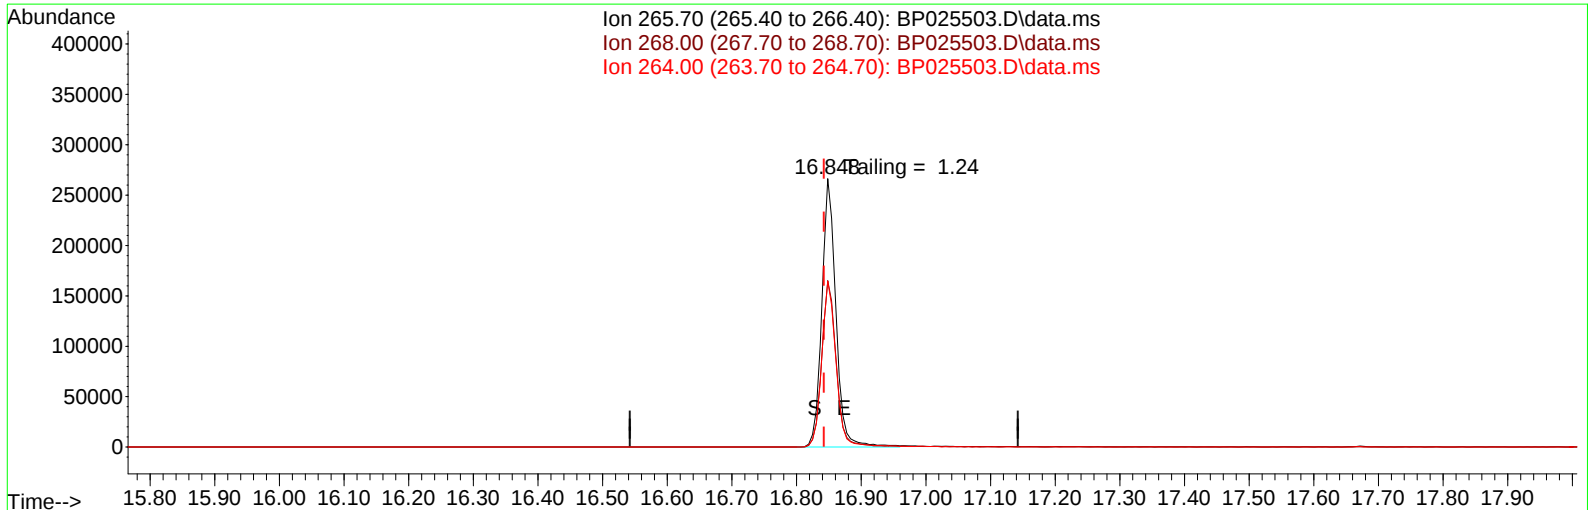

TIC: BP025503.D\data.ms

(70) Pentachlorophenol (C)

16.848min (+ 0.006) 11966.43 ng




response 406984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	61.99
264.00	65.00	61.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025503.D
Acq On : 20 Aug 2025 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 12:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

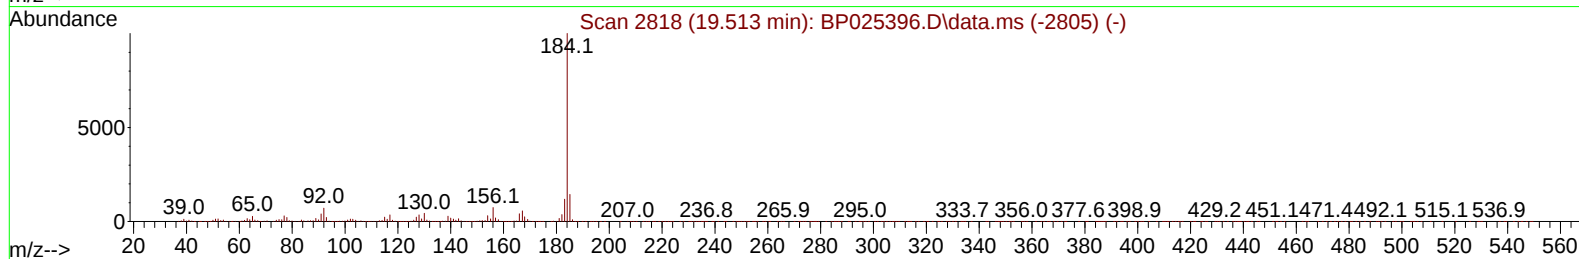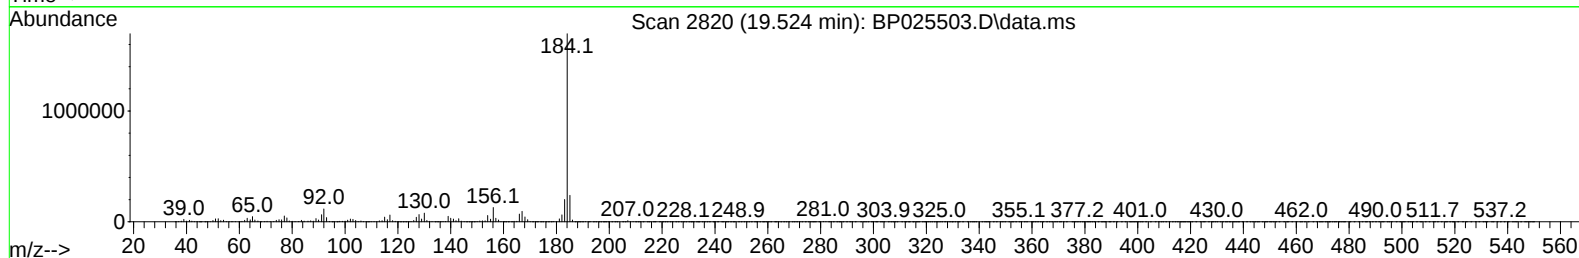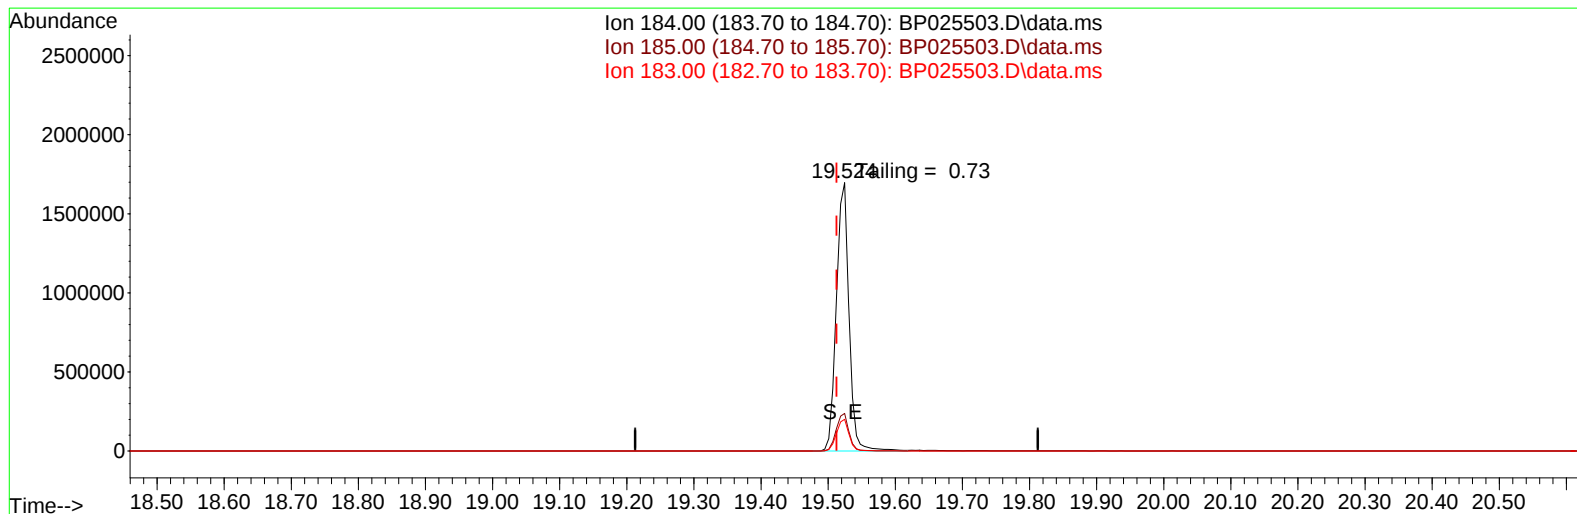

TIC: BP025503.D\data.ms

(77) Benzidine

19.524min (+ 0.012) 12639.84 ng

response 2228895

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.03
183.00	11.80	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2025	BNA_P	<u>BP025503.D</u>
Compound Name	Response	Retention Time
DDT	1135244	20.813
DDD	33801	20.36
DDE	2409	19.824
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36210	1171454	3.09

Instrument :
BNA_P
ClientSampleId :
DFTPP