
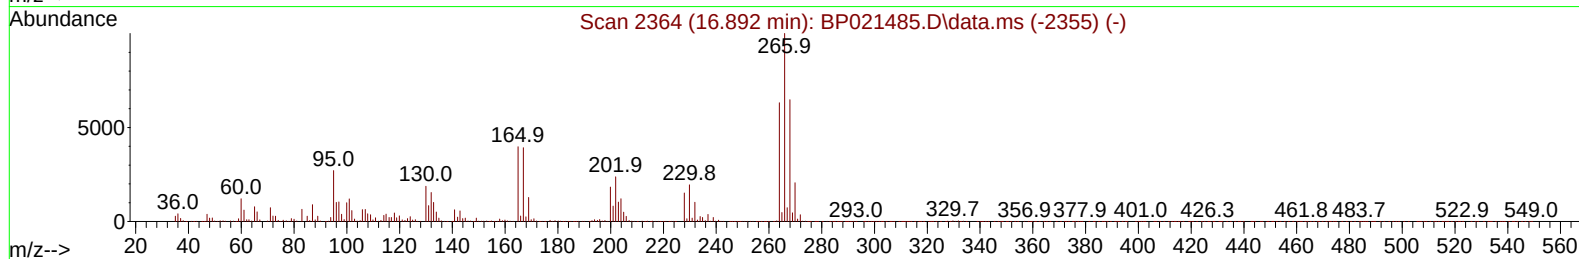
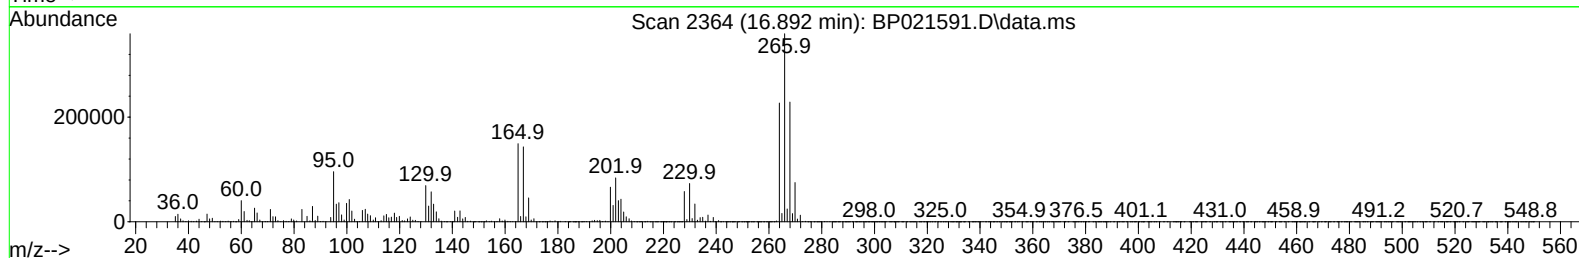


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021591.D
Acq On : 21 Aug 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:32:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

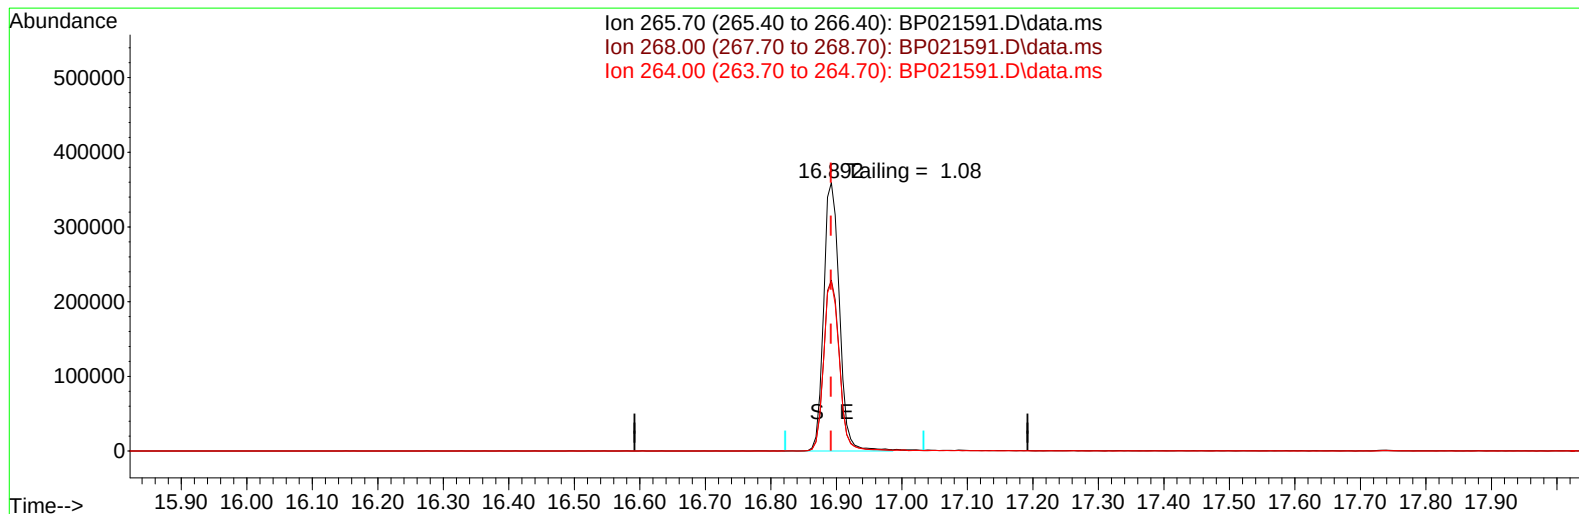

TIC: BP021591.D\data.ms

(70) Pentachlorophenol (C)




16.892min (+ 0.000) 350778.96 ng

response 605832

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.64
264.00	63.10	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021591.D
Acq On : 21 Aug 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:32:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

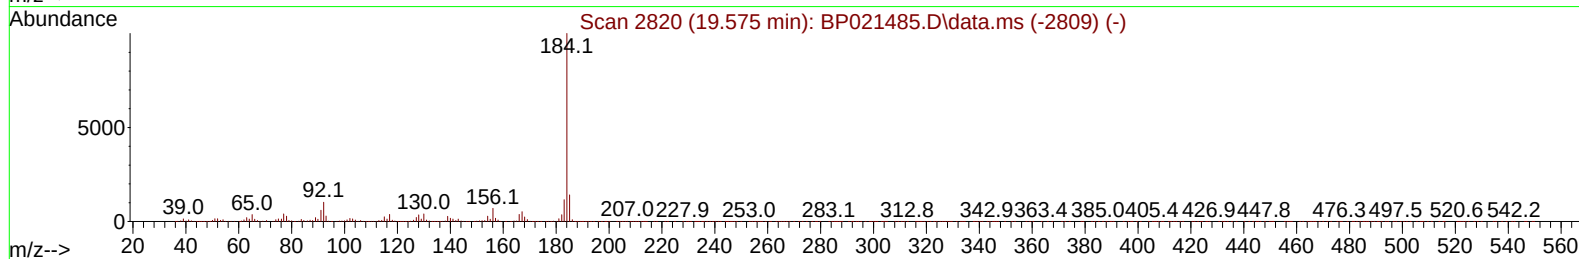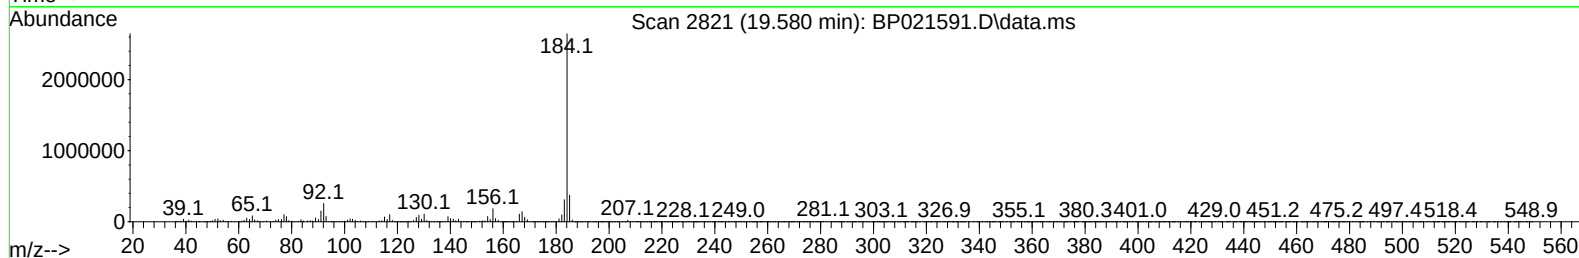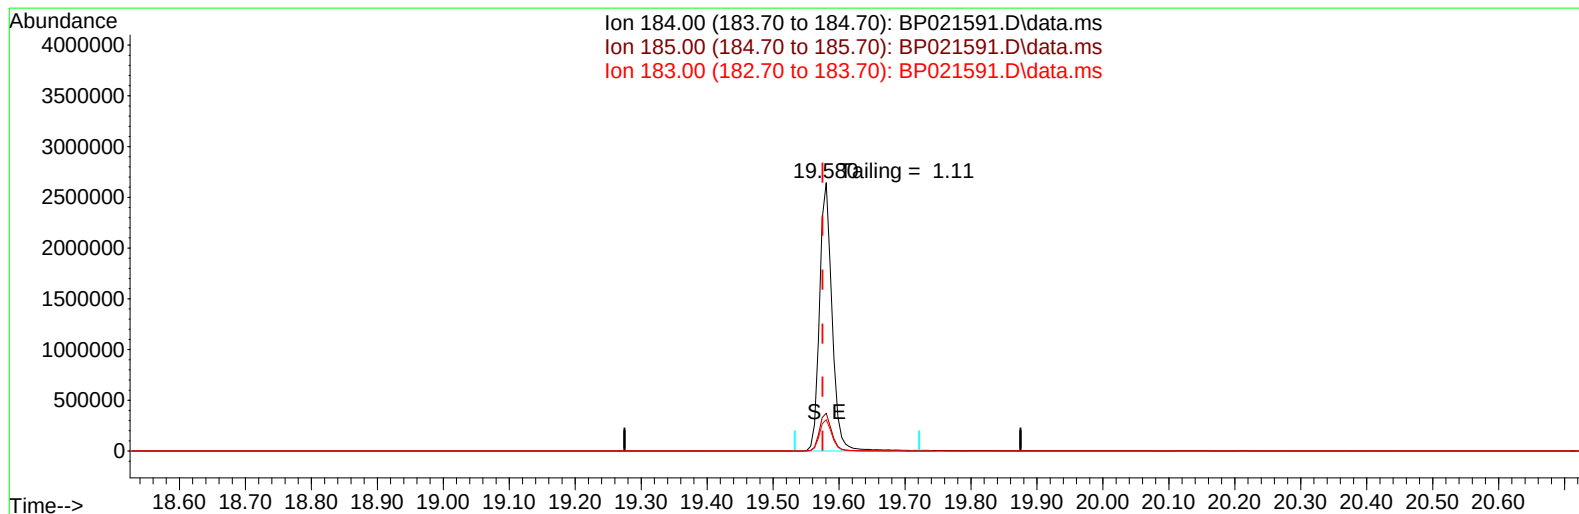

TIC: BP021591.D\data.ms

(77) Benzidine

19.580min (+ 0.005) -20.00 ng

response 3491621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.10
183.00	11.60	11.72
0.00	0.00	0.00