

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
 Data File : BP021601.D
 Acq On : 21 Aug 2024 17:25
 Operator : RC/JU
 Sample : P3666-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SP-303-20240816

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP021601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	27	rVB	13728679	17571854	86.05%	19.814%
2	5.393	402	409	420	rBV	2305542	3549540	17.38%	4.002%
3	6.963	668	676	688	rBV	1449340	2151808	10.54%	2.426%
4	7.799	811	818	827	rBV	937208	1401966	6.87%	1.581%
5	8.946	1004	1013	1027	rBV	3259162	5516527	27.02%	6.220%
6	10.587	1283	1292	1301	rBV	1067008	1897880	9.29%	2.140%
7	13.063	1705	1713	1732	rBV	7882825	11606237	56.84%	13.087%
8	14.457	1942	1950	1962	rBV	1563335	2547405	12.48%	2.872%
9	15.975	2200	2208	2232	rBV	6743161	9699628	47.50%	10.937%
10	17.263	2420	2427	2441	rBV	2362413	3382157	16.56%	3.814%
11	19.998	2884	2892	2904	rBV	12836807	20419374	100.00%	23.025%
12	21.727	3180	3186	3194	rVB2	2361738	4213768	20.64%	4.751%
13	25.168	3763	3771	3785	rVB	1794256	4726465	23.15%	5.330%




Sum of corrected areas: 88684609

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021601.D
Acq On : 21 Aug 2024 17:25
Operator : RC/JU
Sample : P3666-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SP-303-20240816

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

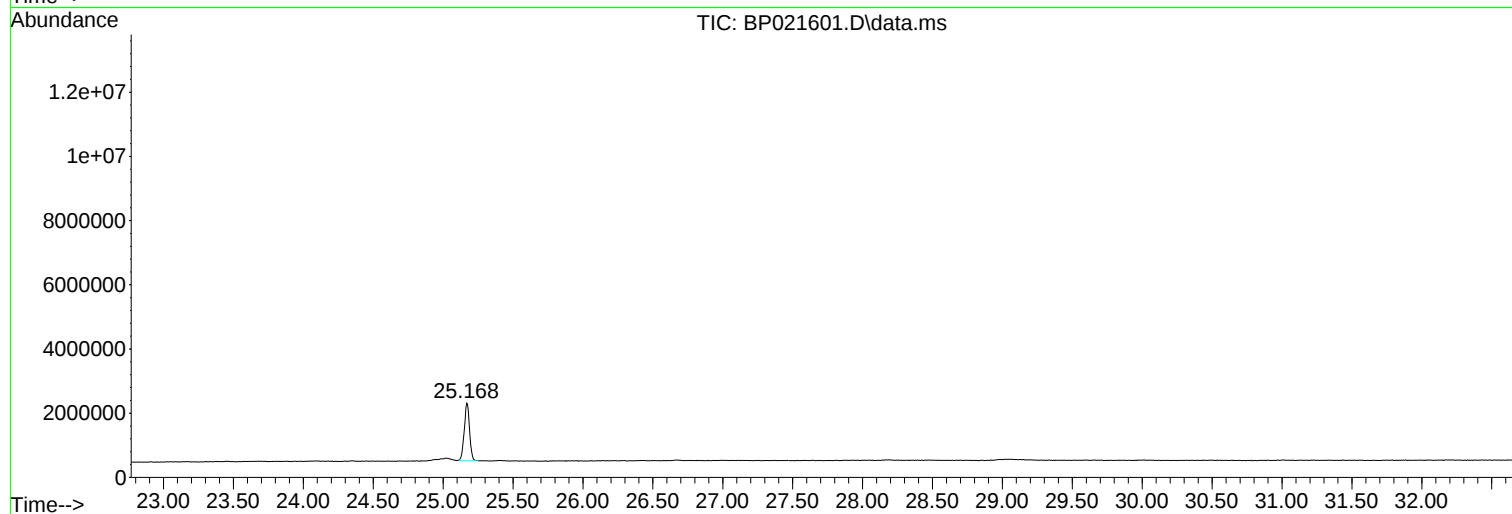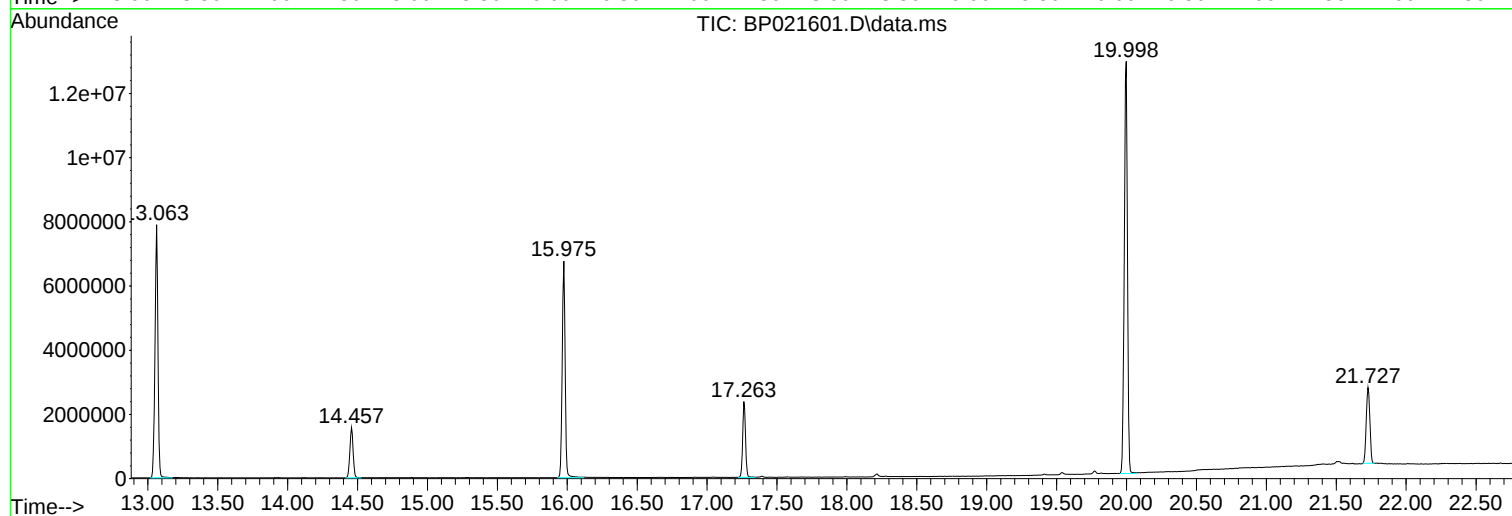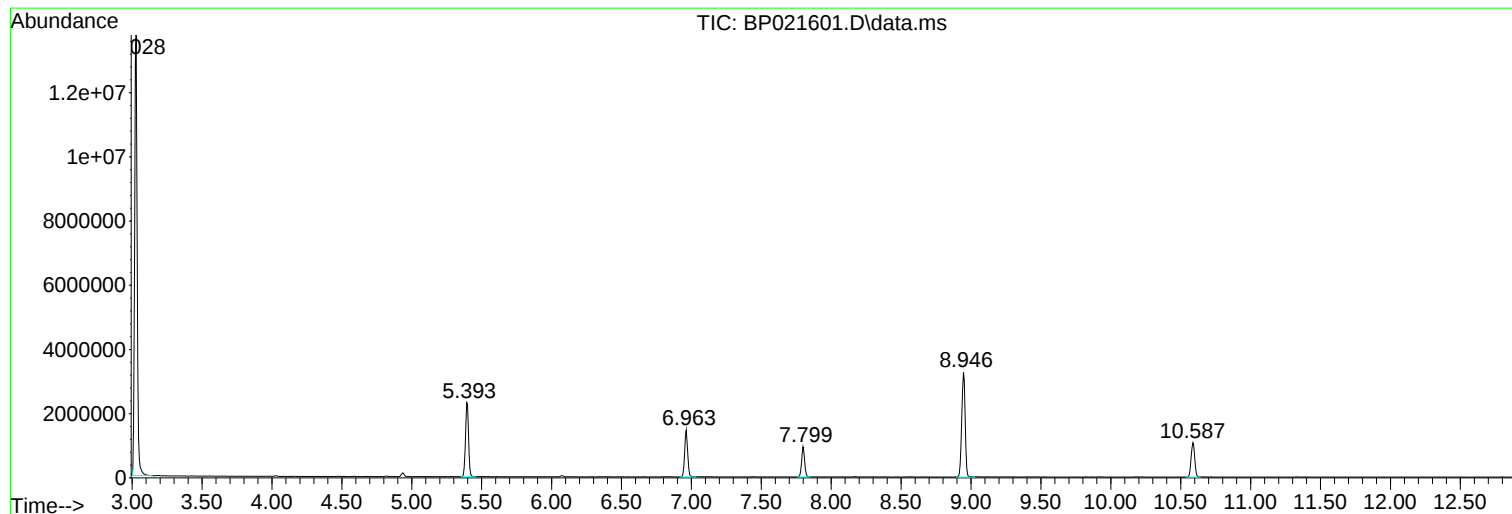

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021601.D
Acq On : 21 Aug 2024 17:25
Operator : RC/JU
Sample : P3666-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SP-303-20240816










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	250.67 ng	17571900	1,4-Dichlorobenzene-d4	7.799

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

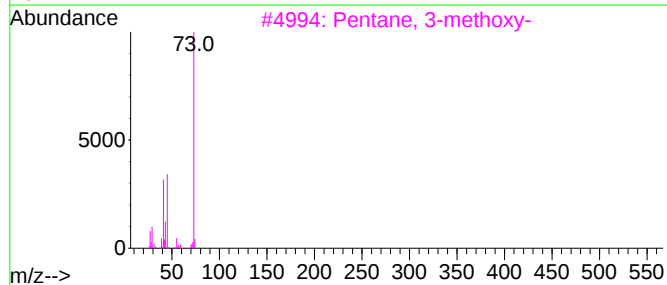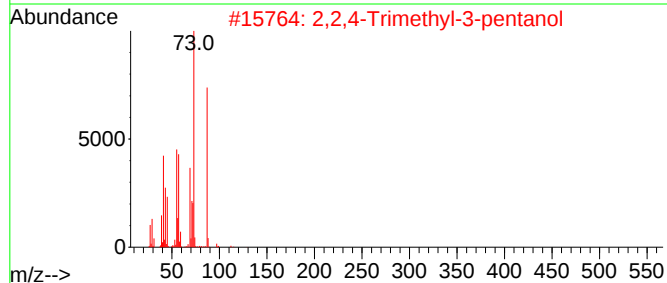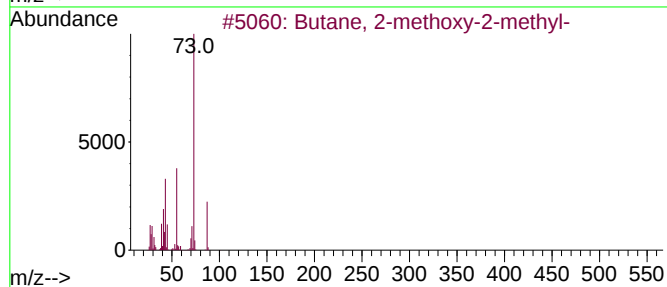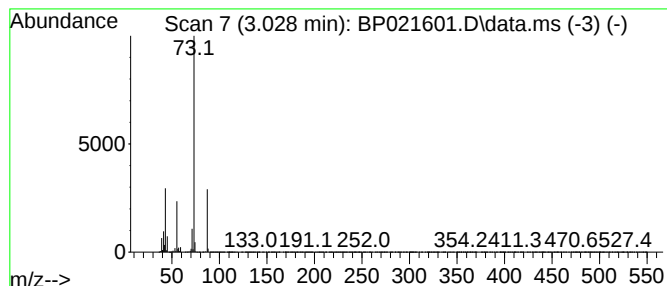

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021601.D
Acq On : 21 Aug 2024 17:25
Operator : RC/JU
Sample : P3666-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SP-303-20240816

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	250.7	ng	17571900	1	7.799	1401970	20.0