

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021602.D
Acq On : 21 Aug 2024 18:08
Operator : RC/JU
Sample : P3617-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
Field Blank

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP021602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	3	6	28	rVB	11272427	14531040	52.67%	14.723%
2	5.393	402	409	419	rBV	2460344	3841964	13.93%	3.893%
3	6.963	669	676	685	rBV	1511944	2438754	8.84%	2.471%
4	7.799	811	818	826	rBV	942767	1537368	5.57%	1.558%
5	8.946	1005	1013	1027	rBV	3350497	5586539	20.25%	5.660%
6	10.593	1285	1293	1308	rVB	1071913	2110868	7.65%	2.139%
7	13.063	1705	1713	1730	rBV	7915184	11760518	42.63%	11.916%
8	14.451	1942	1949	1965	rBV	1898090	2967603	10.76%	3.007%
9	15.969	2199	2207	2228	rBV	8256554	12279972	44.51%	12.442%
10	17.263	2420	2427	2441	rBV	2647297	4128786	14.97%	4.183%
11	19.992	2884	2891	2896	rBV	19733252	27588151	100.00%	27.952%
12	21.727	3179	3186	3199	rBV2	2860738	4966003	18.00%	5.031%
13	25.180	3763	3773	3784	rVB	1594447	4960720	17.98%	5.026%




Sum of corrected areas: 98698286

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021602.D
Acq On : 21 Aug 2024 18:08
Operator : RC/JU
Sample : P3617-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
Field Blank

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

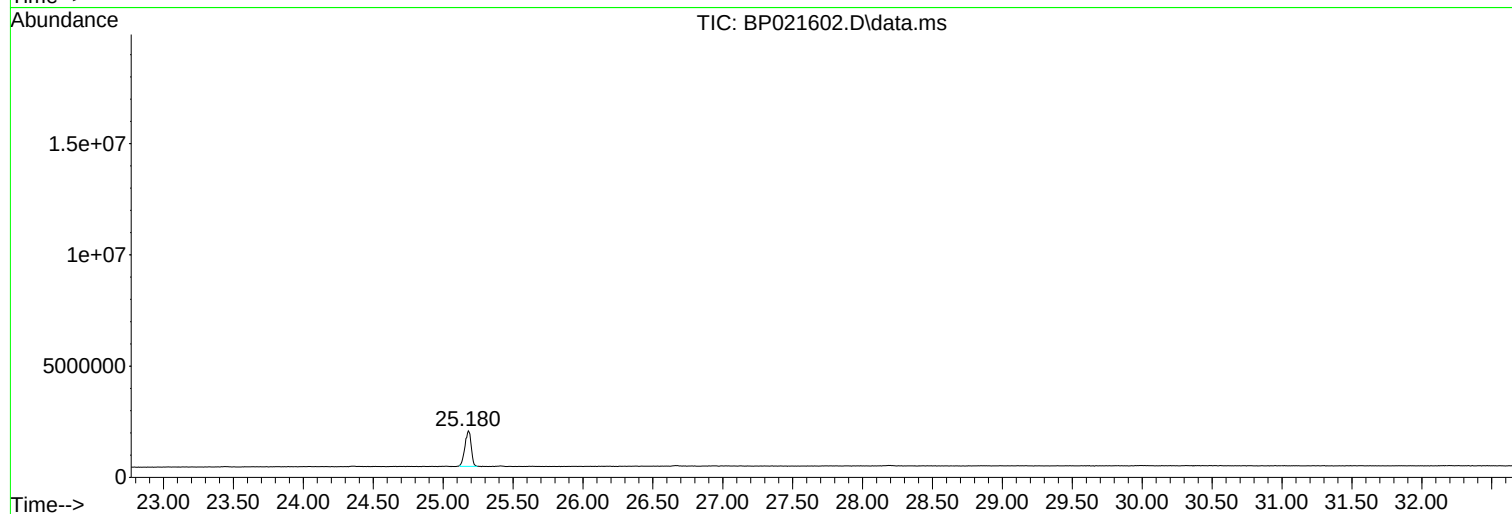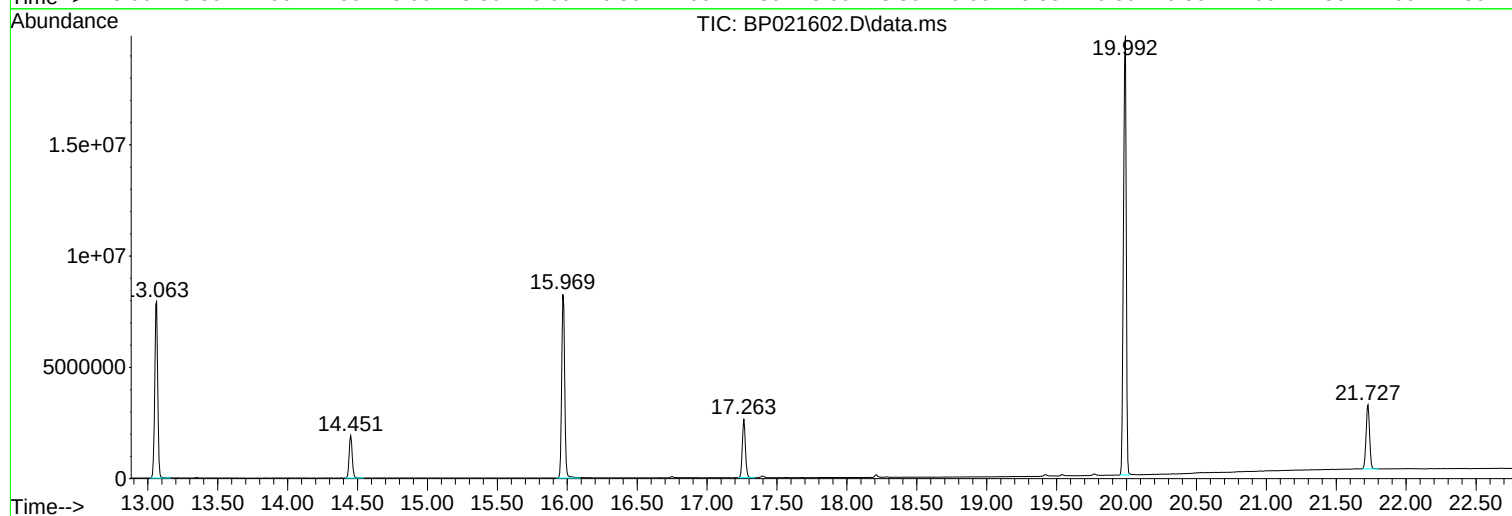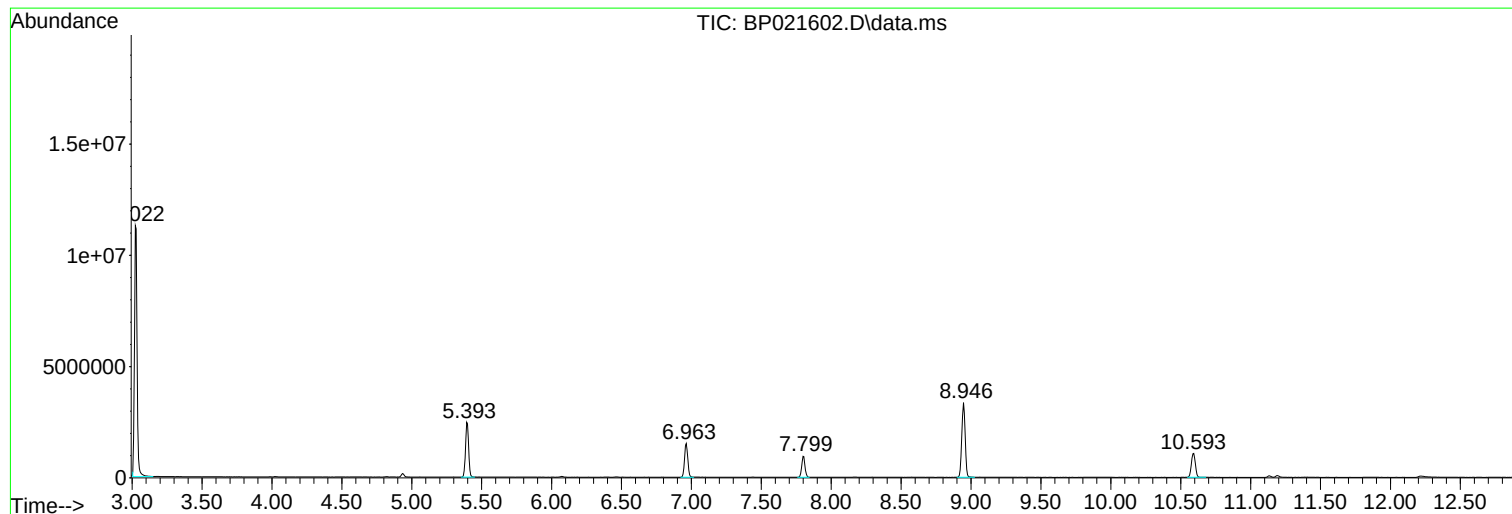

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021602.D
Acq On : 21 Aug 2024 18:08
Operator : RC/JU
Sample : P3617-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
Field Blank










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.022	189.04 ng	14531000	1,4-Dichlorobenzene-d4	7.799

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86		
2	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
3	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17		
4	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

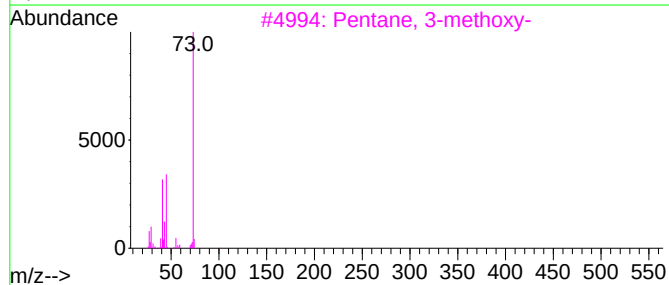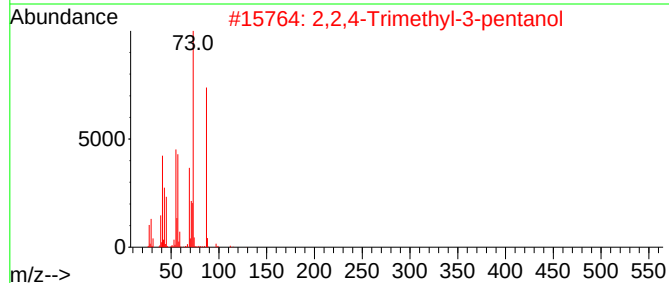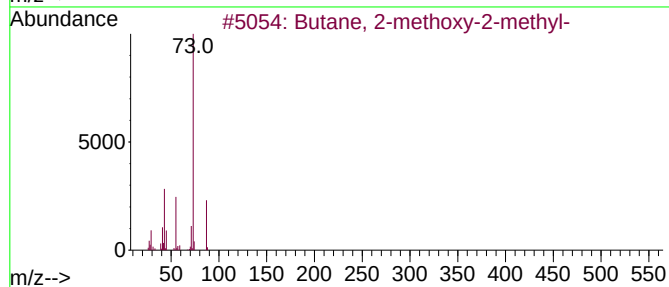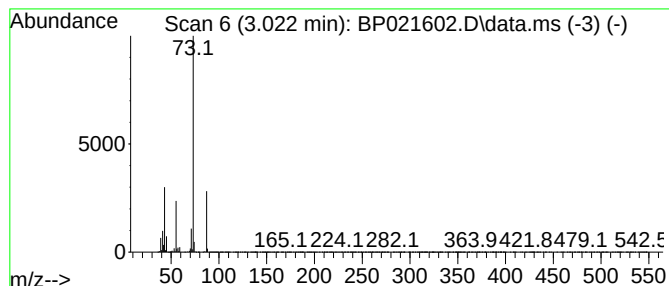

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021602.D
Acq On : 21 Aug 2024 18:08
Operator : RC/JU
Sample : P3617-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
Field Blank

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.022	189.0	ng	14531000	1	7.799	1537370	20.0