

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082222\
 Data File : BP011527.D
 Acq On : 22 Aug 2022 11:41
 Operator : CG/JU
 Sample : PB146656BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	10	14	23	rVB2	32684	44109	2.85%	0.236%
2	3.475	80	83	100	rBV	292644	458962	29.67%	2.455%
3	3.781	133	135	140	rVB2	7022	7636	0.49%	0.041%
4	4.487	253	255	259	rBV5	1708	1962	0.13%	0.010%
5	5.222	374	380	382	rBV6	2045	2992	0.19%	0.016%
6	5.299	392	393	398	rVB5	1833	1569	0.10%	0.008%
7	5.358	401	403	407	rBV4	1399	2103	0.14%	0.011%
8	5.893	492	494	498	rBV3	1847	2374	0.15%	0.013%
9	6.740	630	638	655	rBV	390066	612815	39.62%	3.278%
10	6.905	660	666	677	rVB	286289	434533	28.09%	2.325%
11	7.087	690	697	716	rVB	394080	607065	39.25%	3.248%
12	7.328	734	738	740	rBV5	1128	1568	0.10%	0.008%
13	7.552	770	776	783	rBV	280738	439999	28.45%	2.354%
14	8.275	892	899	915	rVV	442007	714020	46.16%	3.820%
15	8.416	922	923	927	rVB4	2318	2526	0.16%	0.014%
16	8.452	927	929	932	rBV4	1649	2340	0.15%	0.013%
17	8.716	964	974	988	rBV	363737	606298	39.20%	3.243%
18	8.852	994	997	1001	rVB6	2626	4407	0.28%	0.024%
19	8.981	1017	1019	1025	rVV6	1060	1723	0.11%	0.009%
20	9.199	1053	1056	1060	rVB6	1182	1706	0.11%	0.009%
21	9.434	1089	1096	1106	rBV	302645	499345	32.28%	2.671%
22	9.546	1114	1115	1120	rVB4	1592	1687	0.11%	0.009%
23	9.746	1147	1149	1152	rBV3	1476	2120	0.14%	0.011%
24	9.969	1180	1187	1201	rBV	414964	702963	45.45%	3.761%
25	10.340	1243	1250	1261	rVB	381802	616620	39.87%	3.299%
26	10.499	1269	1277	1290	rBV	455648	802281	51.87%	4.292%
27	11.093	1375	1378	1380	rBV4	1439	1726	0.11%	0.009%
28	11.175	1390	1392	1395	rBV3	1846	2622	0.17%	0.014%
29	11.369	1423	1425	1429	rBV4	1191	1635	0.11%	0.009%
30	11.563	1456	1458	1463	rBV5	1338	1932	0.12%	0.010%
31	11.946	1518	1523	1528	rBV3	7172	13223	0.85%	0.071%
32	12.099	1545	1549	1552	rBV5	934	1676	0.11%	0.009%
33	12.163	1555	1560	1564	rBV8	1126	2166	0.14%	0.012%
34	12.234	1569	1572	1575	rBV5	1949	2829	0.18%	0.015%
35	12.416	1601	1603	1606	rBV3	1279	1756	0.11%	0.009%
36	13.040	1705	1709	1710	rVB3	1278	1603	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082222\
 Data File : BP011527.D
 Acq On : 22 Aug 2022 11:41
 Operator : CG/JU
 Sample : PB146656BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	13.140	1723	1726	1729	rVB5	1592	1876	0.12%	0.010%
38	13.187	1729	1734	1740	rBV5	2784	5627	0.36%	0.030%
39	13.528	1788	1792	1796	rVB4	1471	1579	0.10%	0.008%
40	13.651	1807	1813	1825	rVV	749731	1011279	65.38%	5.410%
41	13.916	1849	1858	1872	rBV	776891	1112465	71.93%	5.951%
42	14.022	1874	1876	1880	rVB4	1745	1630	0.11%	0.009%
43	14.228	1904	1911	1919	rBV	515433	731821	47.32%	3.915%
44	14.293	1919	1922	1929	rVB8	2629	5229	0.34%	0.028%
45	14.457	1944	1950	1975	rBV	279251	511039	33.04%	2.734%
46	14.863	2016	2019	2021	rBV3	1581	1843	0.12%	0.010%
47	15.081	2053	2056	2061	rBV7	1329	2229	0.14%	0.012%
48	15.234	2075	2082	2090	rBV	969348	1336616	86.42%	7.150%
49	15.369	2099	2105	2115	rBV	347195	452938	29.28%	2.423%
50	15.475	2118	2123	2127	rVV3	10701	16784	1.09%	0.090%
51	15.504	2127	2128	2135	rVB6	2656	3340	0.22%	0.018%
52	15.581	2135	2141	2144	rBV7	1573	2927	0.19%	0.016%
53	15.798	2176	2178	2181	rBV3	1902	2293	0.15%	0.012%
54	16.022	2212	2216	2222	rBV9	2477	4081	0.26%	0.022%
55	16.134	2232	2235	2238	rBV5	1355	1602	0.10%	0.009%
56	16.192	2241	2245	2250	rVB7	1835	3684	0.24%	0.020%
57	16.292	2258	2262	2264	rBV4	1536	2231	0.14%	0.012%
58	16.675	2325	2327	2331	rVB2	1606	1990	0.13%	0.011%
59	16.945	2370	2373	2376	rBV3	2284	2329	0.15%	0.012%
60	16.998	2376	2382	2388	rBV	600377	811369	52.46%	4.340%
61	17.098	2393	2399	2410	rVV	1038658	1435887	92.84%	7.681%
62	17.369	2443	2445	2448	rBV4	1596	1831	0.12%	0.010%
63	17.692	2497	2500	2502	rVV4	2177	1711	0.11%	0.009%
64	17.734	2505	2507	2512	rBV5	1751	2908	0.19%	0.016%
65	17.916	2535	2538	2542	rBV6	3730	5718	0.37%	0.031%
66	18.363	2613	2614	2616	rBV2	1979	1786	0.12%	0.010%
67	18.933	2708	2711	2717	rVB5	11828	14716	0.95%	0.079%
68	19.004	2719	2723	2727	rBV	11697	17184	1.11%	0.092%
69	19.363	2778	2784	2794	rBV	1230405	1546680	100.00%	8.274%
70	21.127	3079	3084	3089	rBV	681090	811374	52.46%	4.341%
71	23.269	3442	3448	3456	rBV2	763814	1435714	92.83%	7.680%
72	23.416	3467	3473	3483	rVB2	415326	781817	50.55%	4.182%




Sum of corrected areas: 18693018

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082222\
Data File : BP011527.D
Acq On : 22 Aug 2022 11:41
Operator : CG/JU
Sample : PB146656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

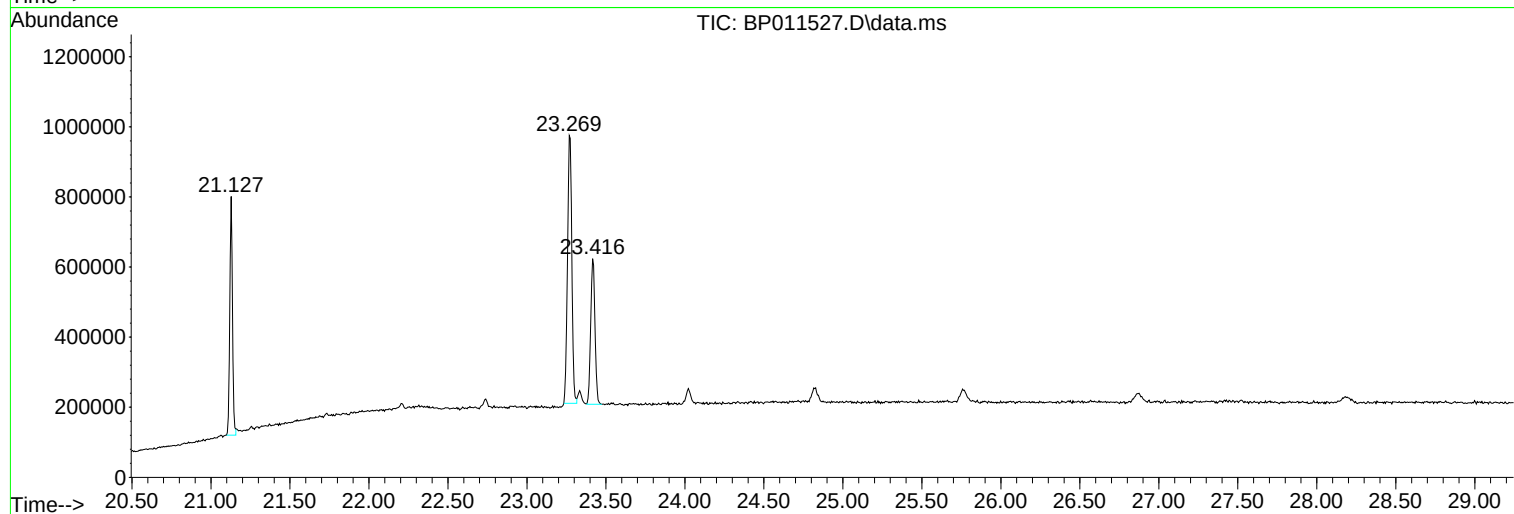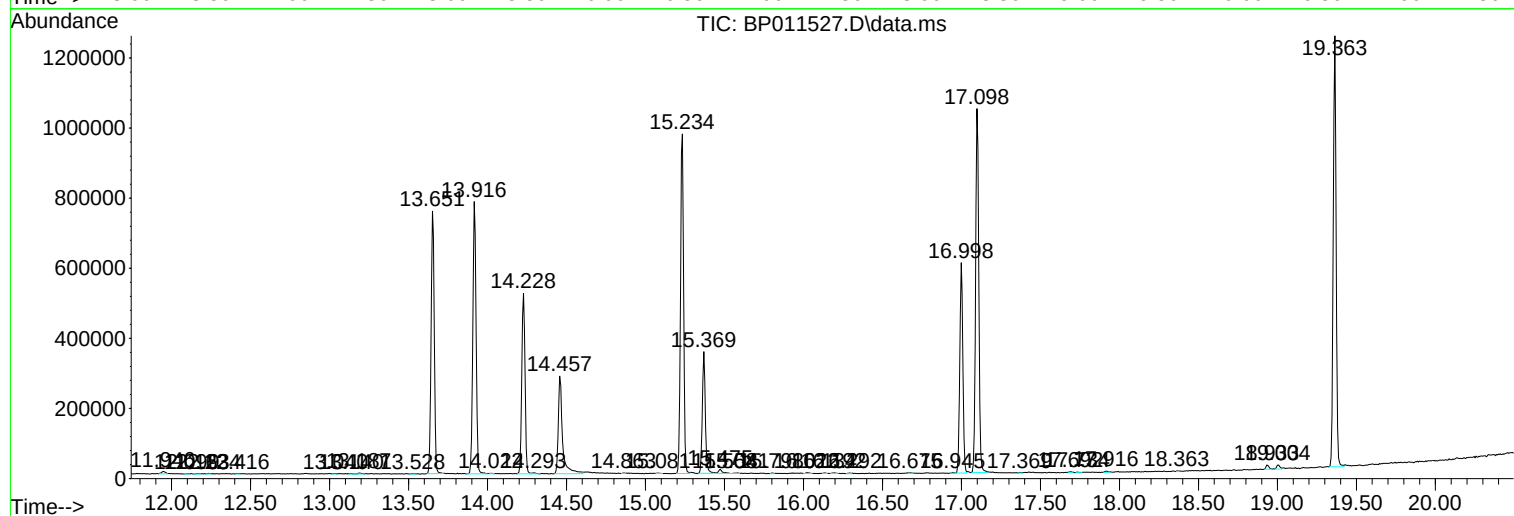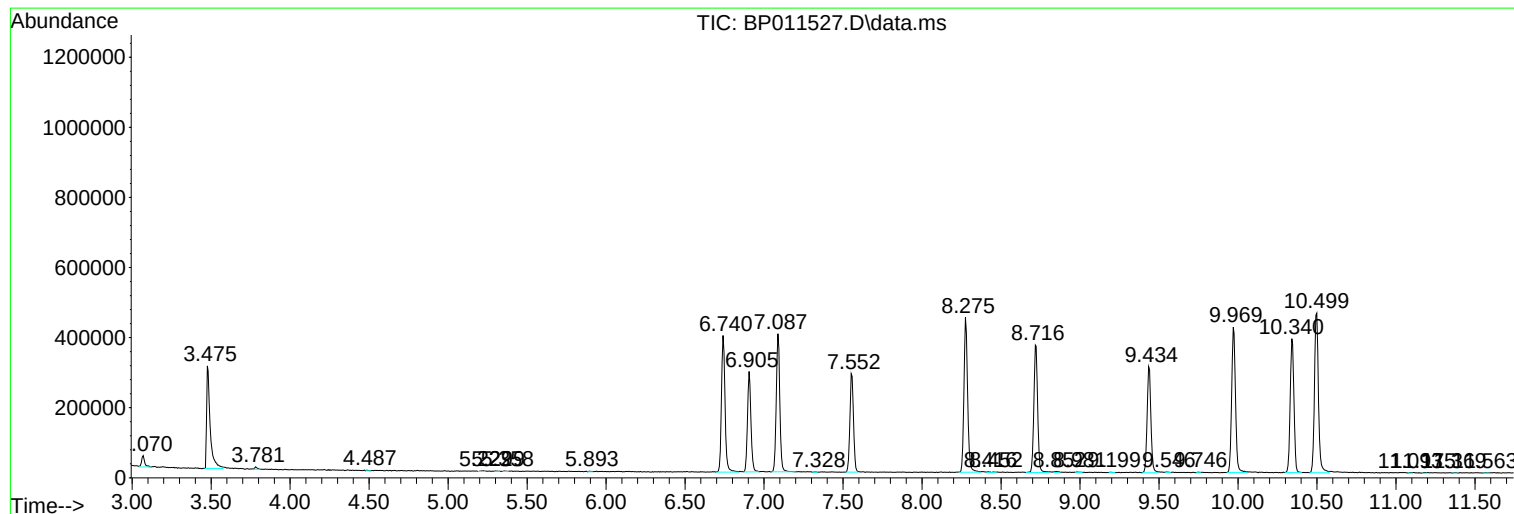

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082222\
Data File : BP011527.D
Acq On : 22 Aug 2022 11:41
Operator : CG/JU
Sample : PB146656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082222\
Data File : BP011527.D
Acq On : 22 Aug 2022 11:41
Operator : CG/JU
Sample : PB146656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc