

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
 Data File : BP021619.D
 Acq On : 22 Aug 2024 18:41
 Operator : RC/JU
 Sample : P3518-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-09-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP021619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	18	rVB	4146872	5306192	44.22%	5.299%
2	3.546	91	95	106	rBV	456096	627106	5.23%	0.626%
3	4.934	326	331	342	rVB	280376	416827	3.47%	0.416%
4	5.399	403	410	419	rBV	4951237	7365212	61.38%	7.355%
5	6.758	633	641	647	rBV	98258	208098	1.73%	0.208%
6	6.969	668	677	692	rBV	4630477	7778850	64.83%	7.768%
7	7.399	743	750	760	rBV	207386	354249	2.95%	0.354%
8	7.799	810	818	825	rBV	1351327	2142373	17.85%	2.139%
9	8.946	1005	1013	1024	rBV	2817558	4872317	40.61%	4.866%
10	9.505	1100	1108	1115	rBV	103386	165922	1.38%	0.166%
11	10.587	1284	1292	1303	rBV	1728943	2976997	24.81%	2.973%
12	11.322	1411	1417	1432	rBV	333285	627184	5.23%	0.626%
13	13.051	1705	1711	1726	rBV	5429374	8414121	70.13%	8.403%
14	14.445	1941	1948	1956	rBV	2689570	3855412	32.13%	3.850%
15	14.698	1979	1991	2004	rBV	5360557	11998741	100.00%	11.982%
16	15.963	2200	2206	2216	rBV	5104721	7723587	64.37%	7.713%
17	17.257	2420	2426	2432	rBV	3041376	4676749	38.98%	4.670%
18	17.310	2432	2435	2442	rVB2	188757	328790	2.74%	0.328%
19	17.404	2443	2451	2455	rBV2	67197	144756	1.21%	0.145%
20	17.892	2526	2534	2537	rBV9	59182	144252	1.20%	0.144%
21	17.975	2544	2548	2556	rVB	109805	172391	1.44%	0.172%
22	18.057	2558	2562	2566	rBV	110366	147063	1.23%	0.147%
23	18.169	2574	2581	2583	rBV3	62506	139265	1.16%	0.139%
24	18.210	2583	2588	2610	rVV	1916539	3038098	25.32%	3.034%
25	18.410	2613	2622	2625	rBV5	164446	407687	3.40%	0.407%
26	18.516	2637	2640	2650	rVB9	131161	289875	2.42%	0.289%
27	19.110	2738	2741	2746	rVB3	79640	131366	1.09%	0.131%
28	19.198	2752	2756	2761	rVB2	264597	340911	2.84%	0.340%
29	19.269	2763	2768	2772	rBV5	79185	169565	1.41%	0.169%
30	19.392	2784	2789	2793	rBV	651509	916104	7.64%	0.915%
31	19.533	2809	2813	2823	rVB2	723617	955179	7.96%	0.954%
32	19.763	2848	2852	2856	rBV	454109	542850	4.52%	0.542%
33	19.980	2884	2889	2899	rVB	9454249	10927458	91.07%	10.912%
34	20.292	2938	2942	2946	rBV2	328258	395038	3.29%	0.394%
35	20.669	3003	3006	3012	rVB	527574	591952	4.93%	0.591%
36	21.392	3124	3129	3144	rVB2	853653	1836446	15.31%	1.834%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
Data File : BP021619.D
Acq On : 22 Aug 2024 18:41
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-09-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.716	3177	3184	3190	rBV2	3252176	5798904	48.33%	5.791%
38	25.145	3758	3767	3768	rBV	1509400	3209853	26.75%	3.205%




Sum of corrected areas: 100137740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
Data File : BP021619.D
Acq On : 22 Aug 2024 18:41
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-09-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

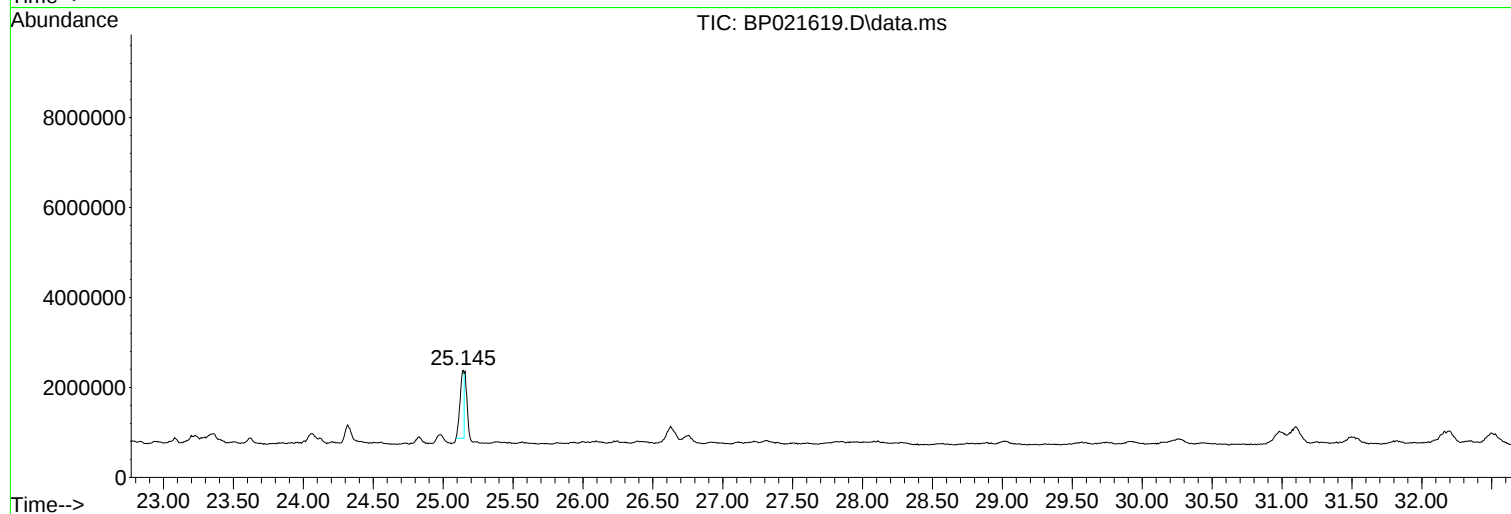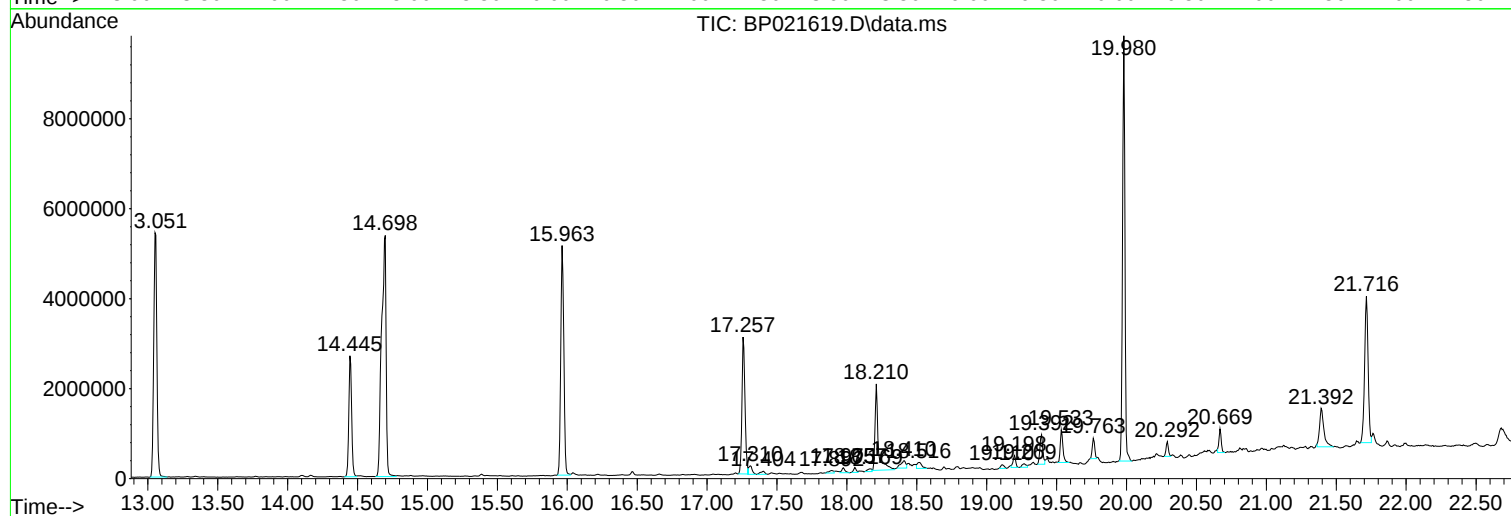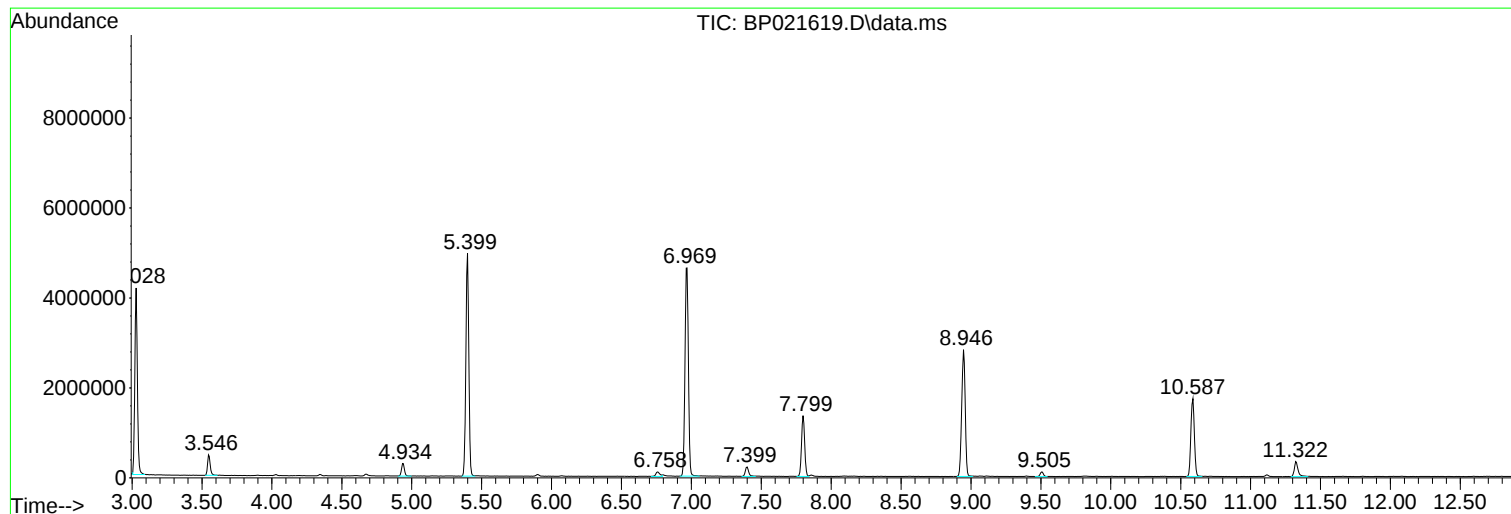

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
Data File : BP021619.D
Acq On : 22 Aug 2024 18:41
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-09-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
Data File : BP021619.D
Acq On : 22 Aug 2024 18:41
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-09-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------