
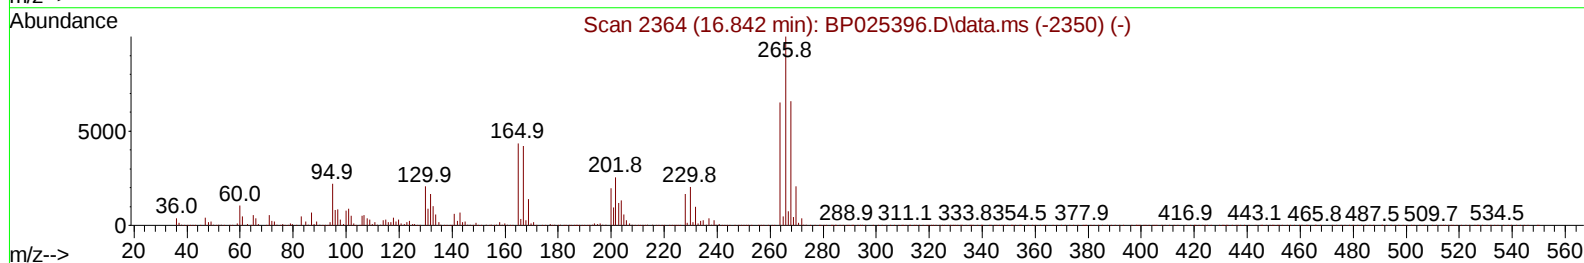
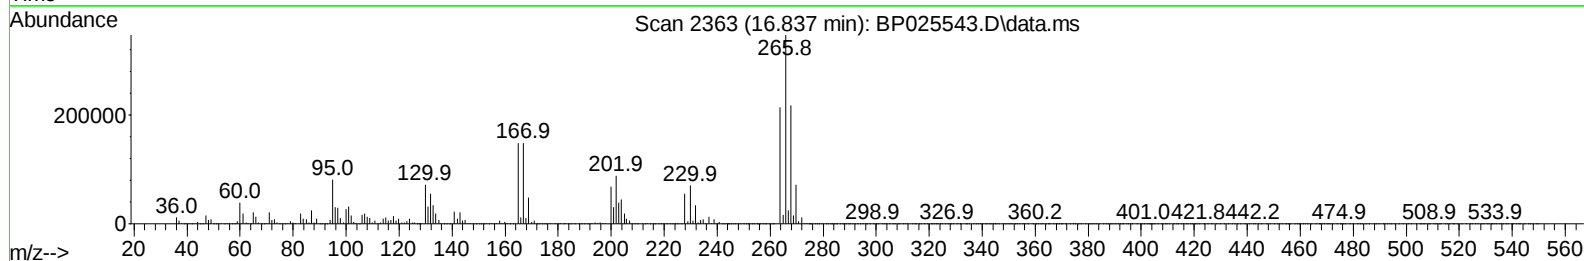


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082225\
Data File : BP025543.D
Acq On : 22 Aug 2025 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 10:56:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

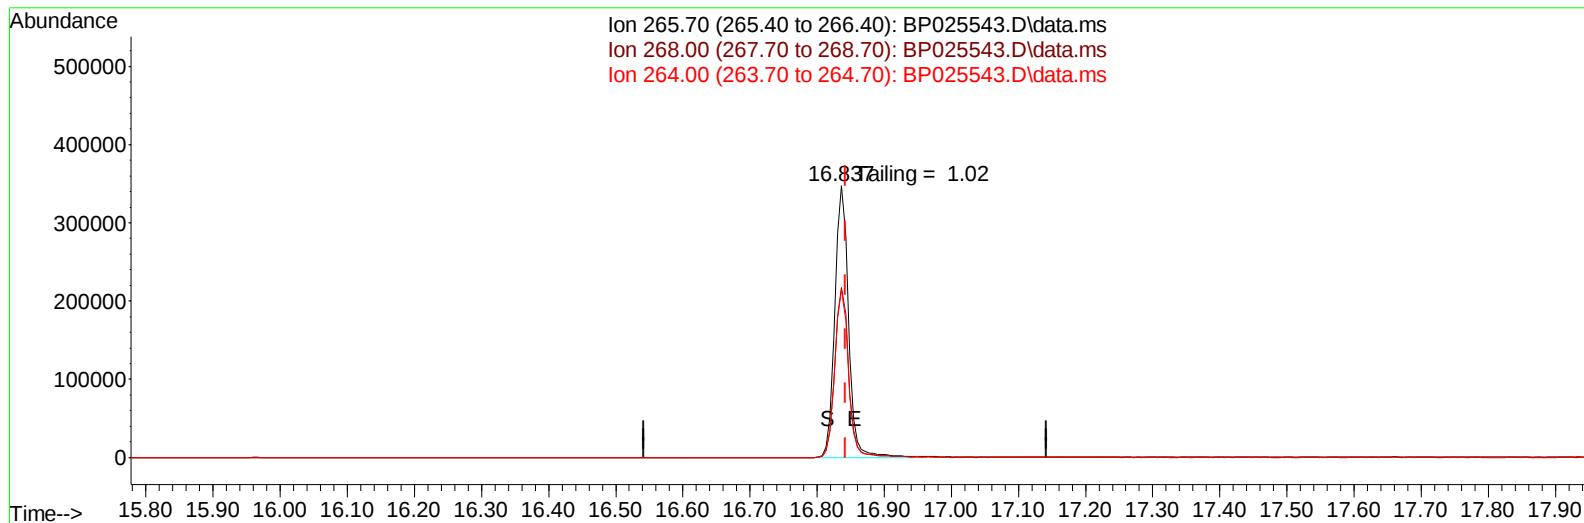

TIC: BP025543.D\data.ms

(70) Pentachlorophenol (C)




16.837min (-0.006) 24379.55 ng

response 490511

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.65
264.00	65.00	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082225\
Data File : BP025543.D
Acq On : 22 Aug 2025 10:08
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 10:56:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

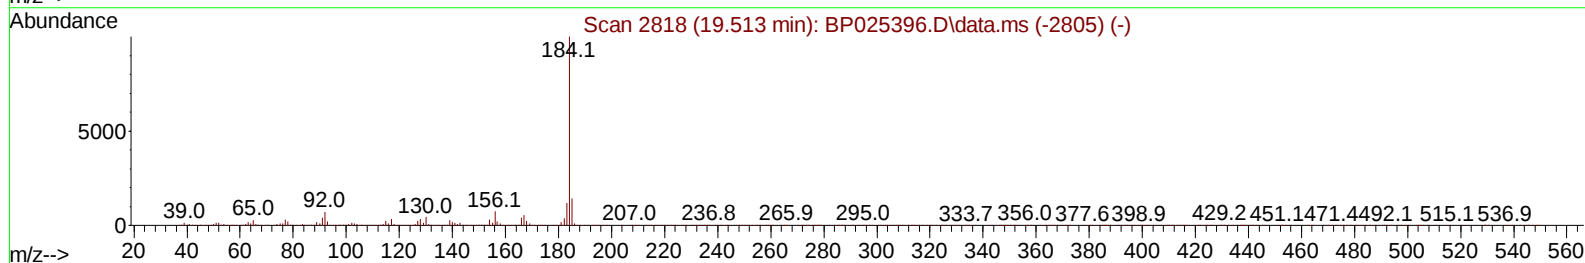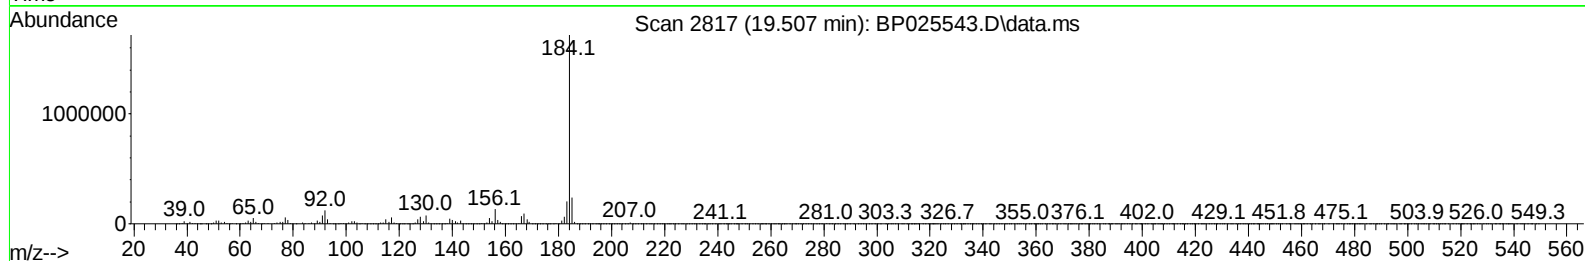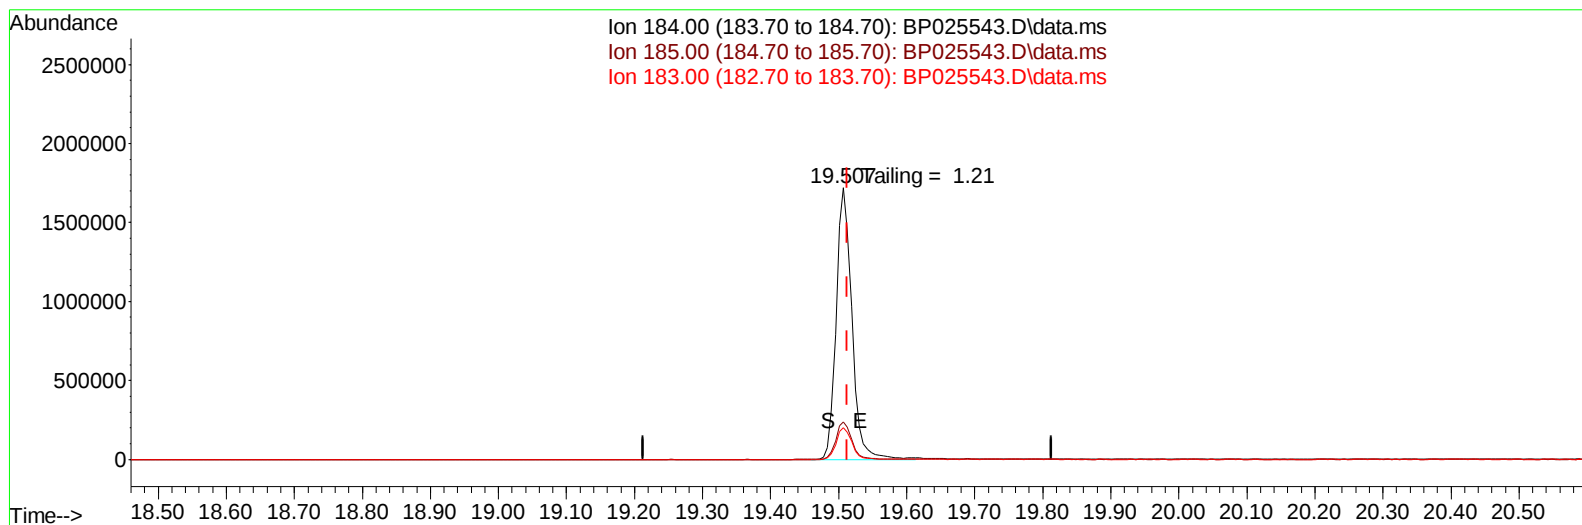

TIC: BP025543.D\data.ms

(77) Benzidine

19.507min (-0.006) 16182.04 ng

response 2751355

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.92
183.00	11.80	11.76
0.00	0.00	0.00