
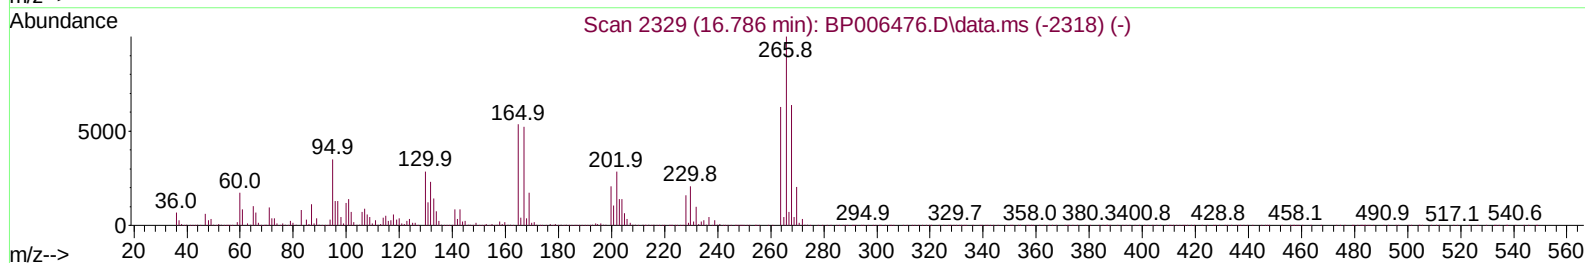
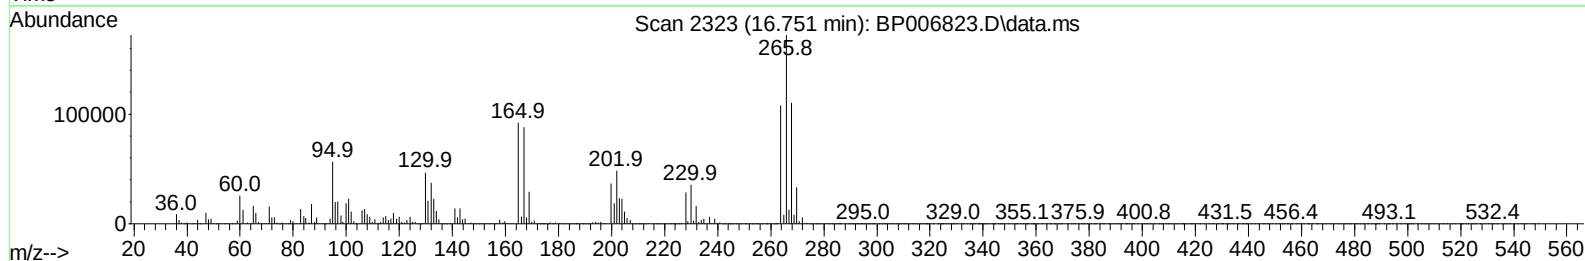


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006823.D
Acq On : 23 Aug 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 11:48:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 11:39:38 2021
Response via : Initial Calibration

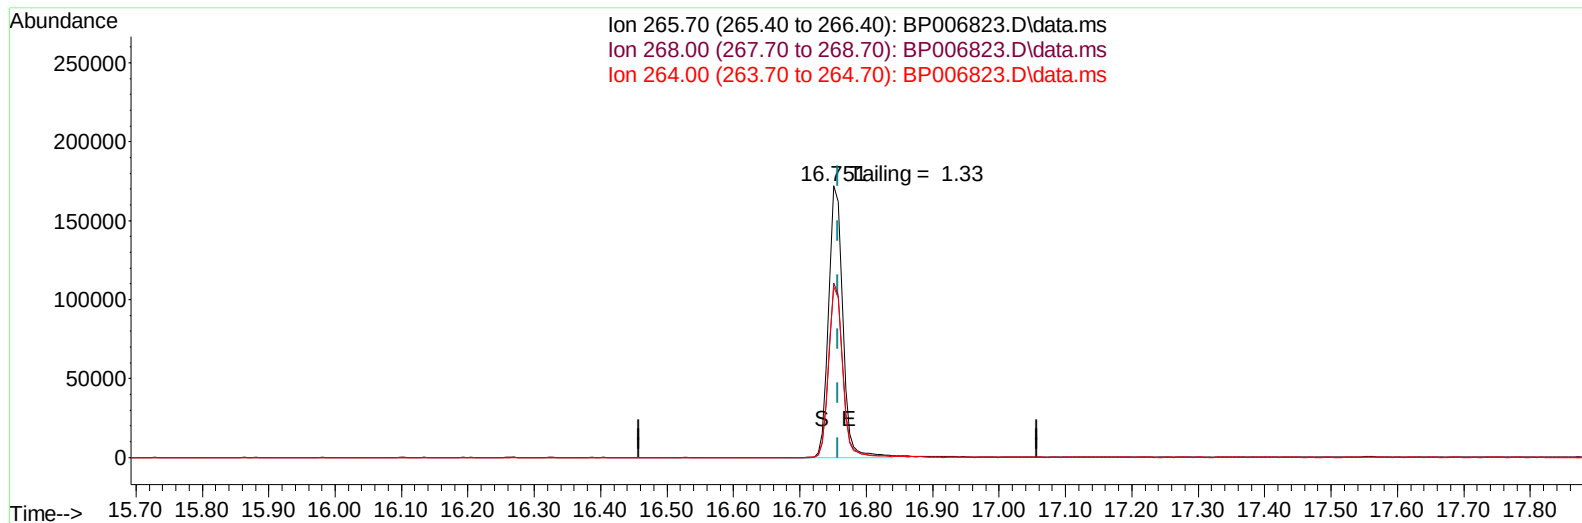

TIC: BP006823.D\data.ms

(70) Pentachlorophenol (C)




16.751min (-0.006) 97490.87 ng

response 253948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.22
264.00	62.90	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006823.D
Acq On : 23 Aug 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 11:48:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 11:39:38 2021
Response via : Initial Calibration

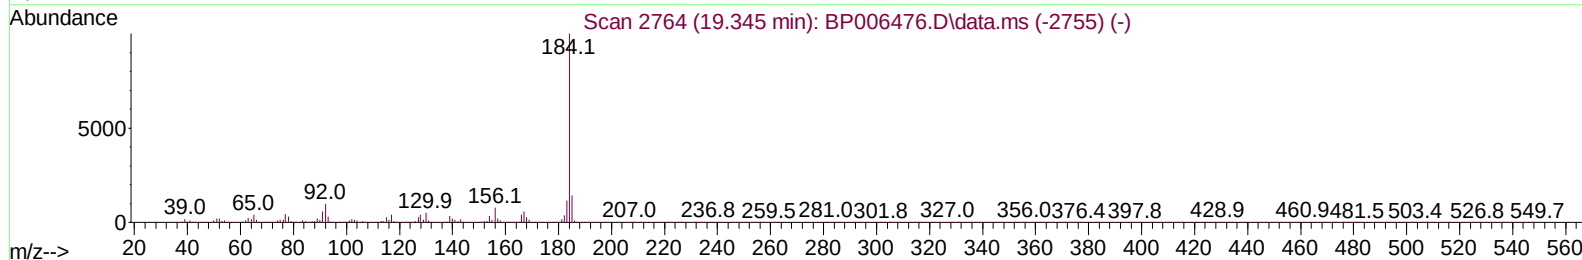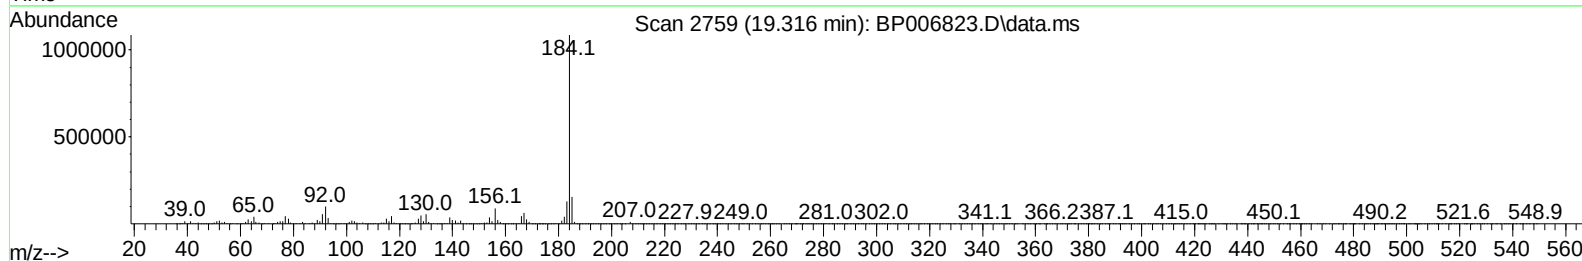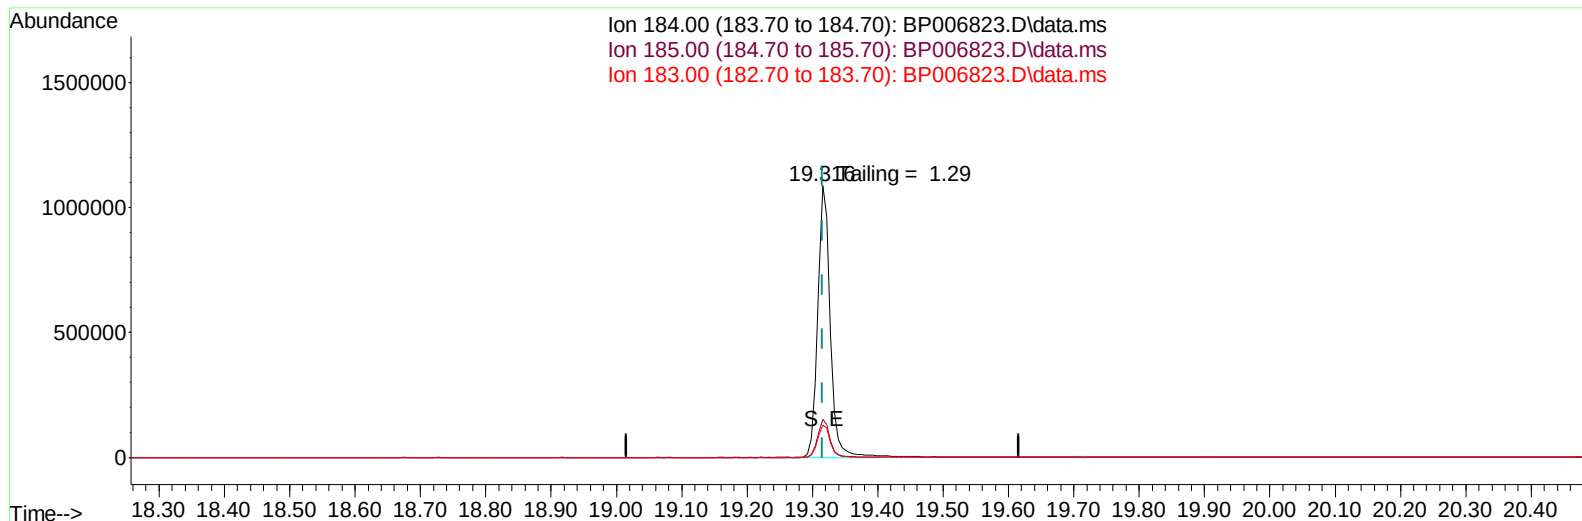

TIC: BP006823.D\data.ms

(77) Benzidine

19.316min (+ 0.000) 25598.00 ng

response 1456604

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.17
183.00	11.90	11.90
0.00	0.00	0.00