

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006825.D
 Acq On : 23 Aug 2021 11:01
 Operator : CG/JU
 Sample : PB138596BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB138596BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	308	rVB	77571	112577	1.10%	0.249%
2	5.305	371	377	385	rBV	3386947	4754898	46.27%	10.536%
3	6.887	639	646	659	rBV	3007974	4724799	45.98%	10.469%
4	7.693	778	783	792	rVB	610056	944287	9.19%	2.092%
5	8.858	974	981	990	rBV	1979454	3190438	31.05%	7.069%
6	10.481	1250	1257	1264	rBV	823076	1324833	12.89%	2.936%
7	12.963	1669	1679	1701	rBV	4709839	6801831	66.19%	15.072%
8	14.340	1906	1913	1934	rBV	1083443	1647682	16.03%	3.651%
9	15.840	2161	2168	2195	rBV	3400524	5119061	49.82%	11.343%
10	17.104	2376	2383	2396	rBV	1317644	1925641	18.74%	4.267%
11	19.686	2816	2822	2828	rBV	8531212	10275812	100.00%	22.769%
12	21.210	3077	3081	3087	rBV	1695133	2048760	19.94%	4.540%
13	23.533	3469	3476	3486	rVB	1152700	2259799	21.99%	5.007%




Sum of corrected areas: 45130418

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006825.D
Acq On : 23 Aug 2021 11:01
Operator : CG/JU
Sample : PB138596BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138596BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

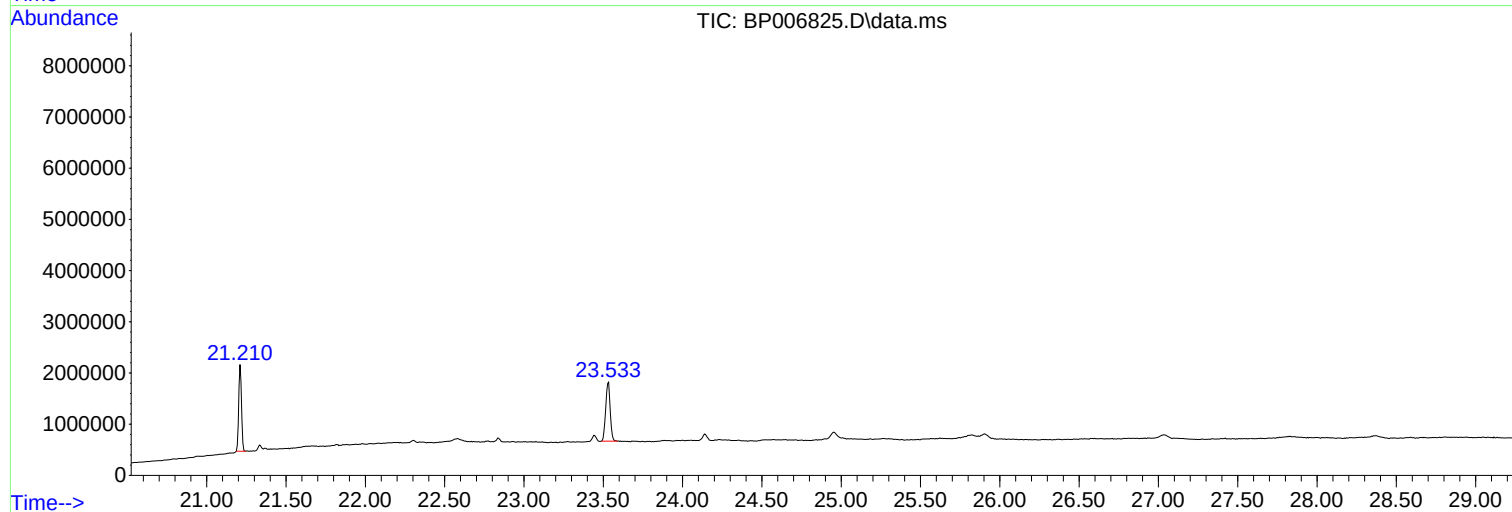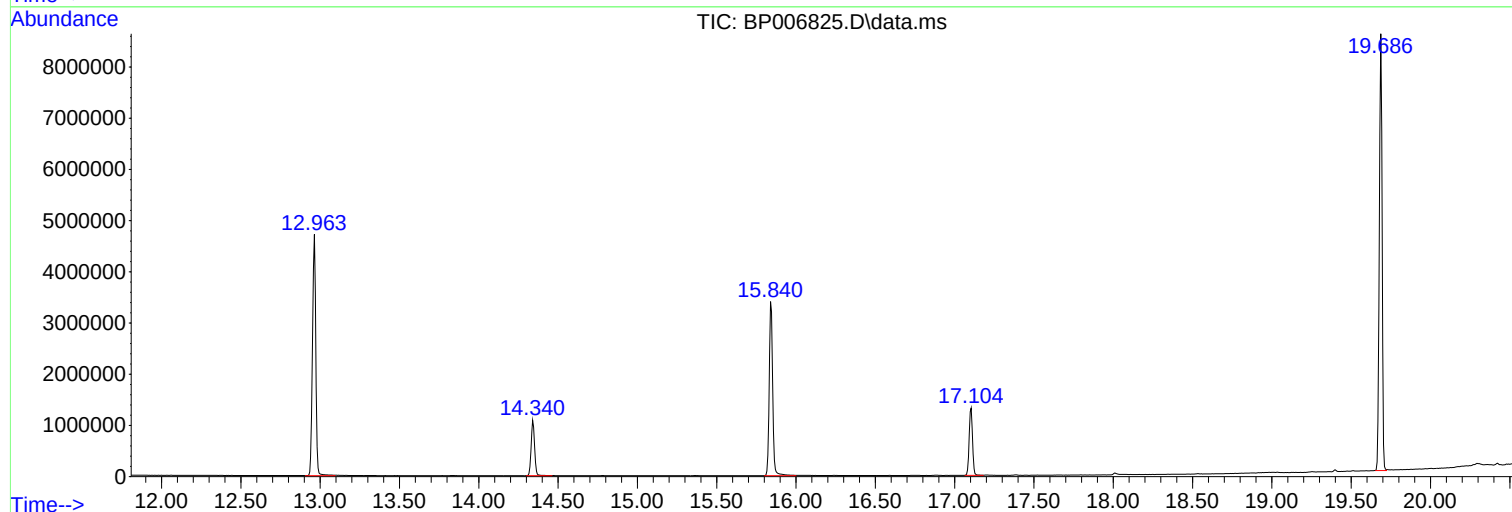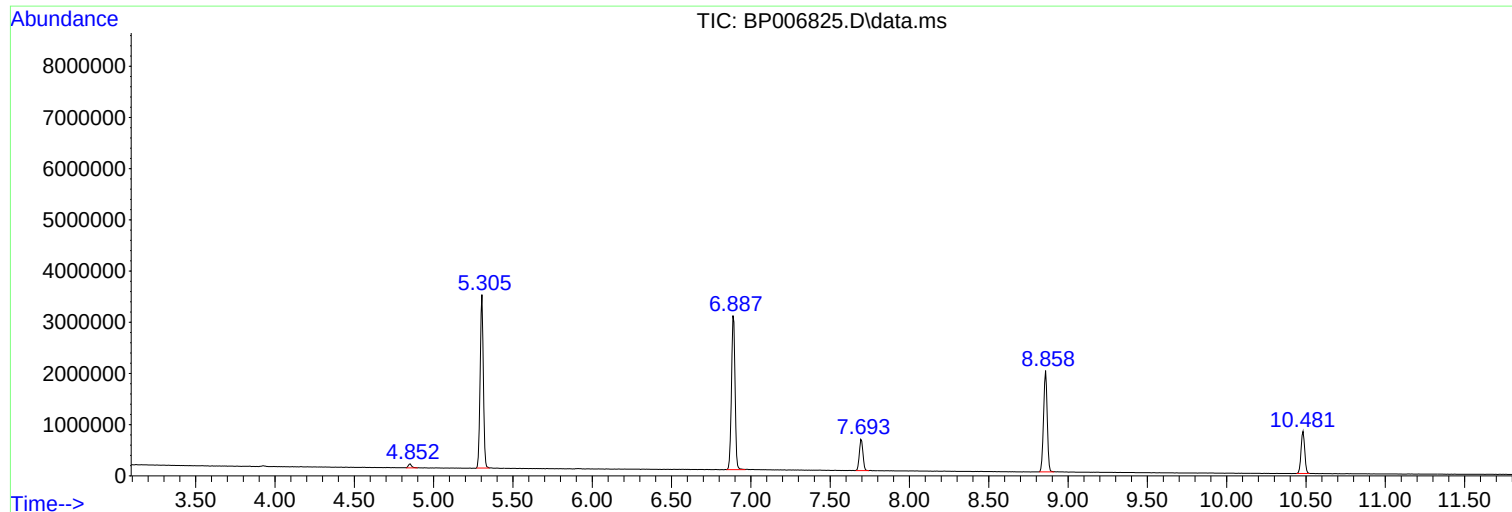

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006825.D
Acq On : 23 Aug 2021 11:01
Operator : CG/JU
Sample : PB138596BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138596BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006825.D
Acq On : 23 Aug 2021 11:01
Operator : CG/JU
Sample : PB138596BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138596BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------