

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006828.D
 Acq On : 23 Aug 2021 13:29
 Operator : CG/JU
 Sample : M3419-23
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-09-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.922	139	142	156	rVB	85645	129803	2.10%	0.228%
2	4.846	295	299	303	rVB	89113	117751	1.90%	0.206%
3	5.299	370	376	382	rBV	2472648	3465824	56.07%	6.075%
4	5.352	382	385	394	rVB	110184	240751	3.89%	0.422%
5	5.717	443	447	454	rVB	130253	186640	3.02%	0.327%
6	6.787	624	629	634	rVB	118382	160844	2.60%	0.282%
7	6.846	635	639	640	rVV	62116	79686	1.29%	0.140%
8	6.887	640	646	657	rVV	2313974	3752919	60.71%	6.578%
9	6.975	657	661	666	rVB	46775	65255	1.06%	0.114%
10	7.081	676	679	689	rVB	63071	102199	1.65%	0.179%
11	7.340	716	723	731	rVB	171865	285286	4.62%	0.500%
12	7.693	777	783	793	rBV	701044	1088543	17.61%	1.908%
13	7.805	798	802	810	rVB	65858	109803	1.78%	0.192%
14	8.234	870	875	881	rVB2	76248	125909	2.04%	0.221%
15	8.328	887	891	897	rVB2	104648	151349	2.45%	0.265%
16	8.793	965	970	974	rBV	66091	102398	1.66%	0.179%
17	8.858	974	981	988	rVV	1526079	2440404	39.48%	4.278%
18	9.369	1064	1068	1078	rVB	54139	97883	1.58%	0.172%
19	10.187	1201	1207	1214	rVB2	52552	98432	1.59%	0.173%
20	10.275	1214	1222	1231	rBV	621003	1049187	16.97%	1.839%
21	10.481	1249	1257	1262	rBV	989742	1676744	27.13%	2.939%
22	10.528	1262	1265	1272	rVB	72181	124874	2.02%	0.219%
23	11.728	1463	1469	1479	rVB3	29299	63035	1.02%	0.110%
24	12.151	1528	1541	1549	rBV2	76377	150158	2.43%	0.263%
25	12.281	1557	1563	1566	rBV	39115	70162	1.14%	0.123%
26	12.369	1574	1578	1588	rVB2	36140	77422	1.25%	0.136%
27	12.963	1670	1679	1691	rBV	3332758	5012174	81.09%	8.786%
28	13.516	1762	1773	1777	rBV7	34566	93961	1.52%	0.165%
29	13.657	1788	1797	1803	rBV4	31034	74208	1.20%	0.130%
30	13.798	1810	1821	1825	rBV5	39165	91344	1.48%	0.160%
31	14.057	1860	1865	1875	rVB	233981	363980	5.89%	0.638%
32	14.340	1907	1913	1920	rBV	1394212	1999602	32.35%	3.505%
33	15.592	2110	2126	2137	rBV4	43805	204245	3.30%	0.358%
34	15.840	2158	2168	2177	rBV	2834181	4032722	65.24%	7.069%
35	16.075	2201	2208	2215	rVB3	67313	167348	2.71%	0.293%
36	16.516	2279	2283	2289	rVB4	56646	82782	1.34%	0.145%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006828.D
Acq On : 23 Aug 2021 13:29
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-09-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.657	2304	2307	2314	rVB5	37169	68665	1.11%	0.120%
38	17.098	2376	2382	2387	rBV	1581273	2326956	37.64%	4.079%
39	17.145	2387	2390	2396	rVV	510584	682095	11.03%	1.196%
40	17.234	2398	2405	2411	rVB	194594	314470	5.09%	0.551%
41	17.422	2433	2437	2441	rVB2	59479	82121	1.33%	0.144%
42	17.510	2450	2452	2461	rVB	61803	93095	1.51%	0.163%
43	17.792	2496	2500	2504	rBV	171022	202041	3.27%	0.354%
44	17.975	2528	2531	2534	rBV2	71527	87224	1.41%	0.153%
45	18.016	2534	2538	2547	rBV2	1469173	2075560	33.58%	3.638%
46	18.163	2560	2563	2567	rVB2	87945	121435	1.96%	0.213%
47	18.463	2611	2614	2618	rBV2	83656	112782	1.82%	0.198%
48	18.504	2618	2621	2631	rVB	121069	175996	2.85%	0.308%
49	19.122	2722	2726	2732	rBV	1147765	1650457	26.70%	2.893%
50	19.263	2745	2750	2758	rBV2	2031479	2913387	47.13%	5.107%
51	19.480	2783	2787	2796	rVB	981462	1328852	21.50%	2.329%
52	19.686	2817	2822	2831	rVB	5227607	6181326	100.00%	10.835%
53	20.369	2936	2938	2941	rBV	179550	152229	2.46%	0.267%
54	20.939	3031	3035	3041	rBV2	1002167	1248731	20.20%	2.189%
55	21.133	3065	3068	3072	rVB	1211516	1296395	20.97%	2.272%
56	21.210	3076	3081	3085	rVV2	2070398	3206247	51.87%	5.620%
57	21.245	3085	3087	3095	rVB	562377	722574	11.69%	1.267%
58	21.845	3185	3189	3196	rVB	1160390	1559776	25.23%	2.734%
59	23.533	3471	3476	3483	rVB2	1257011	2310995	37.39%	4.051%




Sum of corrected areas: 57049036

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006828.D
Acq On : 23 Aug 2021 13:29
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-09-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

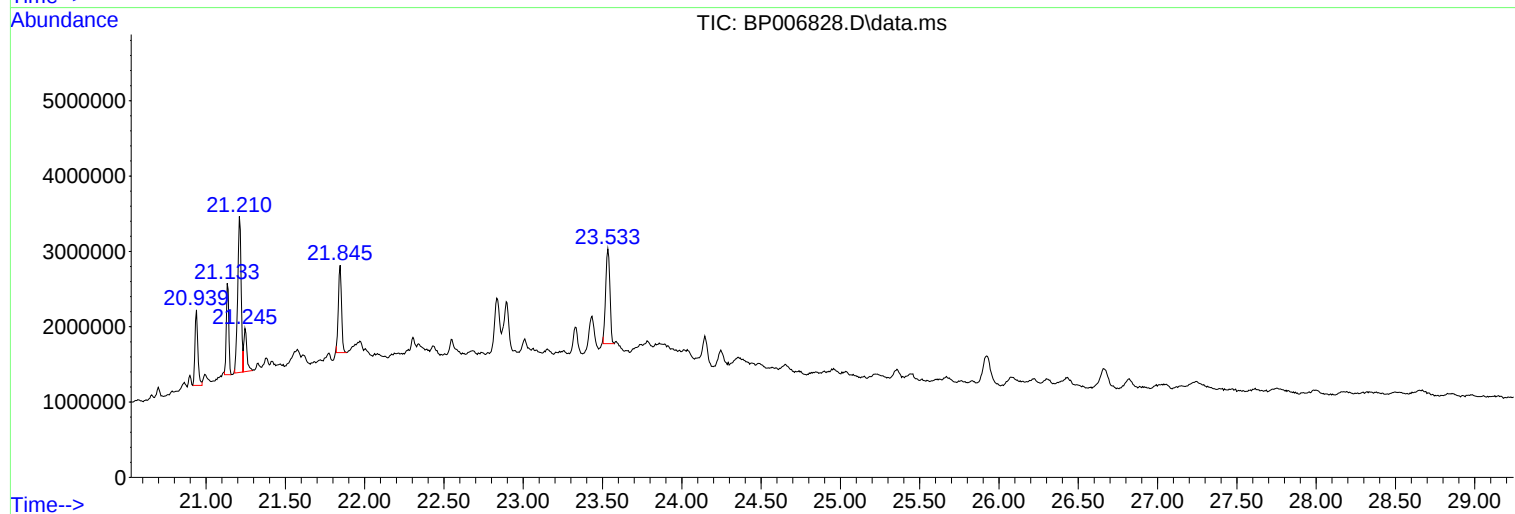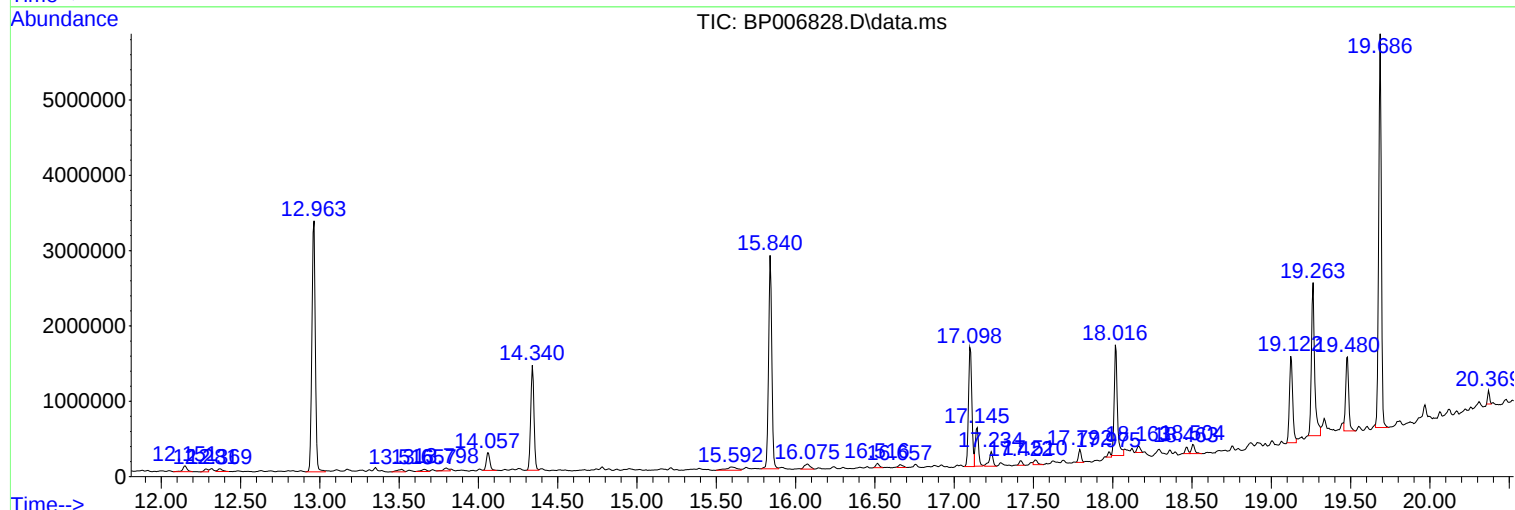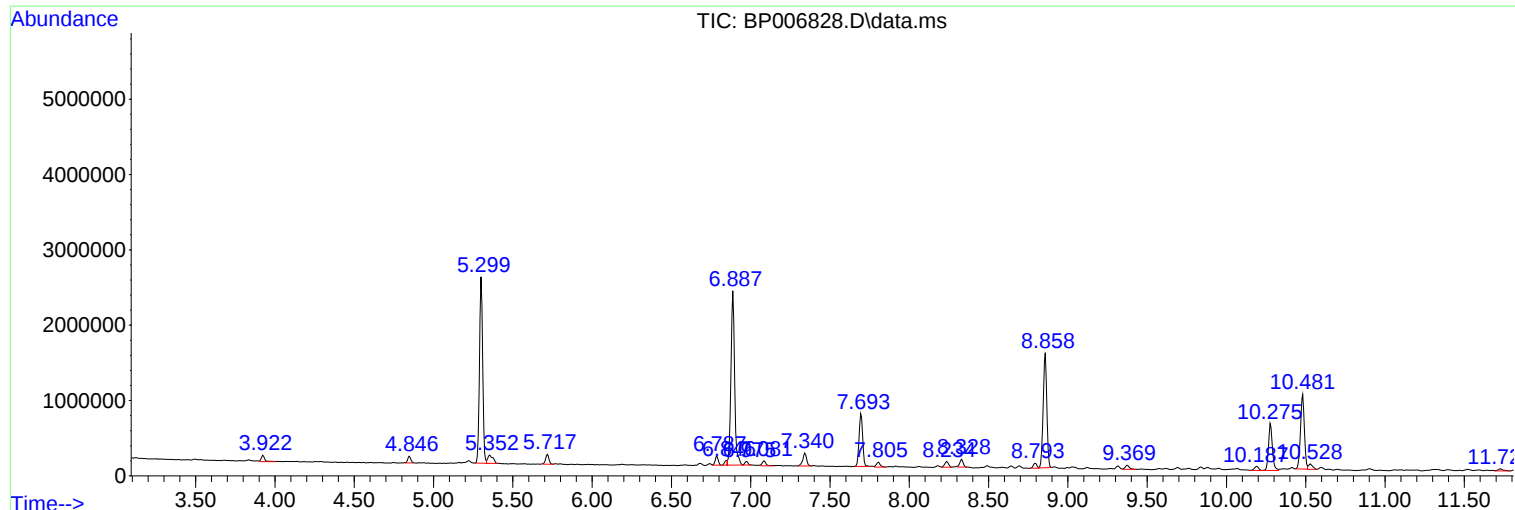

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006828.D
Acq On : 23 Aug 2021 13:29
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-09-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006828.D
Acq On : 23 Aug 2021 13:29
Operator : CG/JU
Sample : M3419-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-09-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------