

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006829.D
 Acq On : 23 Aug 2021 14:04
 Operator : CG/JU
 Sample : M3463-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-18-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006829.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.922	139	142	147	rVB	122655	146744	3.91%	0.383%
2	4.440	226	230	235	rVB2	71862	96507	2.57%	0.252%
3	5.299	370	376	383	rBV	2122245	2967099	79.07%	7.741%
4	6.887	640	646	659	rVB	1930973	2980843	79.44%	7.777%
5	7.693	778	783	791	rVB	535476	848429	22.61%	2.213%
6	8.487	914	918	928	rVB5	26244	50283	1.34%	0.131%
7	8.857	974	981	988	rBV	1243953	2009514	53.55%	5.243%
8	10.275	1215	1222	1232	rBV	249914	445643	11.88%	1.163%
9	10.481	1250	1257	1263	rBV	728747	1190470	31.73%	3.106%
10	10.528	1263	1265	1273	rVB	39646	66068	1.76%	0.172%
11	12.963	1671	1679	1693	rBV	1951980	2932459	78.15%	7.651%
12	13.810	1816	1823	1831	rBV2	57532	107992	2.88%	0.282%
13	14.063	1860	1866	1876	rVB	90142	143264	3.82%	0.374%
14	14.340	1904	1913	1920	rBV	944687	1429647	38.10%	3.730%
15	14.398	1920	1923	1932	rVB5	17706	42245	1.13%	0.110%
16	15.839	2158	2168	2178	rBV	2011130	2938479	78.31%	7.666%
17	16.081	2204	2209	2215	rVB4	35546	64583	1.72%	0.168%
18	16.304	2242	2247	2255	rBV3	37763	74202	1.98%	0.194%
19	16.516	2278	2283	2288	rBV8	28750	49453	1.32%	0.129%
20	16.922	2348	2352	2360	rVB2	30704	50029	1.33%	0.131%
21	17.104	2377	2383	2387	rBV	1239117	1754412	46.75%	4.577%
22	17.145	2387	2390	2397	rVV	268971	398672	10.62%	1.040%
23	17.210	2397	2401	2402	rVV3	37877	49754	1.33%	0.130%
24	17.234	2402	2405	2411	rVB	88684	122914	3.28%	0.321%
25	17.298	2412	2416	2421	rBV4	23364	39401	1.05%	0.103%
26	17.516	2449	2453	2461	rVB2	42794	66190	1.76%	0.173%
27	17.622	2467	2471	2475	rBV2	36467	50737	1.35%	0.132%
28	17.981	2527	2532	2534	rBV	54885	85620	2.28%	0.223%
29	18.016	2534	2538	2547	rVV2	398640	613511	16.35%	1.601%
30	18.157	2557	2562	2567	rBV3	106532	196632	5.24%	0.513%
31	18.428	2605	2608	2611	rBV3	31992	38450	1.02%	0.100%
32	18.469	2612	2615	2618	rVV2	48828	65236	1.74%	0.170%
33	18.504	2619	2621	2627	rVB2	65225	91987	2.45%	0.240%
34	18.745	2658	2662	2666	rBV3	61919	112445	3.00%	0.293%
35	18.869	2677	2683	2688	rBV3	80281	193636	5.16%	0.505%
36	19.128	2722	2727	2733	rBV	735335	999038	26.62%	2.606%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006829.D
Acq On : 23 Aug 2021 14:04
Operator : CG/JU
Sample : M3463-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-18-0002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.257	2746	2749	2756	rBV2	108416	230362	6.14%	0.601%
38	19.451	2779	2782	2783	rBV	75525	81823	2.18%	0.213%
39	19.480	2783	2787	2795	rVB	625935	883444	23.54%	2.305%
40	19.686	2817	2822	2833	rVB	2601605	3159441	84.20%	8.243%
41	19.969	2867	2870	2879	rVB3	198473	289968	7.73%	0.757%
42	20.698	2992	2994	3000	rVB	154924	184976	4.93%	0.483%
43	20.939	3032	3035	3041	rBV2	671066	831158	22.15%	2.168%
44	21.133	3066	3068	3072	rVB	194797	202875	5.41%	0.529%
45	21.210	3076	3081	3085	rVV2	1721461	2672211	71.21%	6.972%
46	21.245	3085	3087	3094	rVB	342911	466924	12.44%	1.218%
47	23.533	3471	3476	3483	rVB2	1118088	2061722	54.94%	5.379%
48	26.986	4056	4063	4079	rVB3	1157726	3752387	100.00%	9.790%




Sum of corrected areas: 38329879

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006829.D
Acq On : 23 Aug 2021 14:04
Operator : CG/JU
Sample : M3463-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-18-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

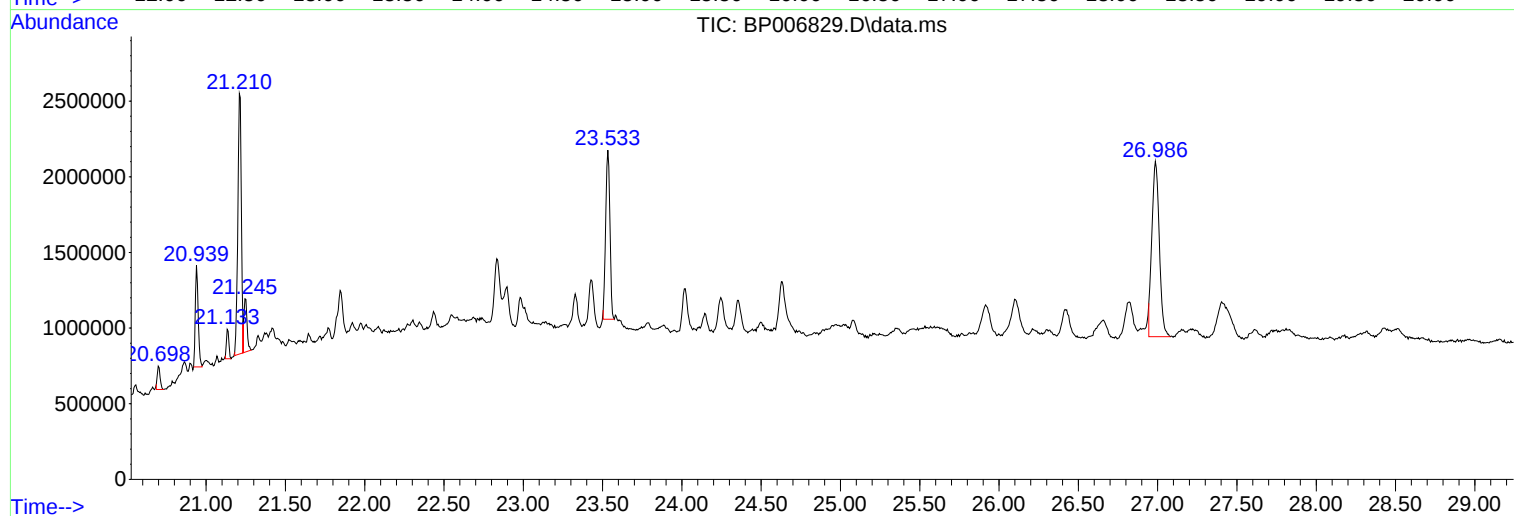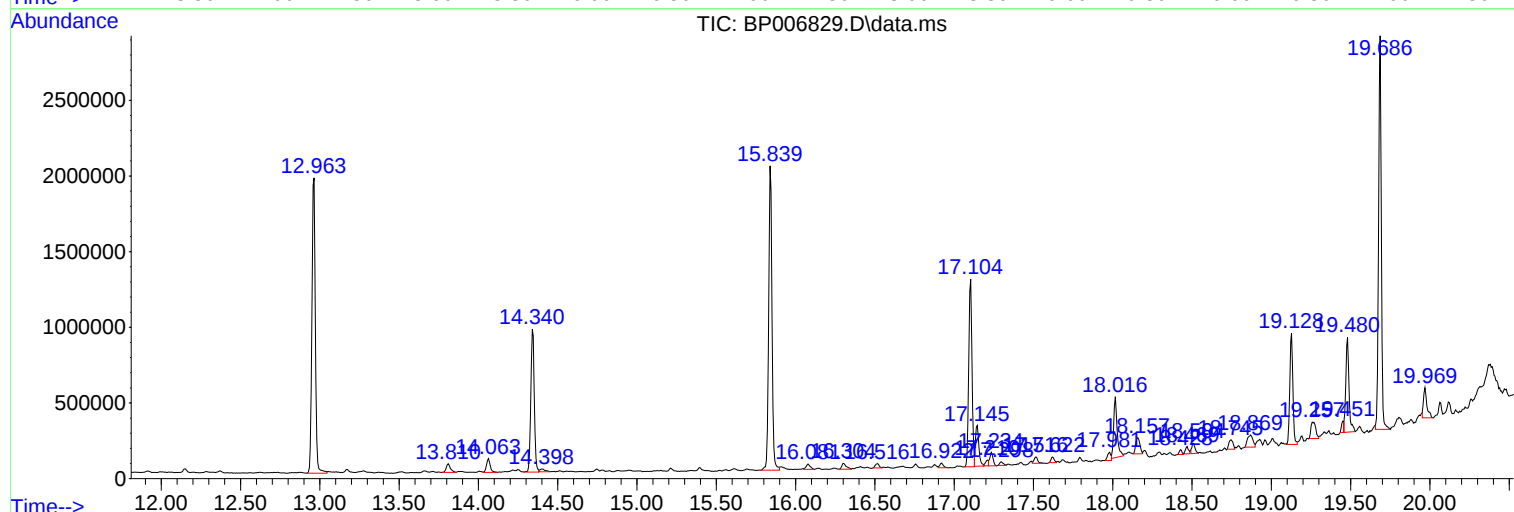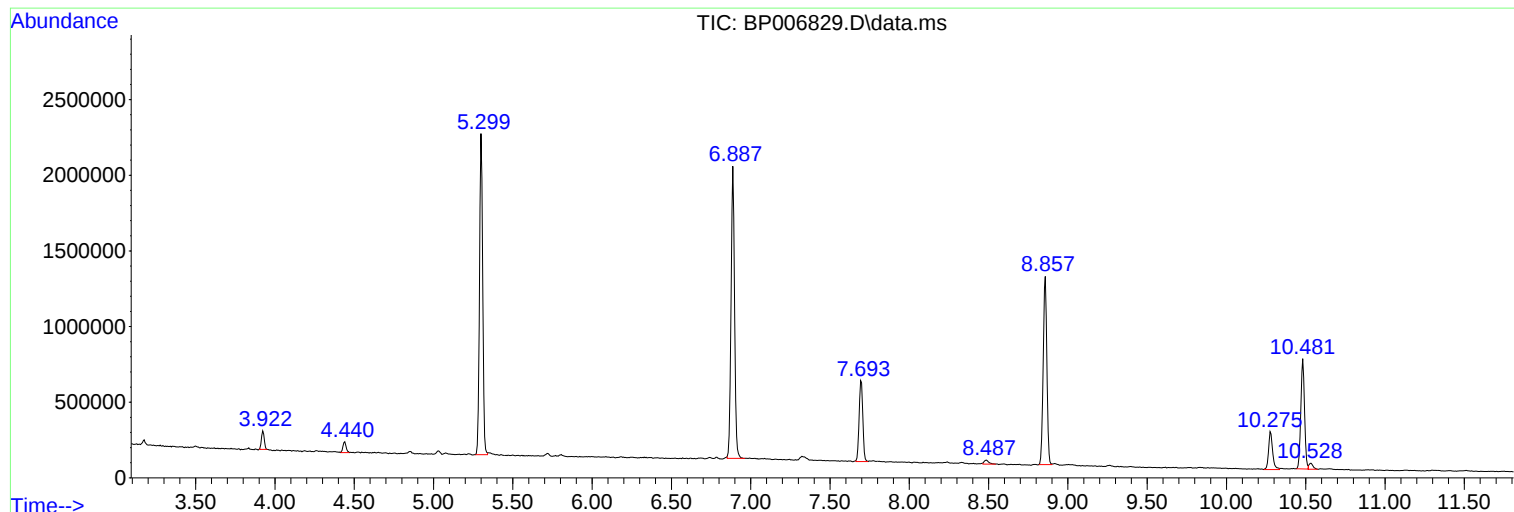

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006829.D
Acq On : 23 Aug 2021 14:04
Operator : CG/JU
Sample : M3463-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-18-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006829.D
Acq On : 23 Aug 2021 14:04
Operator : CG/JU
Sample : M3463-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-18-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
