

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006830.D
 Acq On : 23 Aug 2021 14:38
 Operator : CG/JU
 Sample : M3463-43
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-17-FD-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	370	376	386	rBV	3140433	4599241	50.42%	9.859%
2	6.887	639	646	657	rBV	2934424	4733843	51.90%	10.148%
3	7.693	778	783	790	rVB	556040	857219	9.40%	1.838%
4	8.857	974	981	989	rBV	1939892	3144504	34.47%	6.741%
5	10.275	1217	1222	1233	rBV	195212	345155	3.78%	0.740%
6	10.481	1250	1257	1267	rVB	754435	1234561	13.53%	2.647%
7	12.963	1672	1679	1699	rBV	4599456	6593483	72.29%	14.134%
8	14.340	1907	1913	1922	rBV	1058604	1562605	17.13%	3.350%
9	15.845	2158	2169	2188	rBV	3793643	5607221	61.47%	12.020%
10	17.104	2376	2383	2390	rBV	1287491	1885530	20.67%	4.042%
11	18.016	2533	2538	2552	rBV	270526	484131	5.31%	1.038%
12	19.257	2745	2749	2758	rBV	77079	148932	1.63%	0.319%
13	19.686	2816	2822	2827	rBV	7611457	9121394	100.00%	19.553%
14	20.939	3031	3035	3044	rBV	911574	1255420	13.76%	2.691%
15	21.210	3077	3081	3086	rBV2	1622125	1967209	21.57%	4.217%
16	21.845	3185	3189	3198	rVB2	614213	1093517	11.99%	2.344%
17	23.527	3470	3475	3481	rBV2	1038808	2014519	22.09%	4.319%




Sum of corrected areas: 46648484

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006830.D
Acq On : 23 Aug 2021 14:38
Operator : CG/JU
Sample : M3463-43
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-17-FD-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

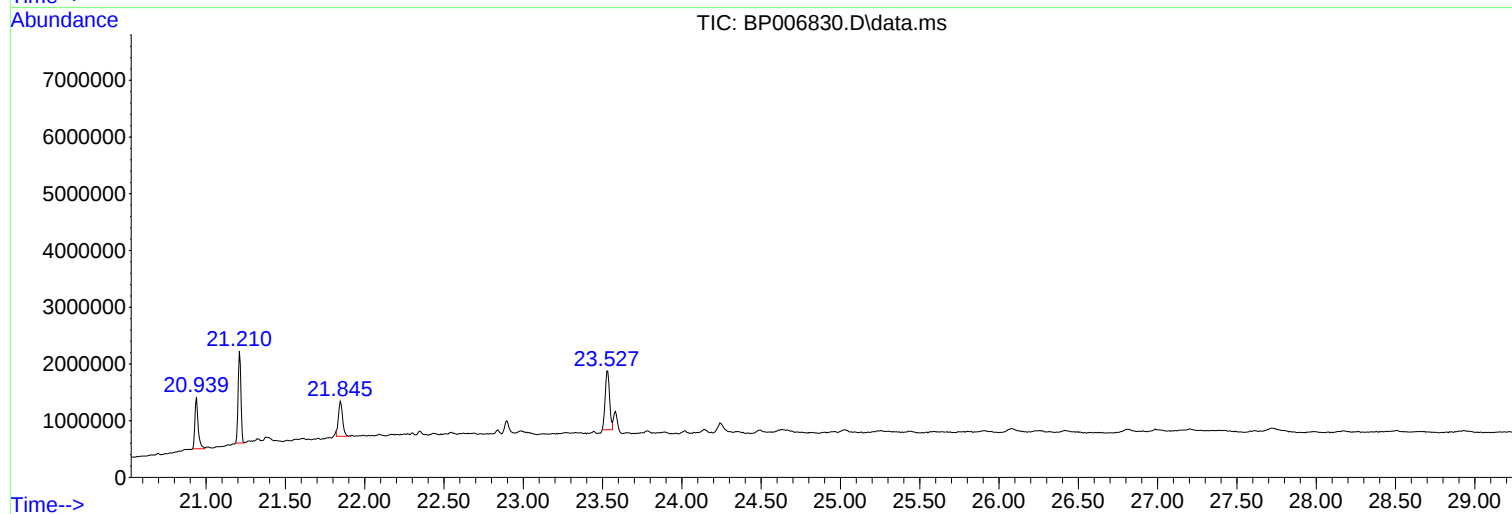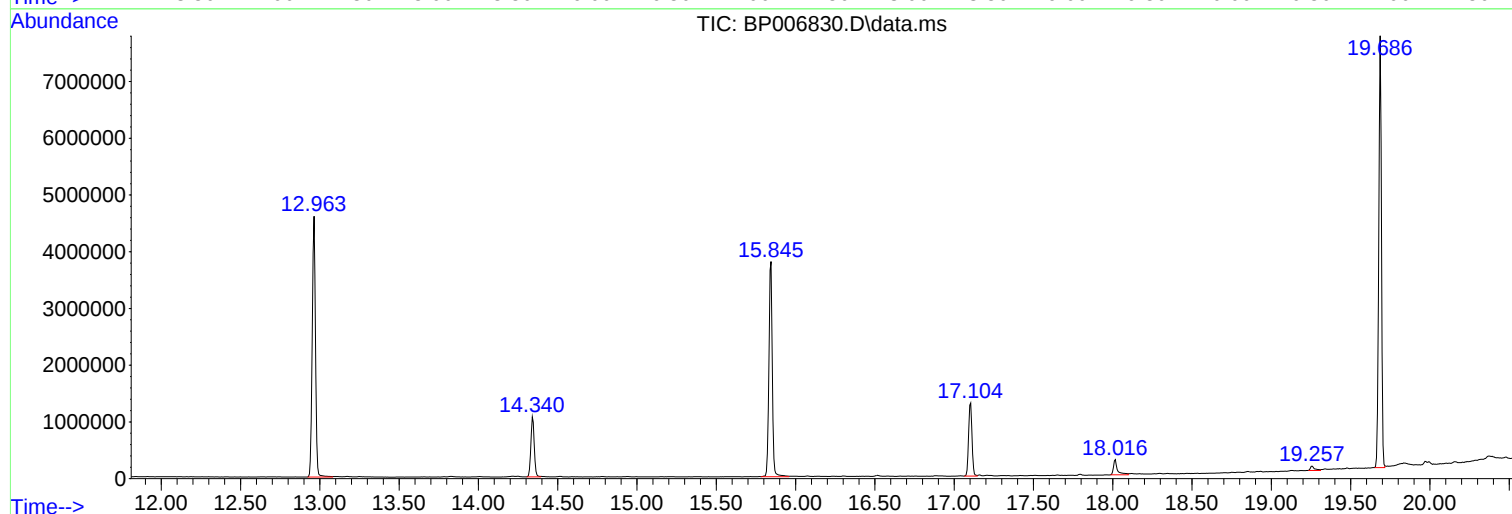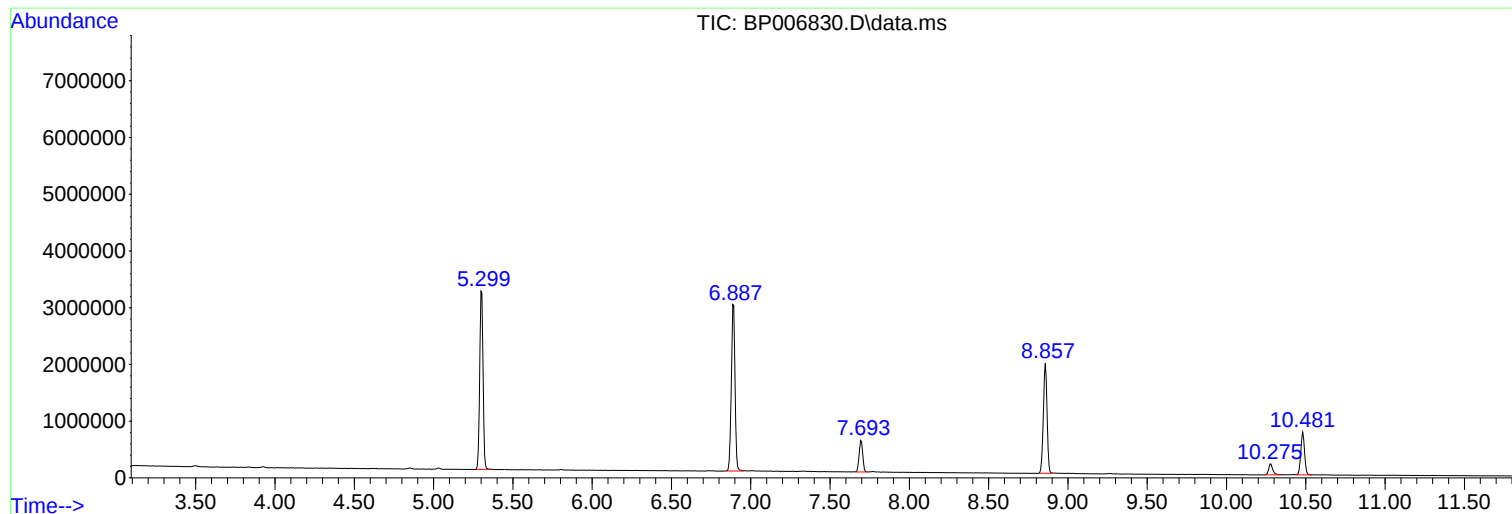

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006830.D
Acq On : 23 Aug 2021 14:38
Operator : CG/JU
Sample : M3463-43
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-17-FD-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006830.D
Acq On : 23 Aug 2021 14:38
Operator : CG/JU
Sample : M3463-43
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-17-FD-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
