

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006831.D
 Acq On : 23 Aug 2021 15:12
 Operator : CG/JU
 Sample : M3463-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-20-0306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.298	371	376	389	rVB	2308236	3342981	73.42%	6.252%
2	6.887	639	646	657	rBV	2236419	3461027	76.01%	6.473%
3	7.692	777	783	790	rBV	596469	956757	21.01%	1.789%
4	8.857	974	981	990	rBV	1431910	2335854	51.30%	4.369%
5	10.275	1216	1222	1235	rBV	231577	408516	8.97%	0.764%
6	10.481	1250	1257	1267	rVB	858816	1415845	31.09%	2.648%
7	12.963	1672	1679	1695	rBV	2458970	3673277	80.67%	6.870%
8	13.275	1724	1732	1737	rBV	33244	55956	1.23%	0.105%
9	13.810	1817	1823	1832	rBV2	19872	50358	1.11%	0.094%
10	14.216	1880	1892	1905	rBV7	20456	63369	1.39%	0.119%
11	14.339	1905	1913	1921	rBV	1241647	1771995	38.92%	3.314%
12	15.839	2158	2168	2192	rBV	2457123	3635835	79.85%	6.800%
13	16.304	2242	2247	2256	rBV	70364	107273	2.36%	0.201%
14	16.510	2276	2282	2291	rBV3	111091	206098	4.53%	0.385%
15	17.104	2376	2383	2389	rBV	1447145	2098099	46.08%	3.924%
16	17.163	2389	2393	2397	rVV	125571	178650	3.92%	0.334%
17	17.204	2397	2400	2408	rVB2	39617	63133	1.39%	0.118%
18	17.486	2444	2448	2450	rBV2	39351	54030	1.19%	0.101%
19	17.621	2466	2471	2475	rBV	50754	71952	1.58%	0.135%
20	18.015	2533	2538	2548	rBV	301283	500409	10.99%	0.936%
21	18.151	2557	2561	2565	rVB3	46913	56500	1.24%	0.106%
22	18.751	2658	2663	2670	rBV4	83136	151169	3.32%	0.283%
23	18.851	2676	2680	2687	rBV	241048	345474	7.59%	0.646%
24	18.962	2695	2699	2703	rBV	127716	141190	3.10%	0.264%
25	19.257	2745	2749	2757	rBV	82639	145870	3.20%	0.273%
26	19.686	2817	2822	2827	rVB	3110613	3649281	80.14%	6.825%
27	19.968	2866	2870	2873	rBV	278444	374994	8.24%	0.701%
28	20.657	2984	2987	2990	rBV2	76459	82391	1.81%	0.154%
29	20.698	2992	2994	2999	rVB	96808	100961	2.22%	0.189%
30	20.939	3031	3035	3045	rBV	968907	1587285	34.86%	2.969%
31	21.062	3053	3056	3061	rVB	362803	447330	9.82%	0.837%
32	21.121	3063	3066	3071	rVB	284000	335322	7.36%	0.627%
33	21.209	3077	3081	3090	rBV	1724805	2226237	48.89%	4.164%
34	21.398	3110	3113	3121	rVB	317607	451022	9.91%	0.844%
35	21.856	3182	3191	3198	rBV2	1953017	3475162	76.32%	6.500%
36	22.351	3271	3275	3283	rVB	634344	955499	20.98%	1.787%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006831.D
Acq On : 23 Aug 2021 15:12
Operator : CG/JU
Sample : M3463-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-20-0306

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	22.839	3354	3358	3362	rBV	398733	567196	12.46%	1.061%
38	22.898	3362	3368	3376	rVV2	1438851	2655341	58.31%	4.966%
39	22.980	3378	3382	3390	rVB	762923	1182457	25.97%	2.212%
40	23.527	3469	3475	3484	rVB2	1392154	2819843	61.93%	5.274%
41	24.239	3591	3596	3608	rVV	547134	1279308	28.10%	2.393%
42	24.350	3610	3615	3628	rVB	628998	1432619	31.46%	2.679%
43	26.980	4055	4062	4076	rVB3	1419452	4553453	100.00%	8.516%




Sum of corrected areas: 53467318

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006831.D
Acq On : 23 Aug 2021 15:12
Operator : CG/JU
Sample : M3463-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-20-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

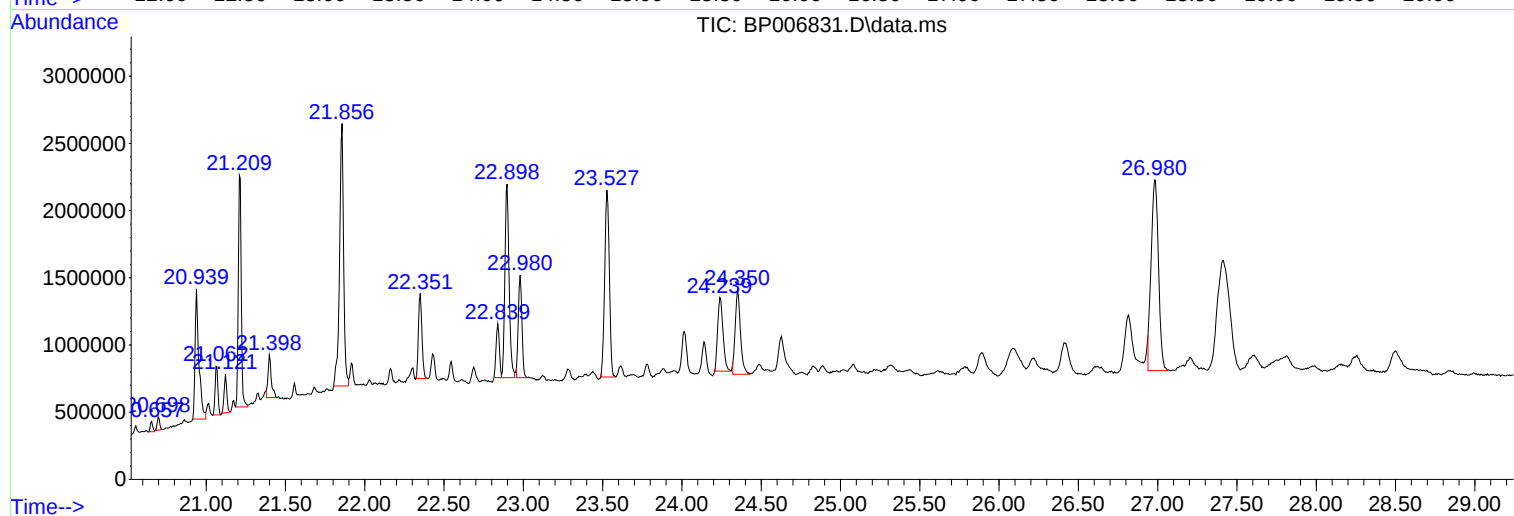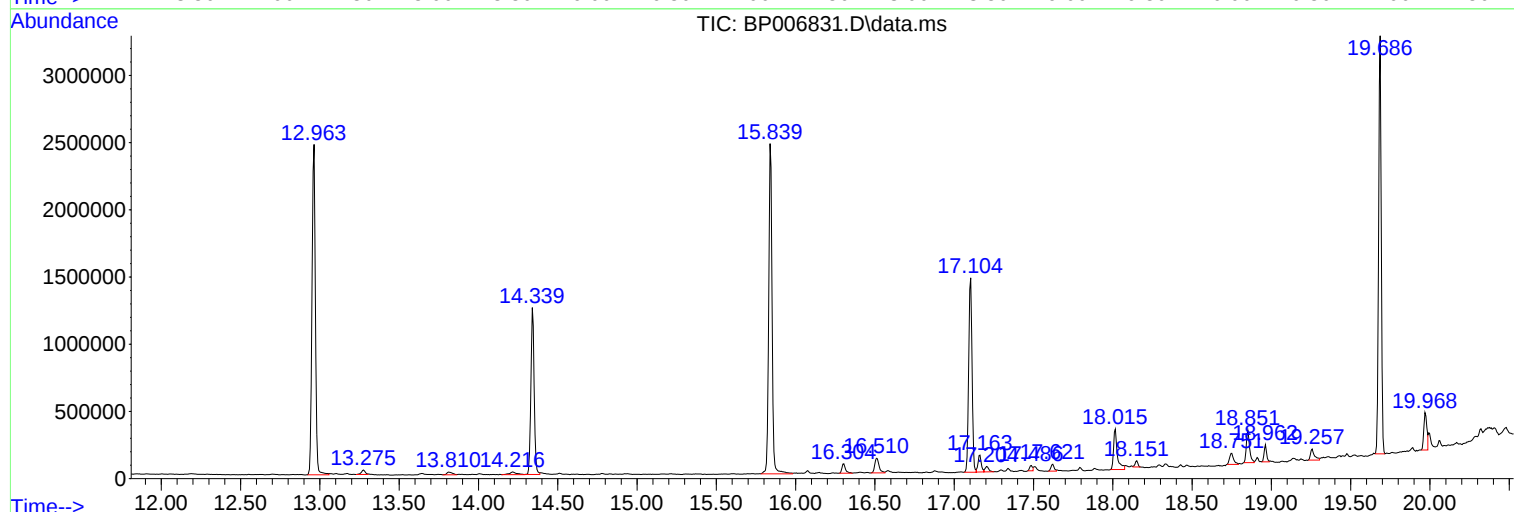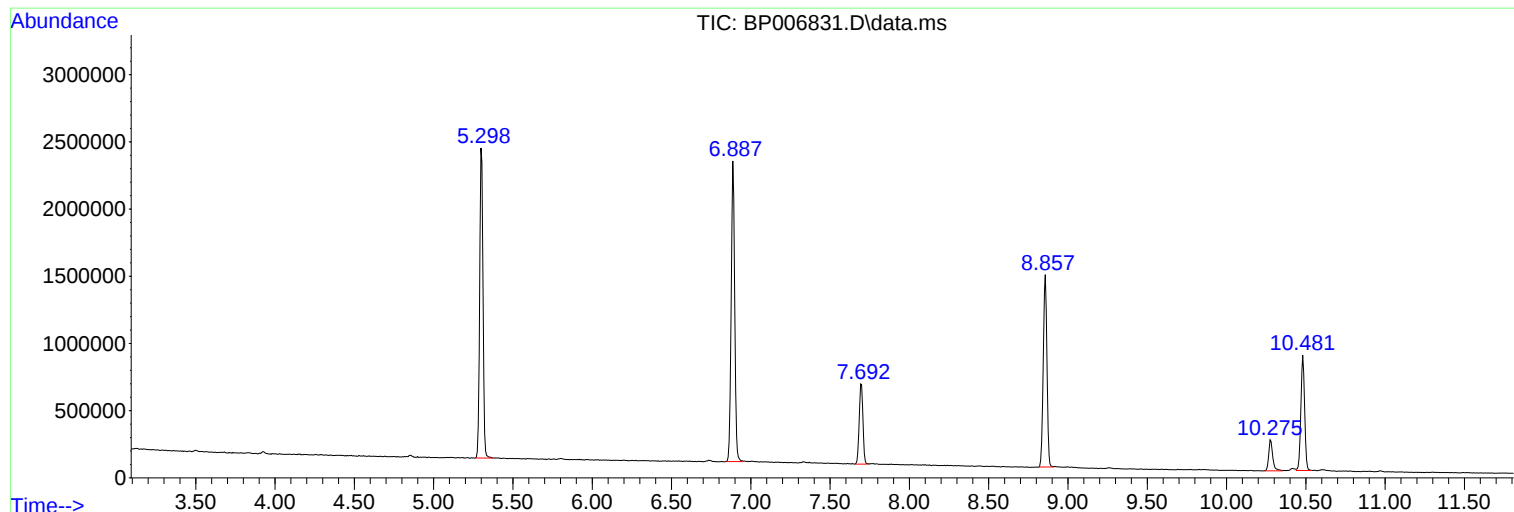

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006831.D
Acq On : 23 Aug 2021 15:12
Operator : CG/JU
Sample : M3463-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-20-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006831.D
Acq On : 23 Aug 2021 15:12
Operator : CG/JU
Sample : M3463-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-20-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------