

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006834.D
 Acq On : 23 Aug 2021 16:55
 Operator : CG/JU
 Sample : M3463-35
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-27-0204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	370	376	389	rVB	3141575	4428636	51.26%	10.322%
2	6.887	639	646	659	rBV	2910787	4540013	52.55%	10.582%
3	7.693	777	783	790	rVB	546676	841023	9.73%	1.960%
4	8.858	974	981	991	rBV	1838601	3030333	35.07%	7.063%
5	10.275	1216	1222	1238	rBV	521960	882641	10.22%	2.057%
6	10.481	1250	1257	1268	rVB	700622	1200504	13.89%	2.798%
7	12.963	1670	1679	1693	rBV	3958800	6168348	71.39%	14.377%
8	14.340	1906	1913	1930	rBV	988237	1475151	17.07%	3.438%
9	15.840	2157	2168	2193	rBV	3530162	5233910	60.58%	12.199%
10	17.098	2376	2382	2389	rBV	1208649	1733356	20.06%	4.040%
11	18.010	2532	2537	2546	rBV	110248	184628	2.14%	0.430%
12	19.686	2816	2822	2827	rBV	7192576	8639880	100.00%	20.138%
13	20.939	3032	3035	3041	rVB	191523	238669	2.76%	0.556%
14	21.210	3076	3081	3086	rBV	1596553	2077780	24.05%	4.843%
15	23.527	3469	3475	3487	rVB2	1125533	2229043	25.80%	5.195%




Sum of corrected areas: 42903915

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006834.D
Acq On : 23 Aug 2021 16:55
Operator : CG/JU
Sample : M3463-35
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-27-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

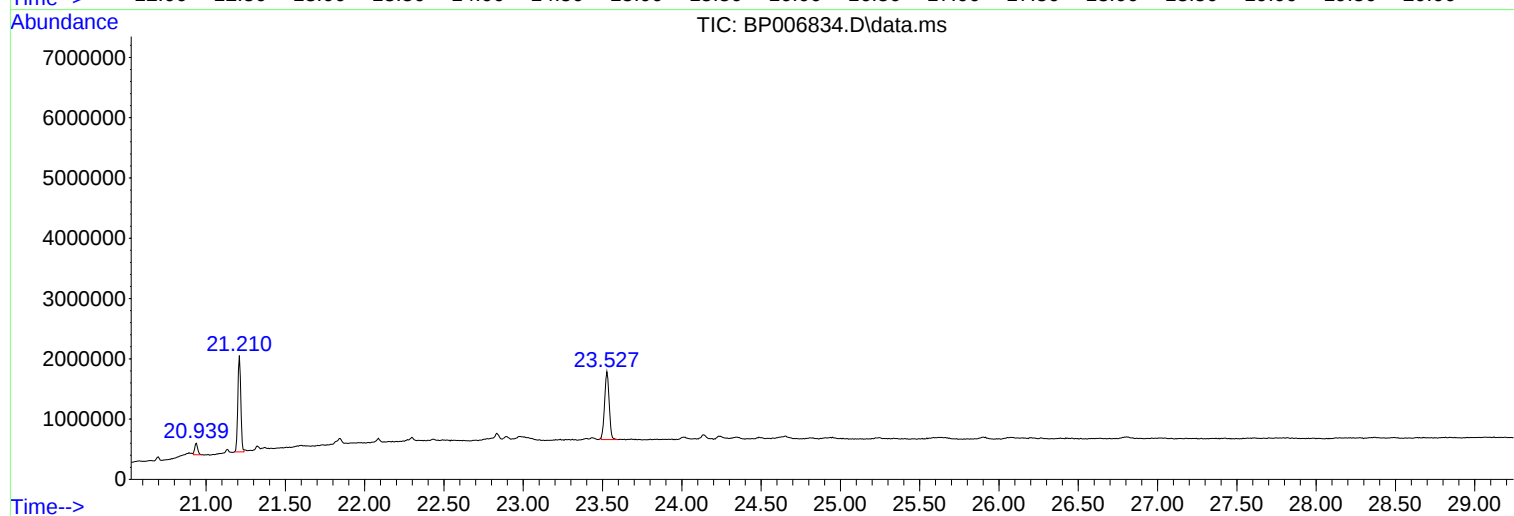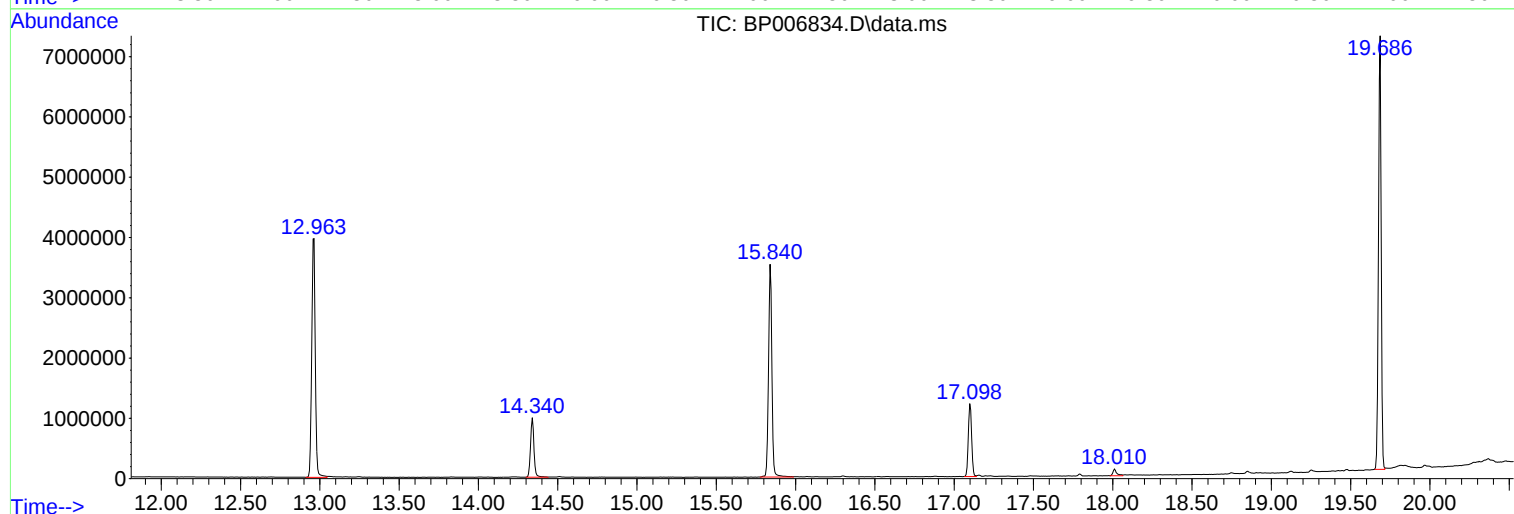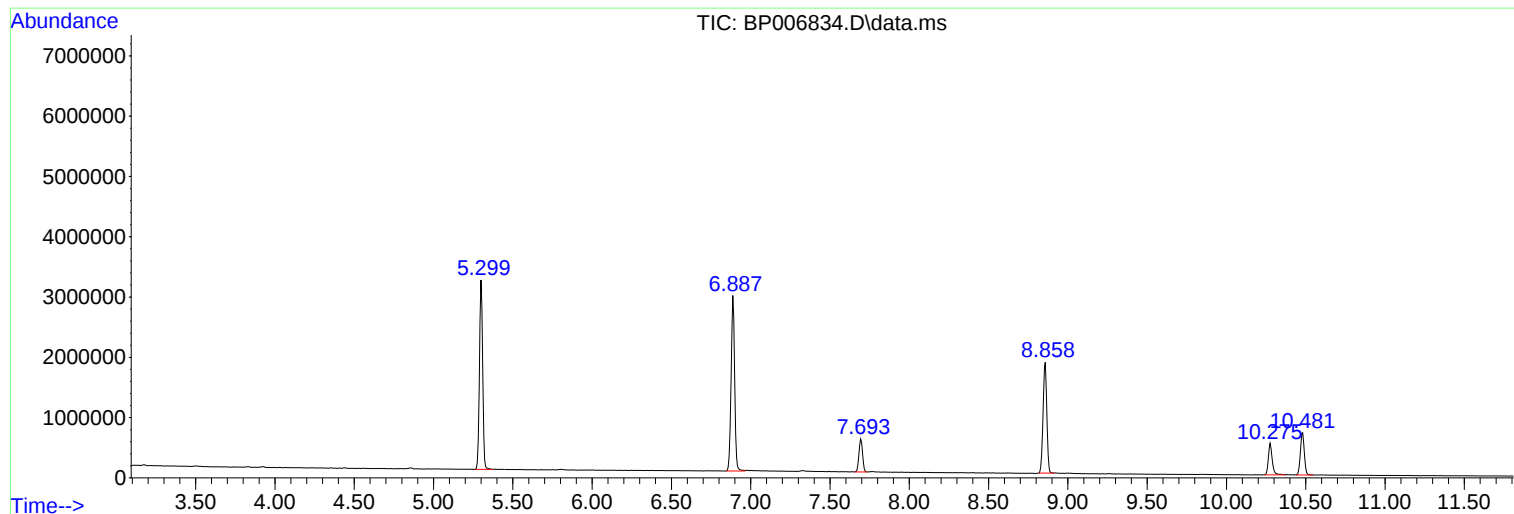

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006834.D
Acq On : 23 Aug 2021 16:55
Operator : CG/JU
Sample : M3463-35
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-27-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006834.D
Acq On : 23 Aug 2021 16:55
Operator : CG/JU
Sample : M3463-35
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-27-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------