

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006836.D
 Acq On : 23 Aug 2021 18:04
 Operator : CG/JU
 Sample : M3502-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 POST-MAEC-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	23	rVB	89015	127457	1.59%	0.215%
2	5.305	371	377	395	rVB	3116196	4471872	55.90%	7.527%
3	6.893	640	647	658	rVB	2909406	4638959	57.99%	7.808%
4	7.693	777	783	792	rVB	643240	1028503	12.86%	1.731%
5	8.857	974	981	988	rBV	1923589	3100045	38.75%	5.218%
6	10.275	1217	1222	1230	rBV	106345	186122	2.33%	0.313%
7	10.481	1249	1257	1263	rBV	890951	1510619	18.88%	2.542%
8	11.316	1391	1399	1409	rBV2	65851	122703	1.53%	0.207%
9	12.963	1670	1679	1696	rBV	4311347	6287837	78.60%	10.583%
10	13.245	1721	1727	1735	rBV	194053	316506	3.96%	0.533%
11	14.339	1903	1913	1920	rBV	1258009	1866099	23.33%	3.141%
12	15.616	2124	2130	2138	rVB4	50817	109654	1.37%	0.185%
13	15.839	2162	2168	2177	rBV	3490659	4979812	62.25%	8.381%
14	16.075	2204	2208	2210	rBV	93243	130479	1.63%	0.220%
15	16.922	2349	2352	2361	rVB	80659	135643	1.70%	0.228%
16	17.104	2377	2383	2387	rBV	1407281	2121198	26.51%	3.570%
17	17.145	2387	2390	2396	rVB	247294	337480	4.22%	0.568%
18	17.233	2402	2405	2411	rVB	72444	99044	1.24%	0.167%
19	17.616	2467	2470	2474	rBV4	69465	85117	1.06%	0.143%
20	18.016	2534	2538	2548	rBV2	720562	1085078	13.56%	1.826%
21	18.286	2580	2584	2590	rBV2	327735	465571	5.82%	0.784%
22	18.486	2614	2618	2628	rVB	841923	1153239	14.42%	1.941%
23	18.698	2652	2654	2658	rVB	132510	133725	1.67%	0.225%
24	18.851	2677	2680	2683	rBV2	201708	265513	3.32%	0.447%
25	18.892	2683	2687	2695	rVB	575473	845554	10.57%	1.423%
26	19.127	2722	2727	2730	rBV	488884	708677	8.86%	1.193%
27	19.186	2734	2737	2741	rVB2	147947	204054	2.55%	0.343%
28	19.257	2746	2749	2758	rVV5	271778	654758	8.18%	1.102%
29	19.474	2783	2786	2790	rVB	355422	414121	5.18%	0.697%
30	19.639	2811	2814	2817	rBV2	171619	228541	2.86%	0.385%
31	19.686	2817	2822	2831	rVB	6775661	8000006	100.00%	13.465%
32	19.886	2853	2856	2861	rVB	602807	702774	8.78%	1.183%
33	20.686	2989	2992	2998	rVB3	637457	738412	9.23%	1.243%
34	20.939	3031	3035	3043	rVB	1149948	1654059	20.68%	2.784%
35	21.016	3045	3048	3055	rVB3	516885	686059	8.58%	1.155%
36	21.210	3076	3081	3084	rBV	1841870	2588310	32.35%	4.356%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006836.D
Acq On : 23 Aug 2021 18:04
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.610	3145	3149	3155	rVB	1142893	1394782	17.43%	2.348%
38	21.680	3157	3161	3169	rVB	1046577	1313469	16.42%	2.211%
39	22.268	3257	3261	3265	rVB	694049	920156	11.50%	1.549%
40	22.733	3336	3340	3346	rVB2	923411	1403477	17.54%	2.362%
41	23.533	3471	3476	3482	rVB2	1187149	2199506	27.49%	3.702%




Sum of corrected areas: 59414990

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006836.D
Acq On : 23 Aug 2021 18:04
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

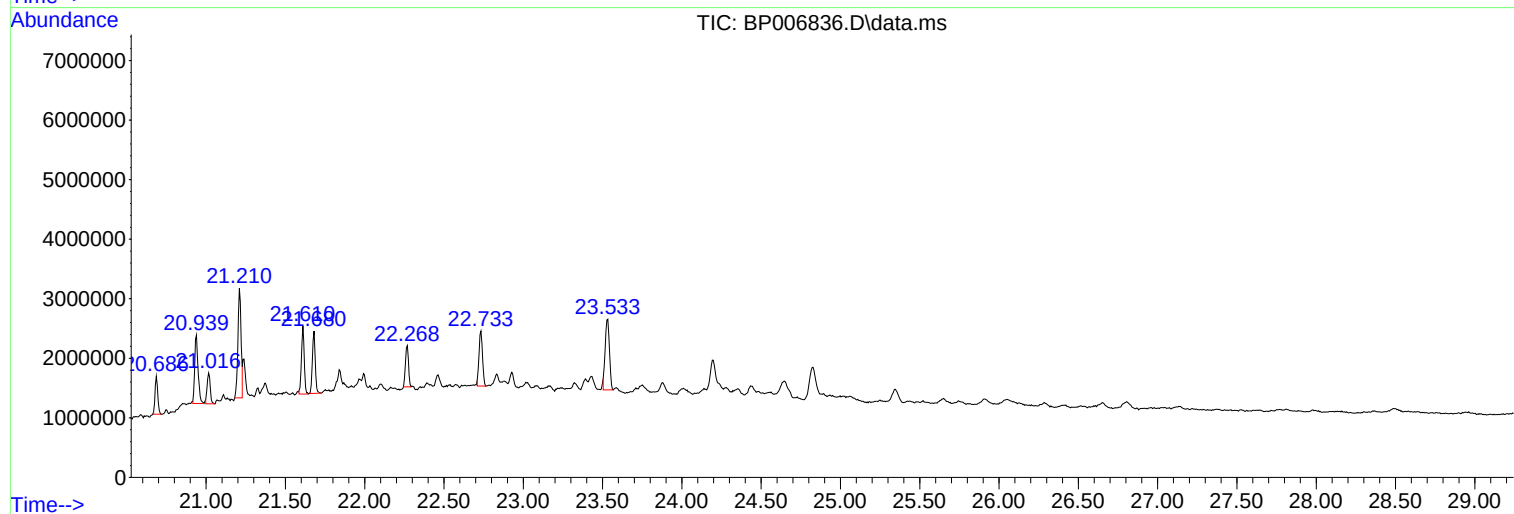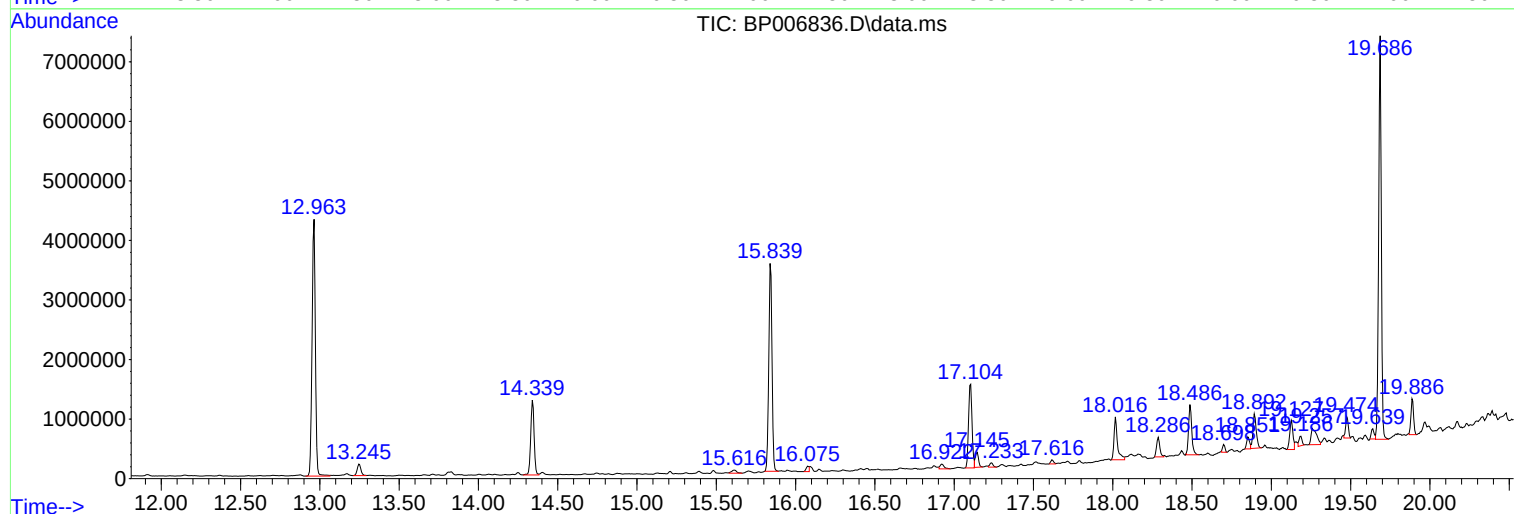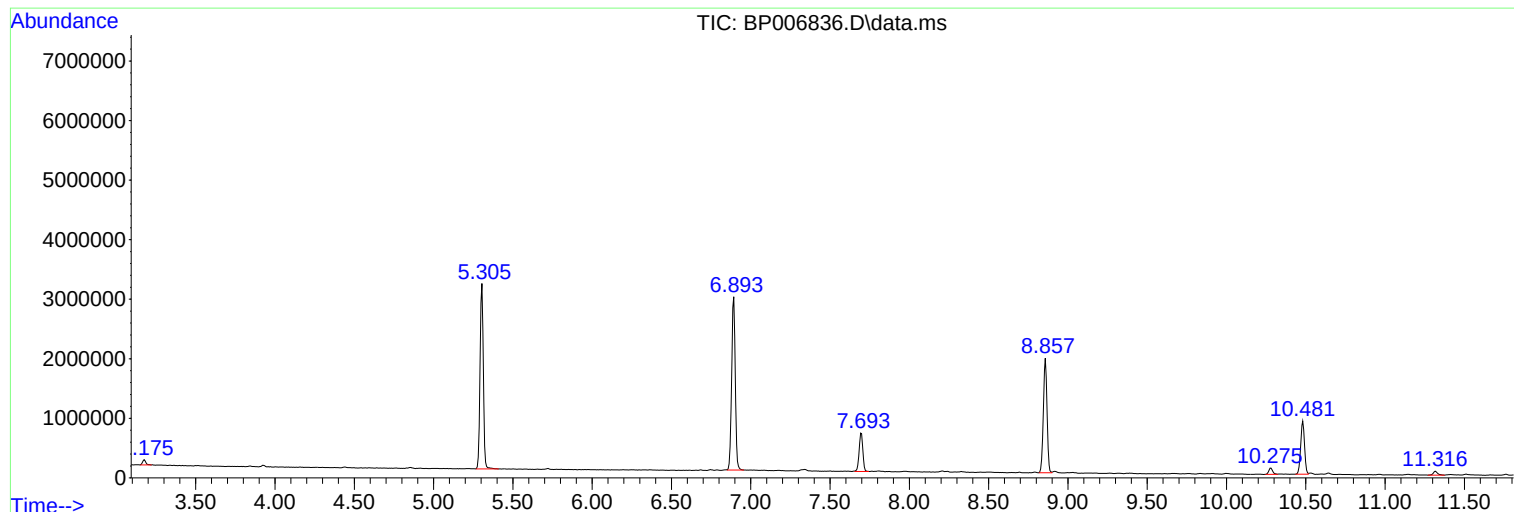

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006836.D
Acq On : 23 Aug 2021 18:04
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006836.D
Acq On : 23 Aug 2021 18:04
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------