

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006837.D
 Acq On : 23 Aug 2021 18:38
 Operator : CG/JU
 Sample : M3463-39
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-29-0204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	22	rVB	150736	216728	2.20%	0.393%
2	4.440	226	230	238	rVB2	89179	132352	1.34%	0.240%
3	5.304	371	377	386	rBV	3785824	5320176	53.94%	9.642%
4	6.893	640	647	658	rBV	3585528	5556226	56.33%	10.070%
5	7.693	778	783	792	rVB	639323	1015593	10.30%	1.841%
6	8.857	973	981	999	rBV	2296265	3734649	37.86%	6.769%
7	10.275	1216	1222	1231	rBV	225413	393901	3.99%	0.714%
8	10.481	1250	1257	1264	rBV	888113	1470623	14.91%	2.665%
9	12.963	1671	1679	1693	rBV	5260971	7765270	78.73%	14.074%
10	14.339	1906	1913	1922	rBV	1223737	1836126	18.62%	3.328%
11	15.839	2158	2168	2178	rBV	4123245	6142413	62.28%	11.133%
12	17.098	2376	2382	2387	rBV	1421856	2081478	21.10%	3.773%
13	17.157	2387	2392	2396	rVB2	266552	381246	3.87%	0.691%
14	17.480	2443	2447	2451	rBV	129066	180640	1.83%	0.327%
15	18.015	2533	2538	2547	rBV	280038	464630	4.71%	0.842%
16	19.121	2723	2726	2731	rBV	193986	249056	2.53%	0.451%
17	19.257	2746	2749	2755	rBV2	92468	144214	1.46%	0.261%
18	19.474	2783	2786	2790	rVB	171284	186129	1.89%	0.337%
19	19.686	2816	2822	2827	rBV	8538475	9863365	100.00%	17.877%
20	20.857	3018	3021	3026	rVB	685737	820764	8.32%	1.488%
21	20.933	3031	3034	3040	rVV	426066	548328	5.56%	0.994%
22	21.068	3054	3057	3062	rBV3	286078	391697	3.97%	0.710%
23	21.133	3065	3068	3074	rVB	533368	527161	5.34%	0.955%
24	21.209	3077	3081	3085	rBV	1785247	2169731	22.00%	3.932%
25	22.833	3353	3357	3362	rBV2	803292	1190257	12.07%	2.157%
26	23.527	3470	3475	3484	rVB2	1205067	2392120	24.25%	4.336%




Sum of corrected areas: 55174873

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006837.D
Acq On : 23 Aug 2021 18:38
Operator : CG/JU
Sample : M3463-39
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-29-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

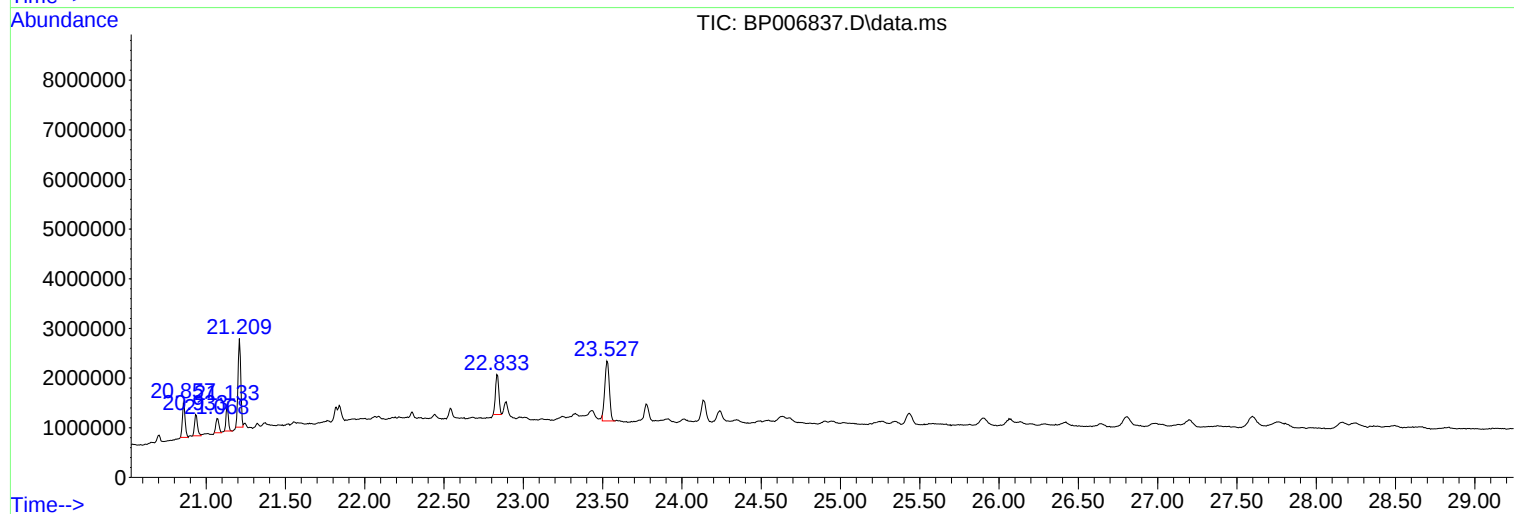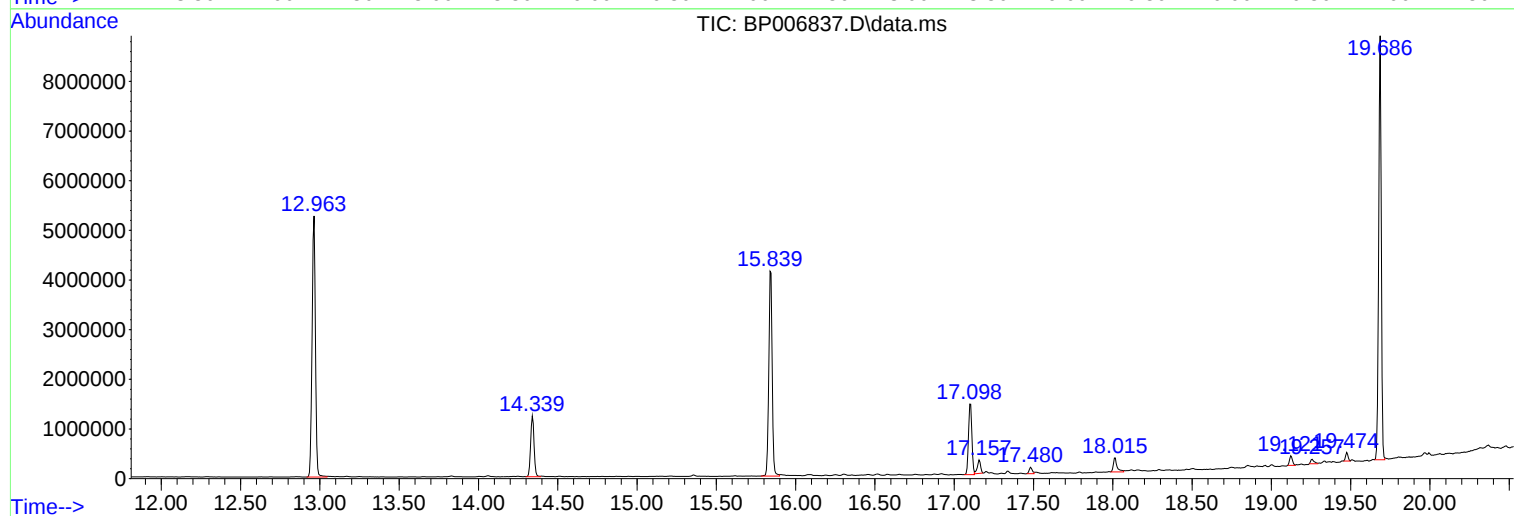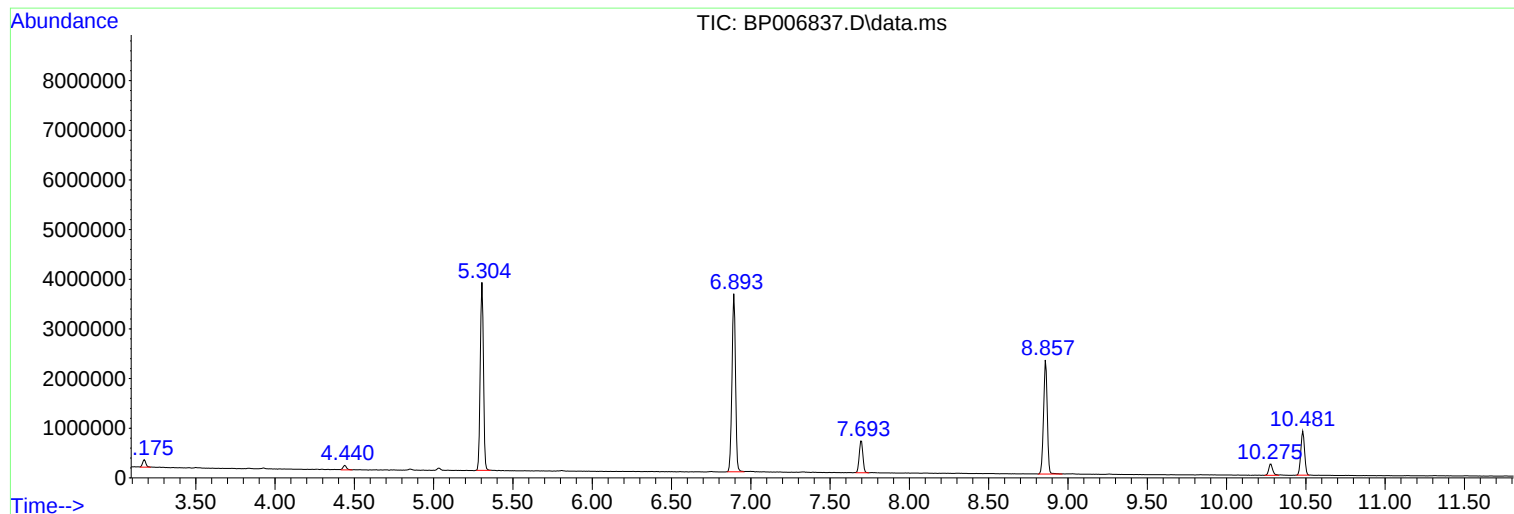

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006837.D
Acq On : 23 Aug 2021 18:38
Operator : CG/JU
Sample : M3463-39
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-29-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006837.D
Acq On : 23 Aug 2021 18:38
Operator : CG/JU
Sample : M3463-39
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-29-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
