

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006838.D
 Acq On : 23 Aug 2021 19:12
 Operator : CG/JU
 Sample : M3502-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 POST-MAEC-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	25	rVB	189793	265150	3.32%	0.453%
2	5.305	370	377	393	rBV	2992717	4385799	54.97%	7.486%
3	6.893	640	647	659	rVB	2860712	4518332	56.64%	7.712%
4	7.693	777	783	791	rVB	662153	1035139	12.98%	1.767%
5	8.857	974	981	988	rBV	1865665	3056712	38.32%	5.217%
6	10.275	1217	1222	1232	rBV	109326	195705	2.45%	0.334%
7	10.481	1249	1257	1263	rBV	943542	1545244	19.37%	2.637%
8	11.316	1388	1399	1409	rBV2	60797	121611	1.52%	0.208%
9	12.963	1669	1679	1693	rBV	4211731	6282036	78.74%	10.722%
10	13.245	1721	1727	1736	rVB	62011	104798	1.31%	0.179%
11	13.810	1817	1823	1830	rBV2	86461	198620	2.49%	0.339%
12	14.340	1907	1913	1920	rBV	1329355	1864095	23.37%	3.182%
13	15.610	2124	2129	2137	rVB2	51915	105085	1.32%	0.179%
14	15.839	2162	2168	2177	rBV	3540777	5014523	62.86%	8.559%
15	16.081	2204	2209	2210	rBV2	90173	136544	1.71%	0.233%
16	16.922	2349	2352	2360	rVB2	84641	139913	1.75%	0.239%
17	17.098	2377	2382	2387	rBV	1501331	2238912	28.06%	3.821%
18	17.139	2387	2389	2397	rVB	168279	230603	2.89%	0.394%
19	18.016	2534	2538	2546	rBV	955399	1377998	17.27%	2.352%
20	18.286	2580	2584	2589	rBV2	298726	425137	5.33%	0.726%
21	18.486	2614	2618	2626	rVB	795065	1112110	13.94%	1.898%
22	18.892	2683	2687	2696	rVB	529154	775443	9.72%	1.324%
23	19.128	2723	2727	2730	rBV	310763	469788	5.89%	0.802%
24	19.257	2746	2749	2759	rBV3	472600	933966	11.71%	1.594%
25	19.475	2783	2786	2790	rVB	237321	261794	3.28%	0.447%
26	19.639	2811	2814	2817	rBV3	163510	213973	2.68%	0.365%
27	19.686	2817	2822	2832	rVB	6531400	7977819	100.00%	13.617%
28	19.886	2853	2856	2862	rVB	583484	702137	8.80%	1.198%
29	20.686	2989	2992	2997	rVB3	626096	718362	9.00%	1.226%
30	20.939	3031	3035	3043	rVV	1287808	1806027	22.64%	3.083%
31	21.016	3045	3048	3054	rVB2	537442	703752	8.82%	1.201%
32	21.210	3077	3081	3084	rBV	1829507	2383050	29.87%	4.067%
33	21.610	3145	3149	3155	rVB	1155210	1446285	18.13%	2.469%
34	21.680	3157	3161	3169	rVB	989725	1262285	15.82%	2.155%
35	22.269	3257	3261	3265	rBV2	672201	904285	11.33%	1.543%
36	22.733	3336	3340	3345	rVB	861777	1299893	16.29%	2.219%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006838.D
Acq On : 23 Aug 2021 19:12
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.533	3471	3476	3482	rVB	1300824	2375291	29.77%	4.054%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 58588216

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006838.D
Acq On : 23 Aug 2021 19:12
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

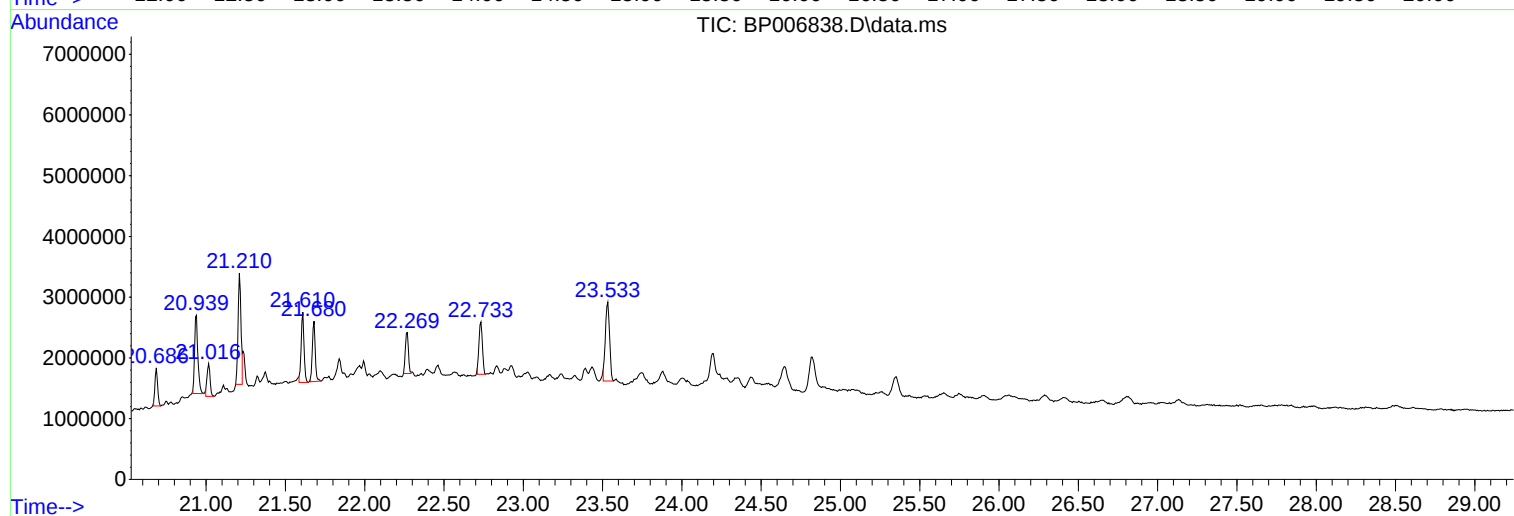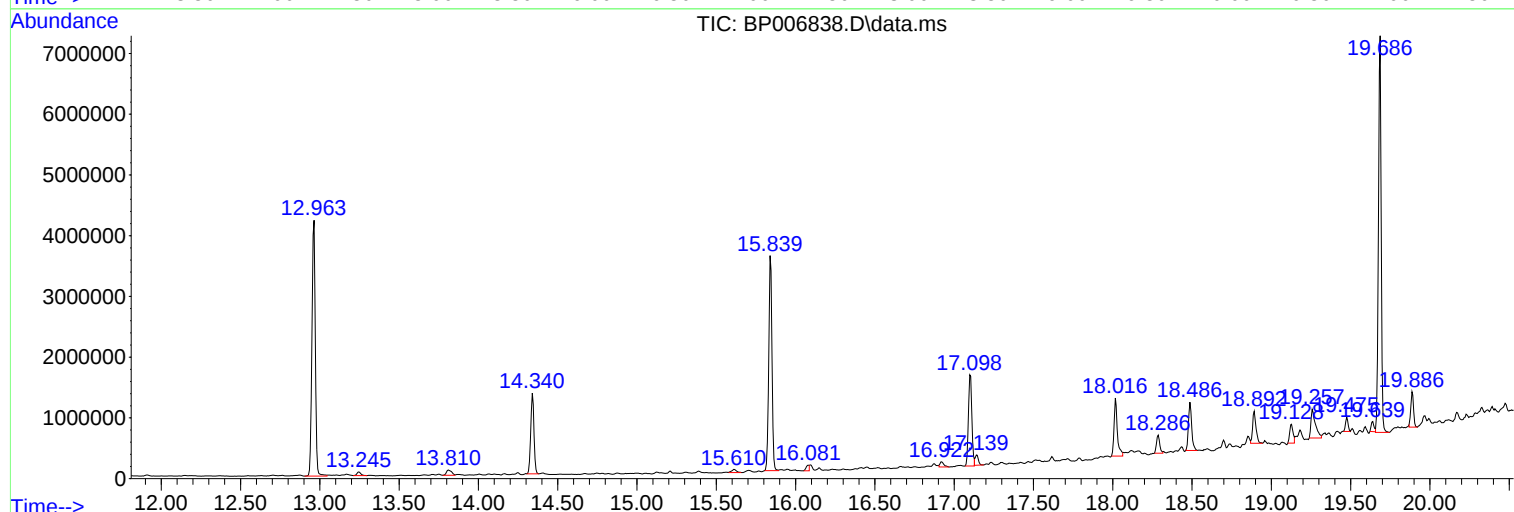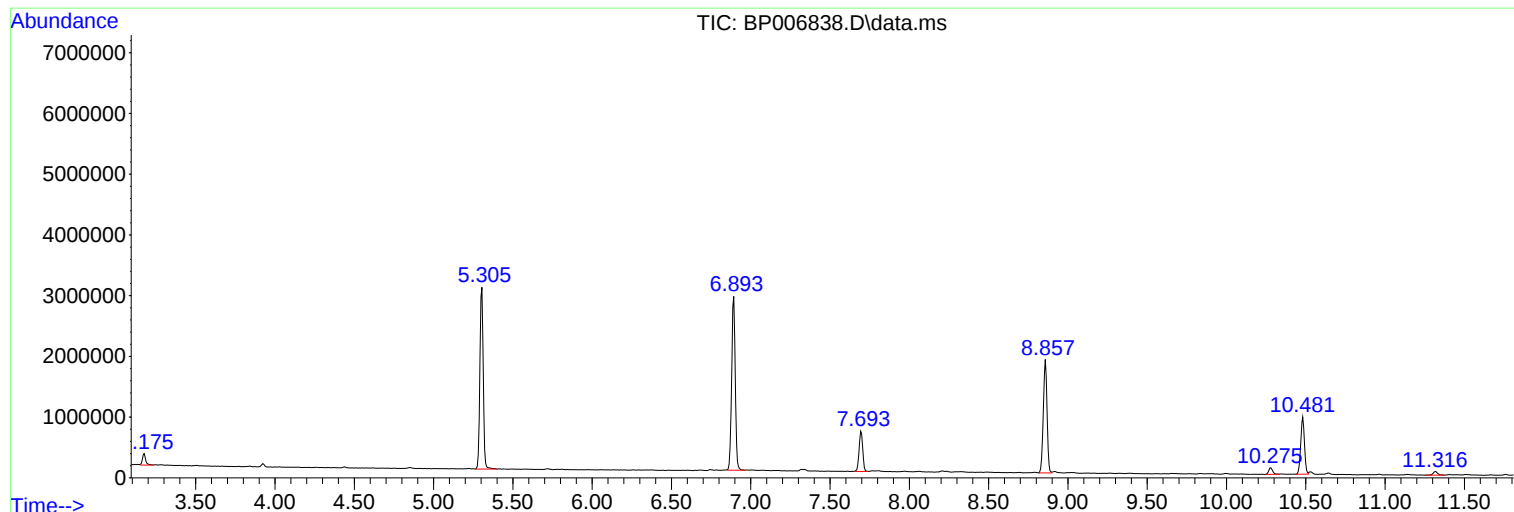

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006838.D
Acq On : 23 Aug 2021 19:12
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006838.D
Acq On : 23 Aug 2021 19:12
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------