
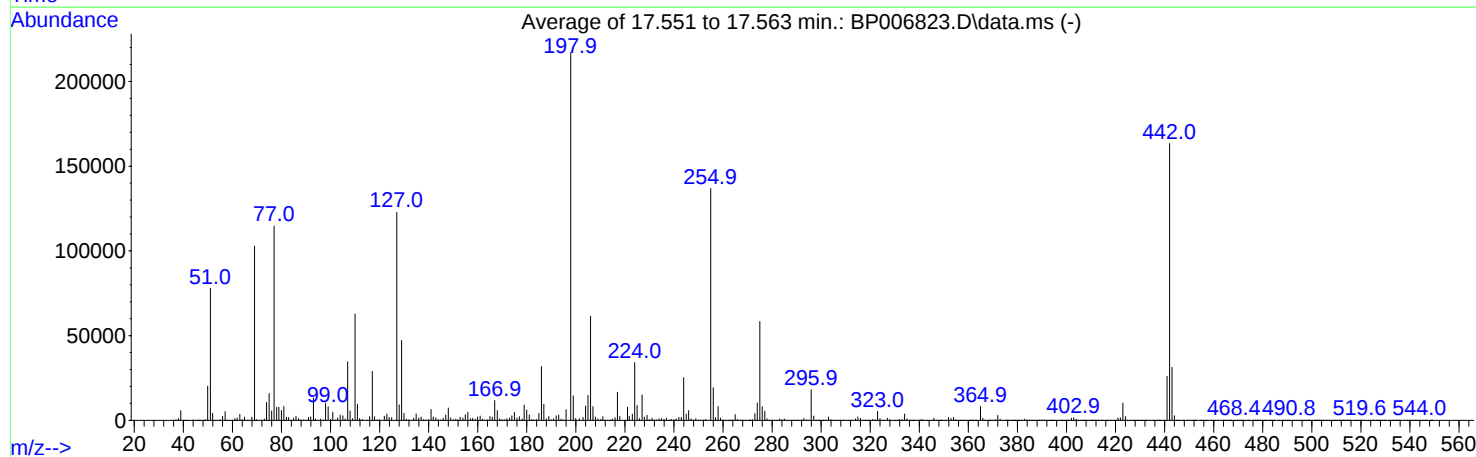


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
 Data File : BP006823.D
 Acq On : 23 Aug 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 23 11:39:38 2021

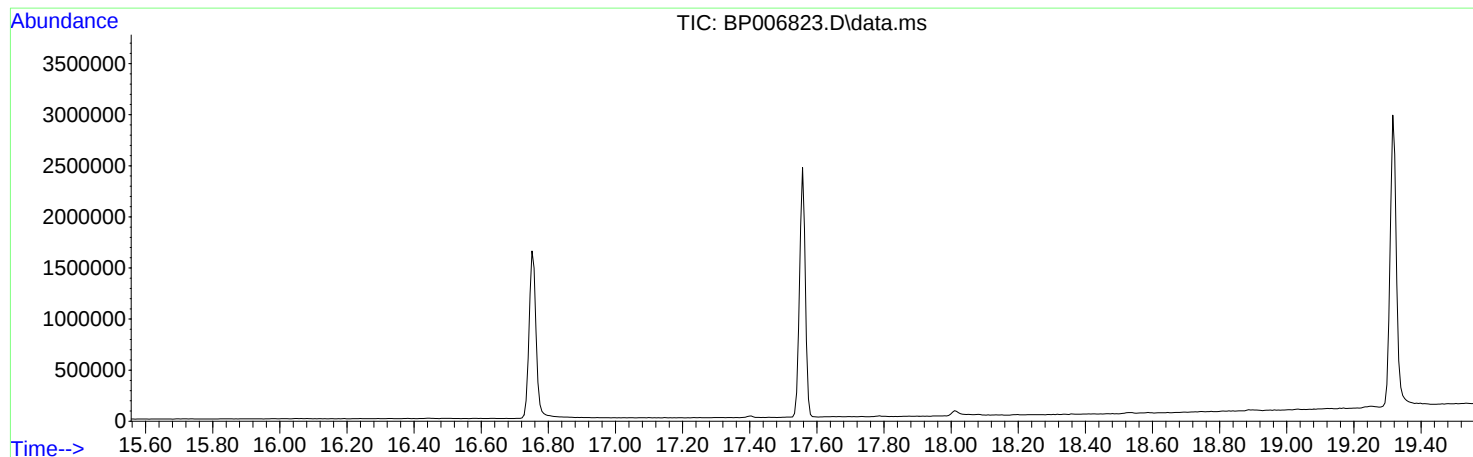




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	77876	PASS
68	69	0.00	2	1.9	1938	PASS
69	198	0.00	100	47.4	102848	PASS
70	69	0.00	2	0.4	442	PASS
127	198	10	80	56.6	122793	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	217099	PASS
199	198	5	9	6.7	14489	PASS
275	198	10	60	26.9	58368	PASS
365	198	1	100	3.8	8211	PASS
441	198	0.01	100	12.0	25960	PASS
442	442	100	100	100.0	163389	PASS
443	442	15	24	19.1	31280	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006823.D
Acq On : 23 Aug 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 23 11:48:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 11:39:38 2021
Response via : Initial Calibration

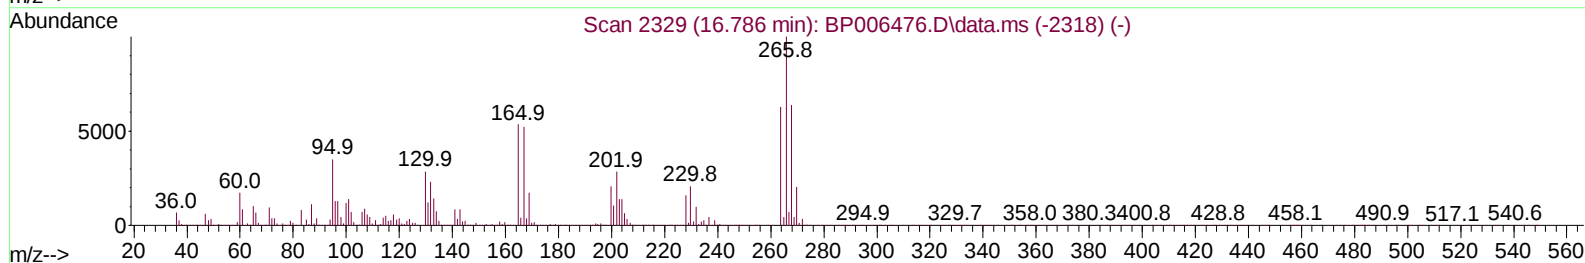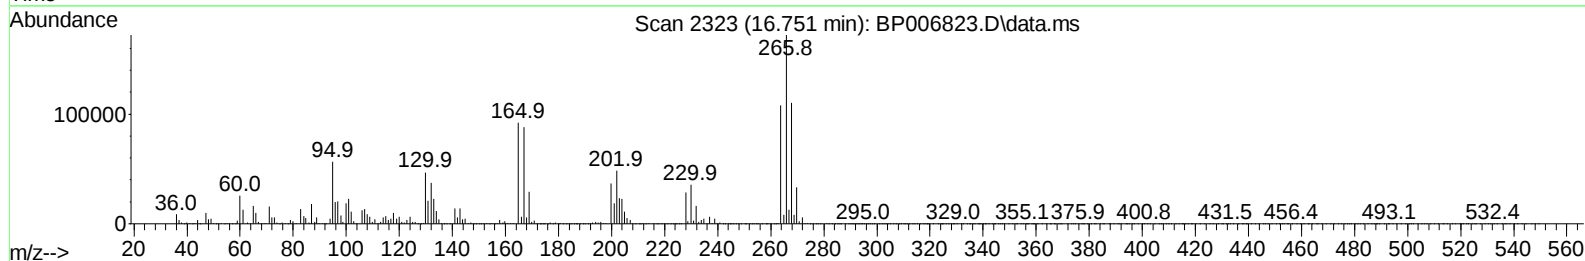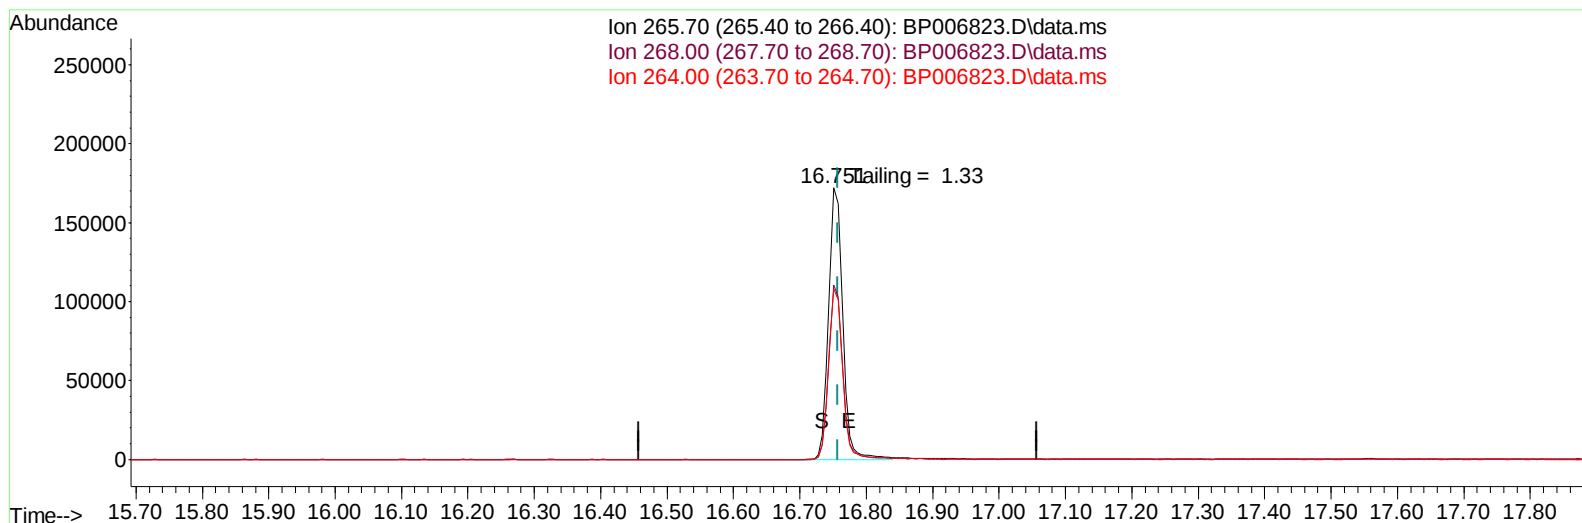

TIC: BP006823.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.006) 97490.87 ng




response 253948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.22
264.00	62.90	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082321\
Data File : BP006823.D
Acq On : 23 Aug 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 23 11:48:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 11:39:38 2021
Response via : Initial Calibration

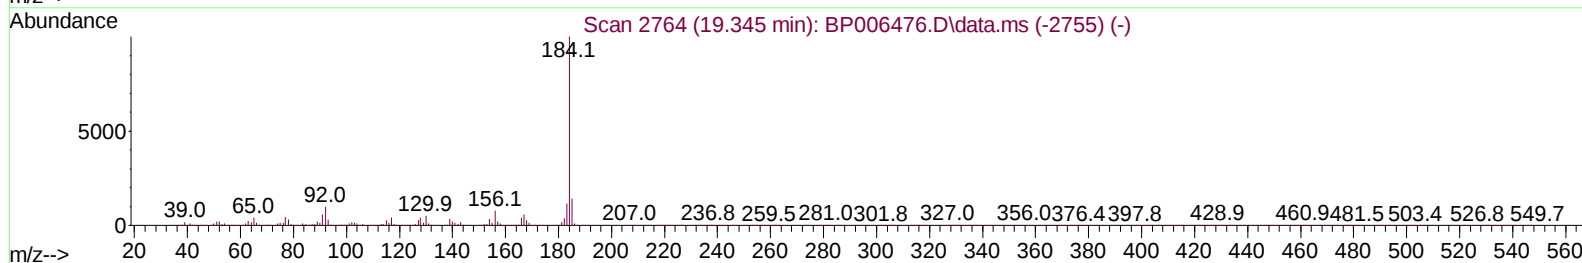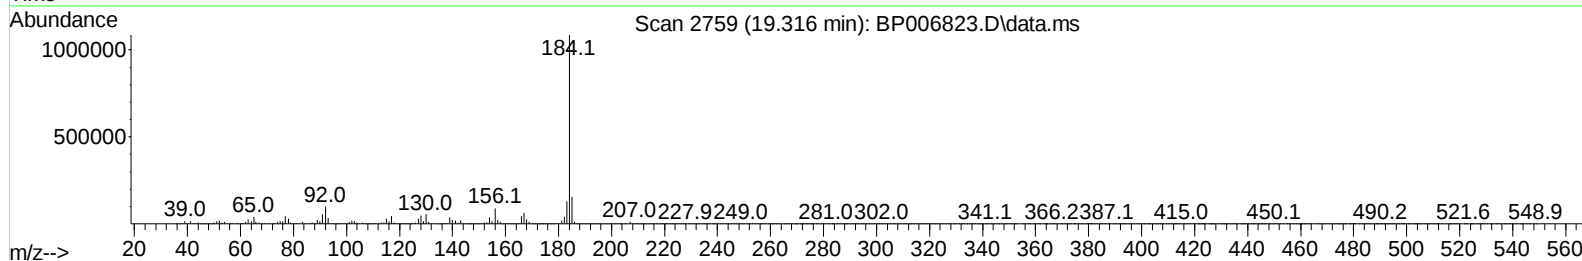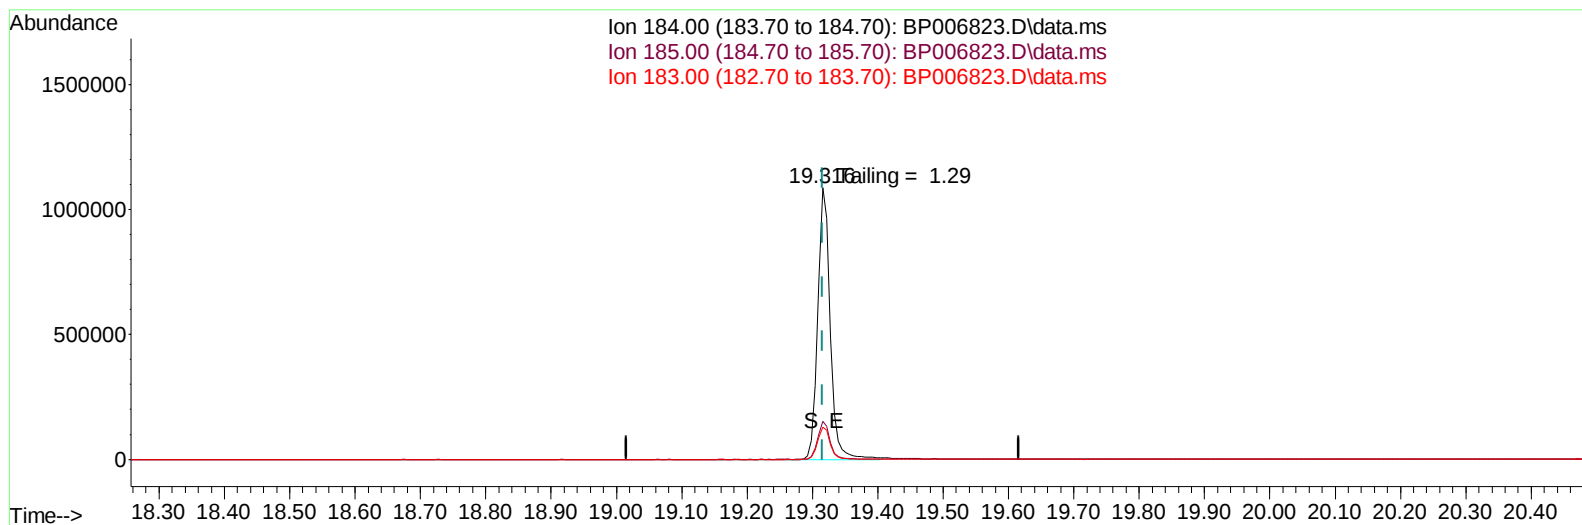

TIC: BP006823.D\data.ms

(77) Benzidine

19.316min (+ 0.000) 25598.00 ng

response 1456604

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.17
183.00	11.90	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2021	BNA_P	<u>BP006823.D</u>
Compound Name	Response	Retention Time
DDT	721644	20.522
DDD	23156	20.09
DDE	3499	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26655	748299	3.56

Instrument :
BNA_P
ClientSampleId :
DFTPP