
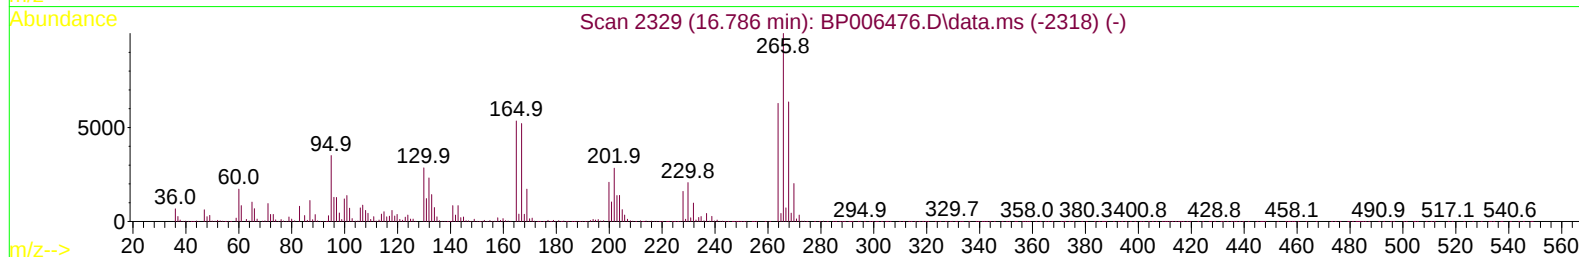
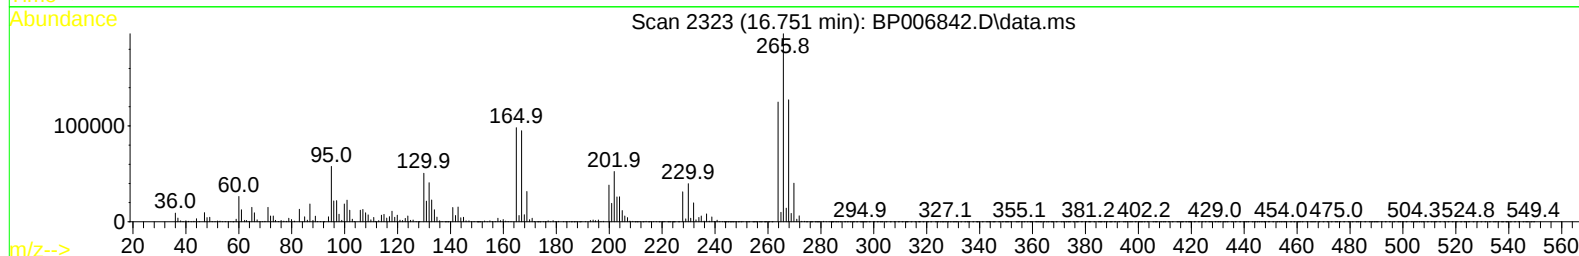


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006842.D
 Acq On : 24 Aug 2021 10:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 13:36:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 11:39:38 2021
 Response via : Initial Calibration

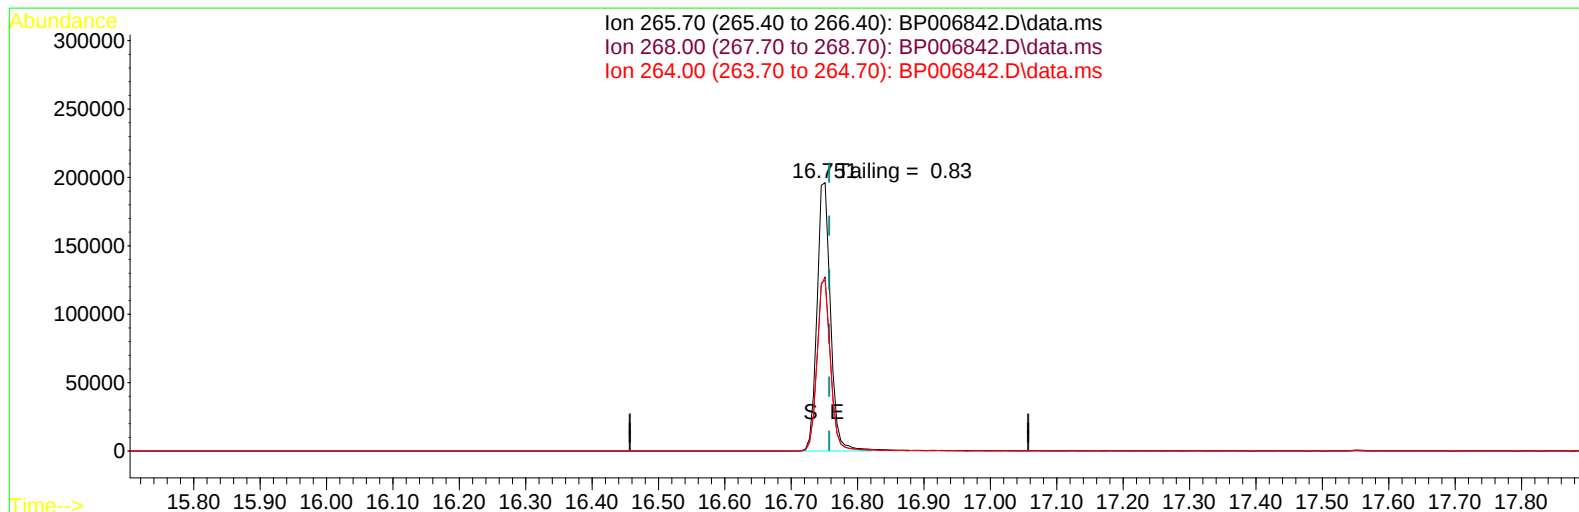

TIC: BP006842.D\data.ms

(70) Pentachlorophenol (C)




16.751min (-0.006) 3685146.18 ng

response 280828

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.86
264.00	62.90	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006842.D
 Acq On : 24 Aug 2021 10:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 13:36:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 11:39:38 2021
 Response via : Initial Calibration

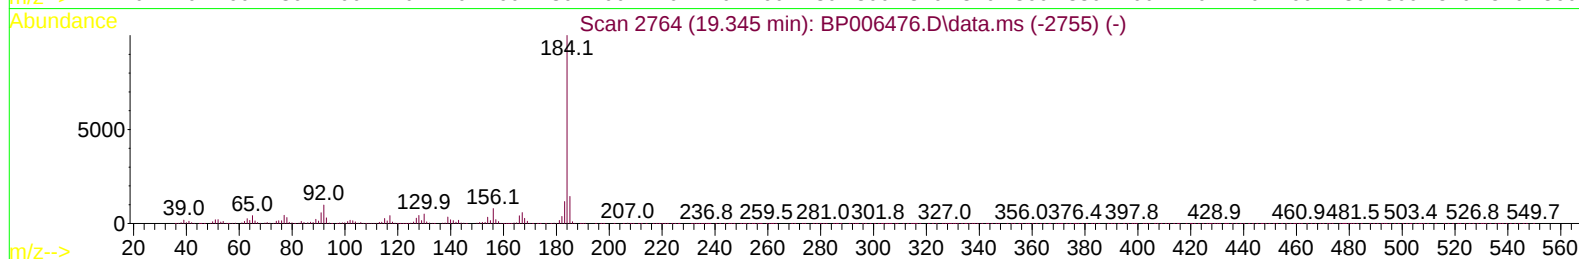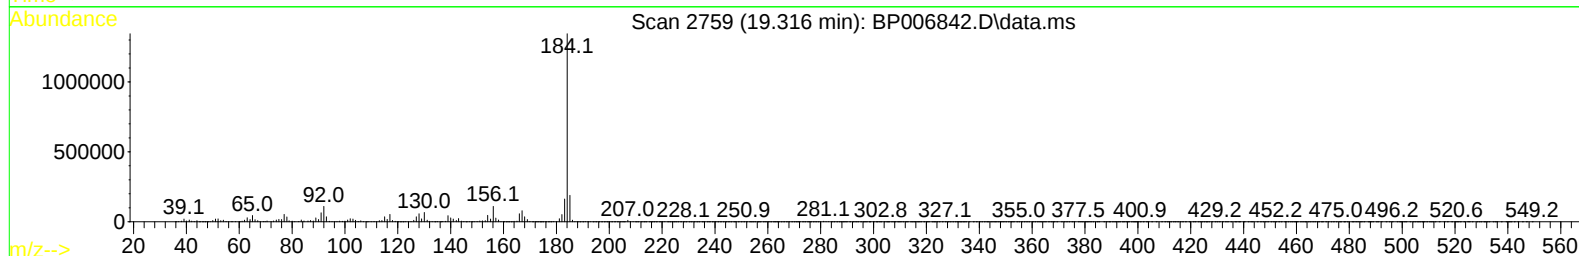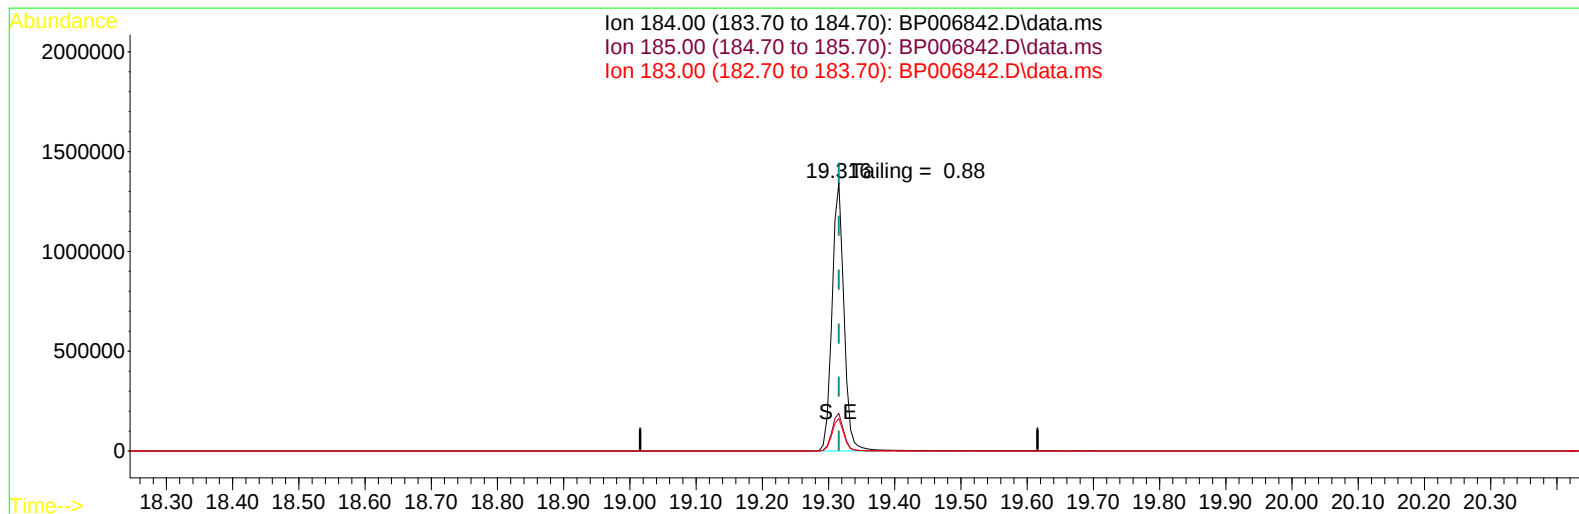

TIC: BP006842.D\data.ms

(77) Benzidine**19.316min (-0.000) 420550.98 ng****response 1694297**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.05
183.00	11.90	12.10
0.00	0.00	0.00