
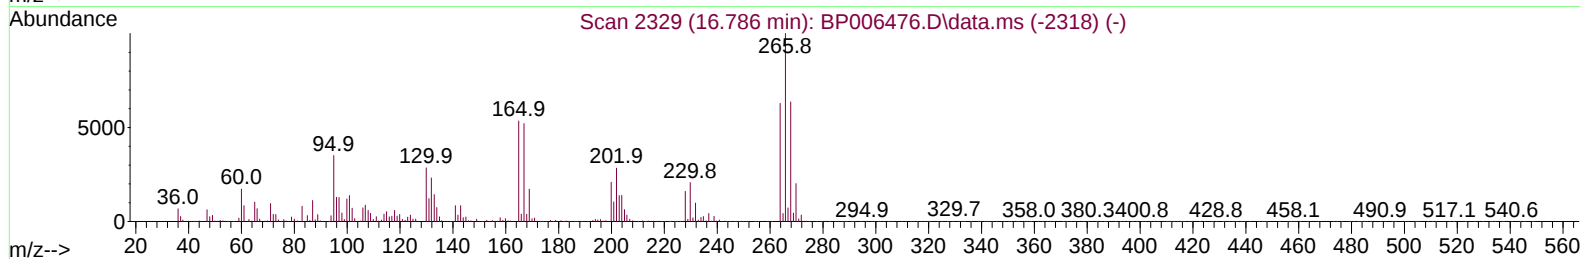
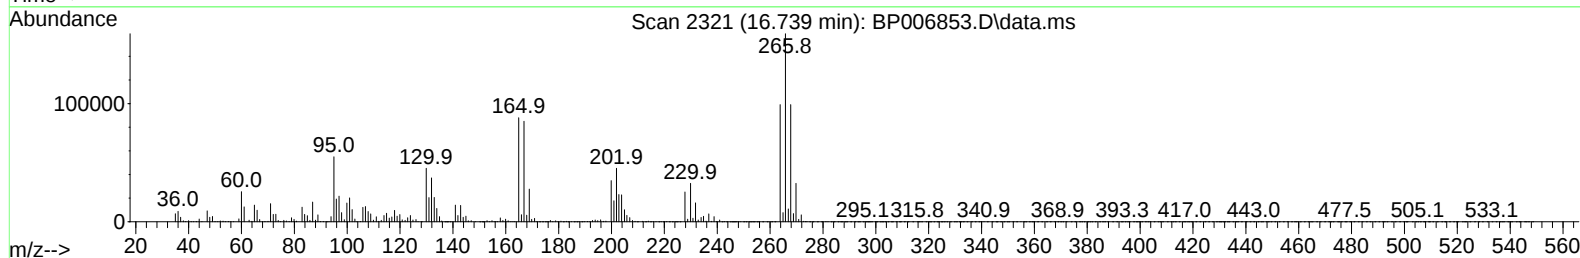


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006853.D
Acq On : 24 Aug 2021 18:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 05:40:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 13:40:38 2021
Response via : Initial Calibration

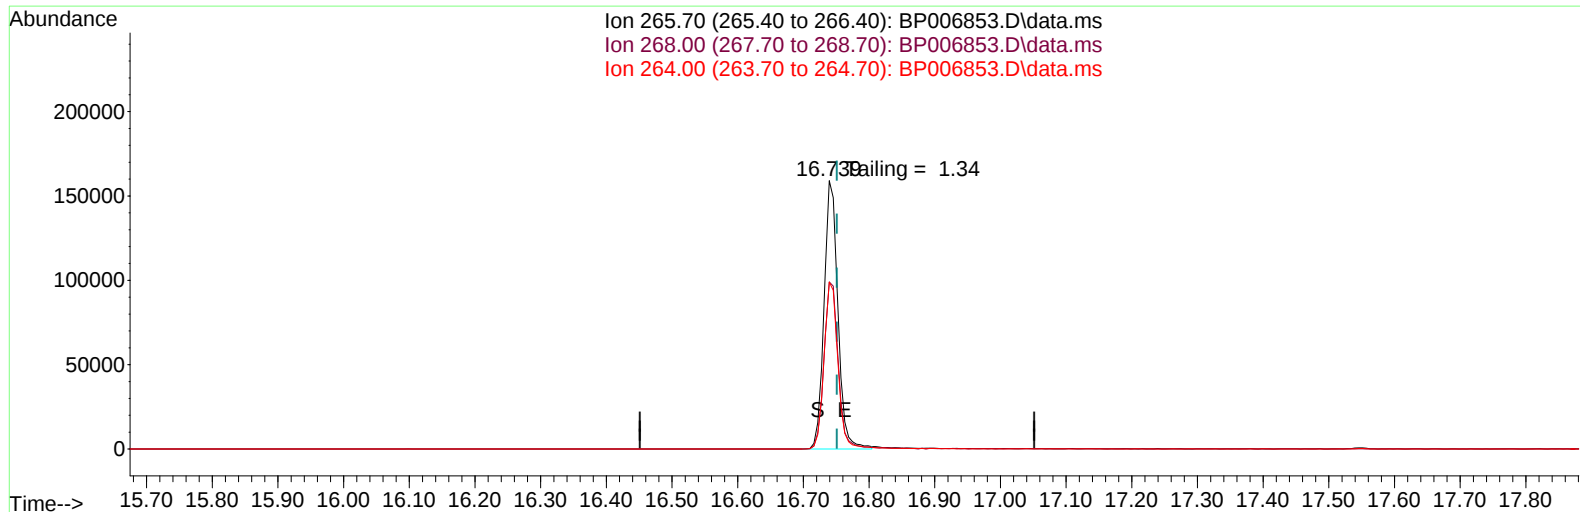

TIC: BP006853.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.012) 1172618.21 ng

response 235585

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.28
264.00	62.90	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006853.D
Acq On : 24 Aug 2021 18:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 05:40:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 13:40:38 2021
Response via : Initial Calibration

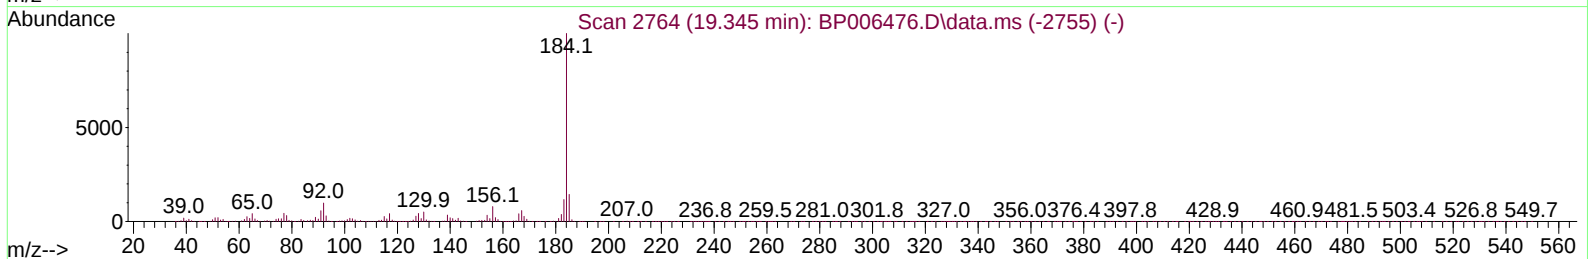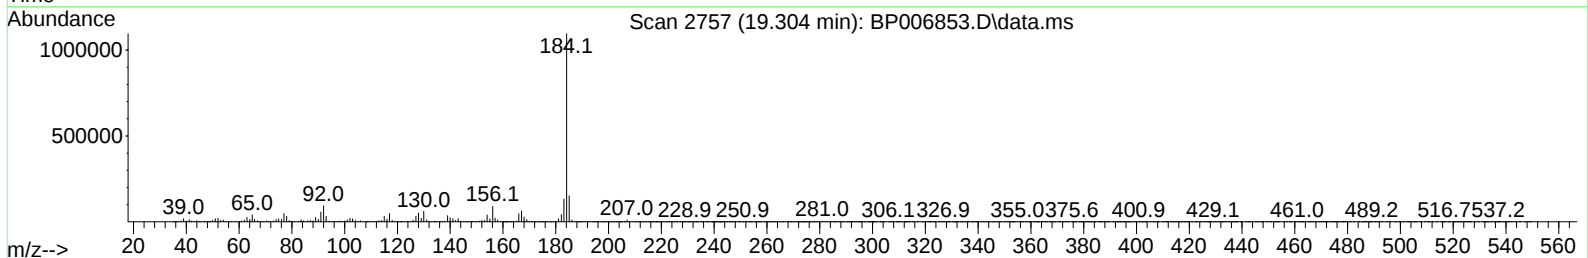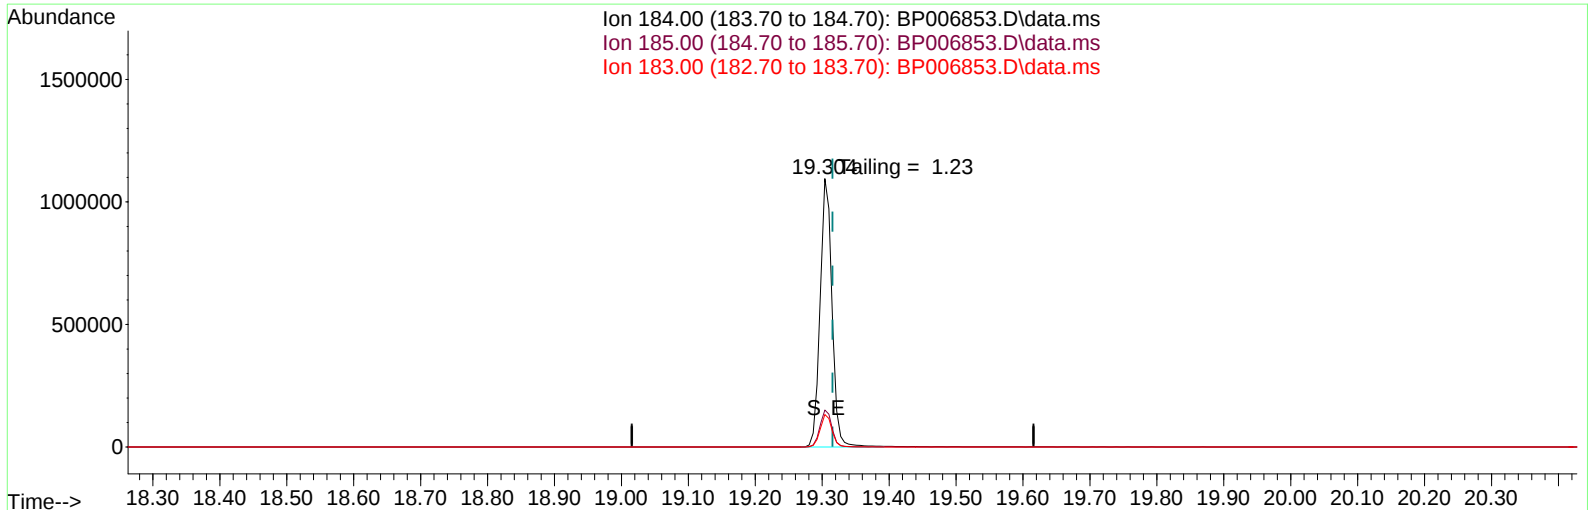

TIC: BP006853.D\data.ms

(77) Benzidine**19.304min (-0.012) 433477.16 ng****response 1355880**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.81
183.00	11.90	12.13
0.00	0.00	0.00